


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061716\
 Data File : BF088090.D
 Acq On : 17 Jun 2016 11:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 17 16:09:13 2016

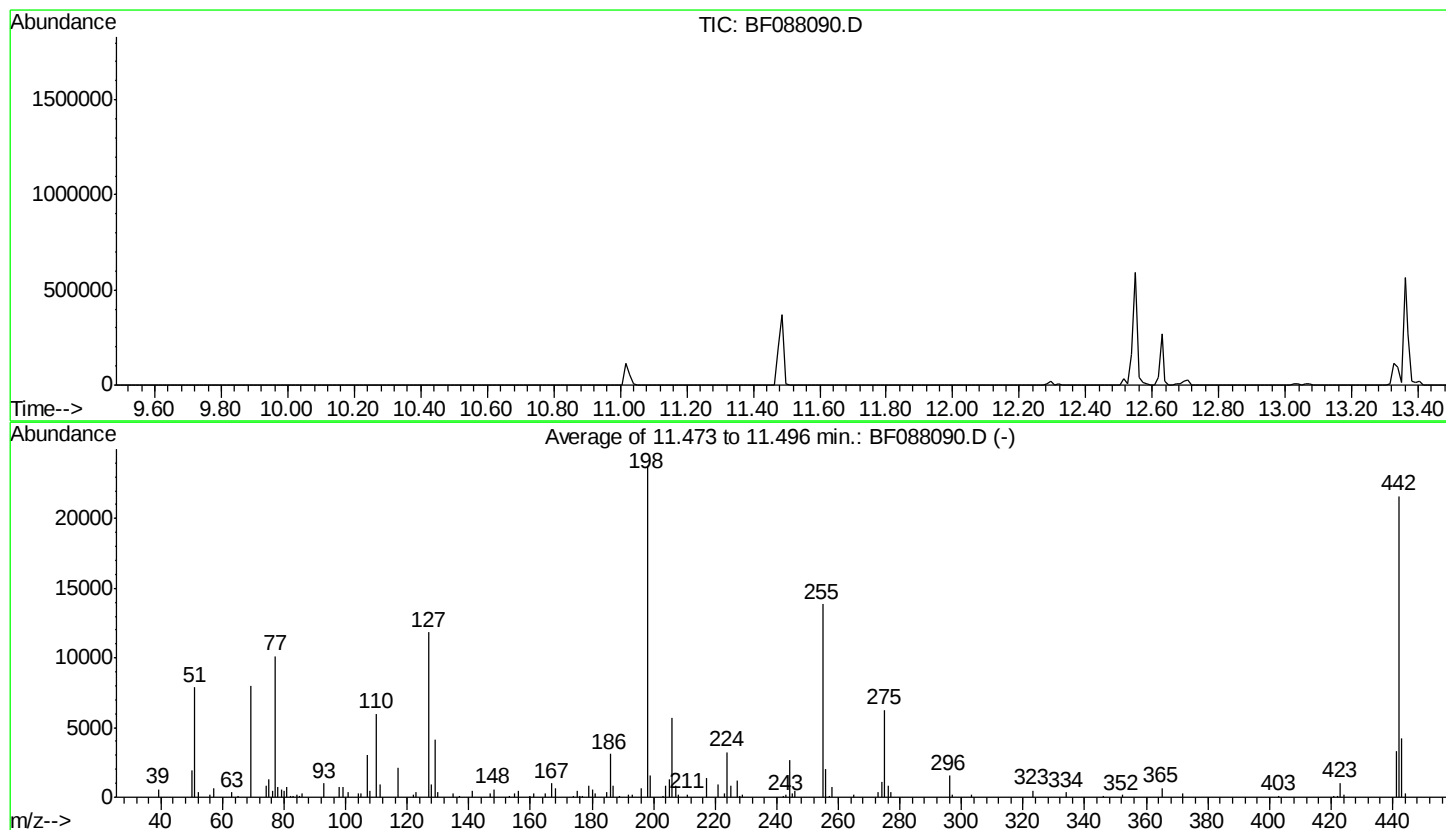

AutoFind: Scans 865, 866, 867; Background Corrected with Scan 862

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	7897	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	8042	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	11834	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23803	PASS
199	198	5	9	6.7	1596	PASS
275	198	10	60	26.4	6279	PASS
365	198	1	100	2.9	686	PASS
441	442	0.01	24	15.2	3287	PASS
442	198	50	100	90.8	21620	PASS
443	442	15	24	19.4	4193	PASS