
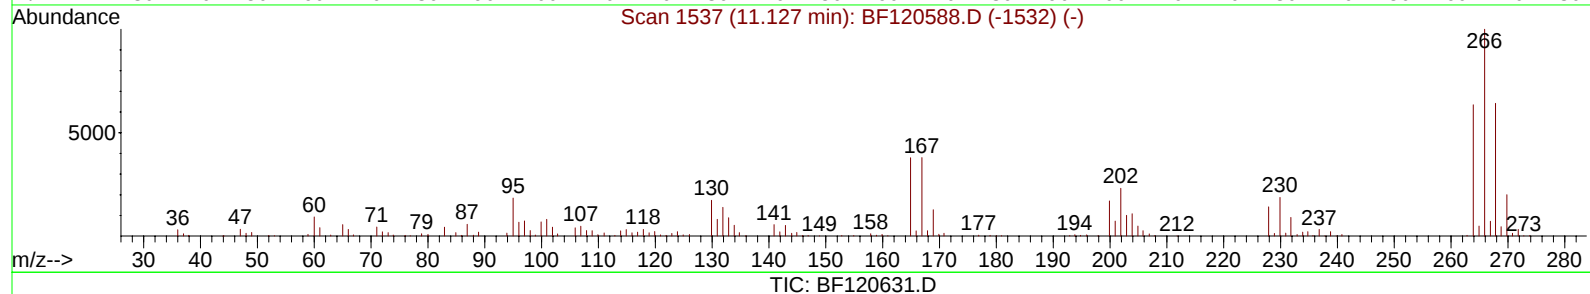
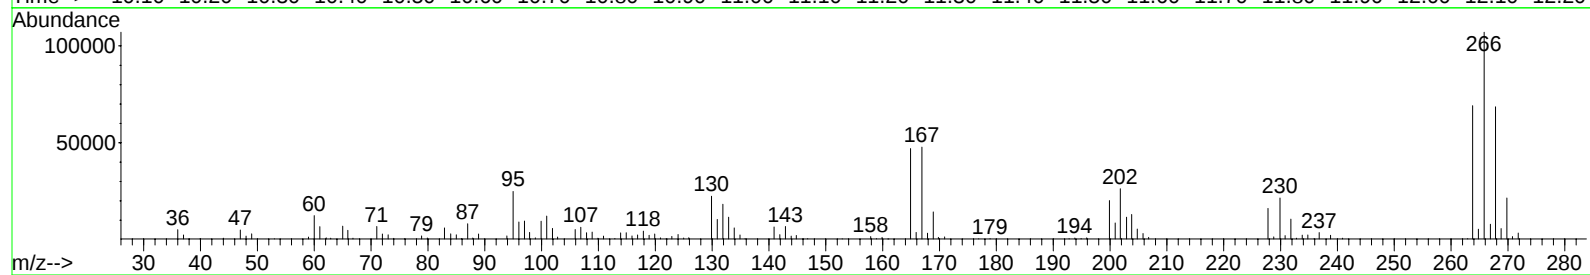


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061720\
Data File : BF120631.D
Acq On : 17 Jun 2020 14:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 18:23:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 11:28:22 2020
Response via : Initial Calibration

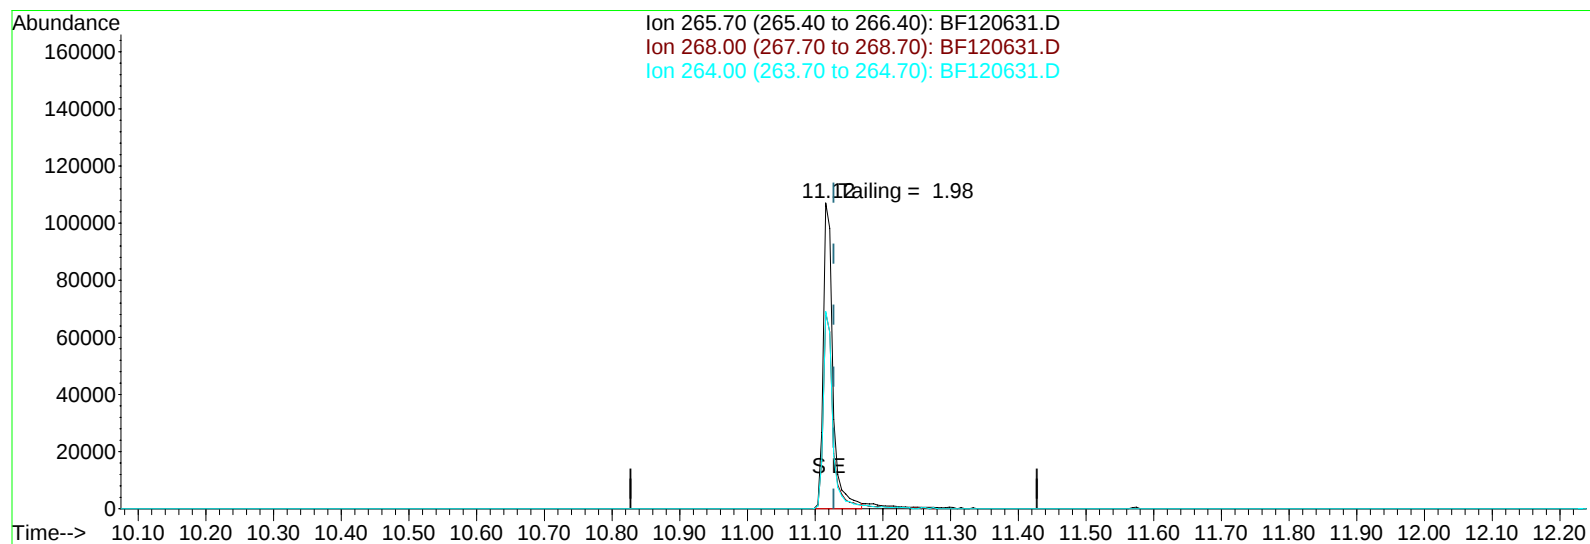

(70) Pentachlorophenol (C)




11.116min (-0.012) 18953.45ng

response 110192

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	64.08
264.00	63.50	64.55
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061720\
 Data File : BF120631.D
 Acq On : 17 Jun 2020 14:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 18:23:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

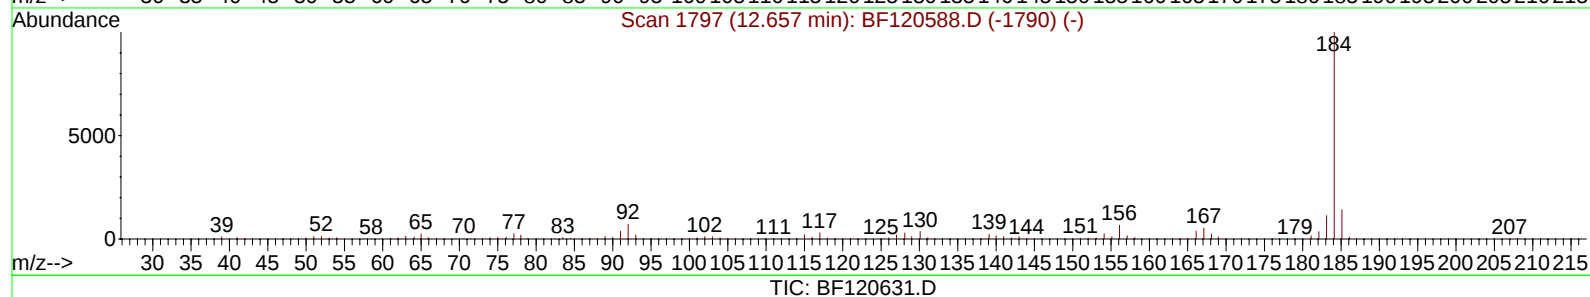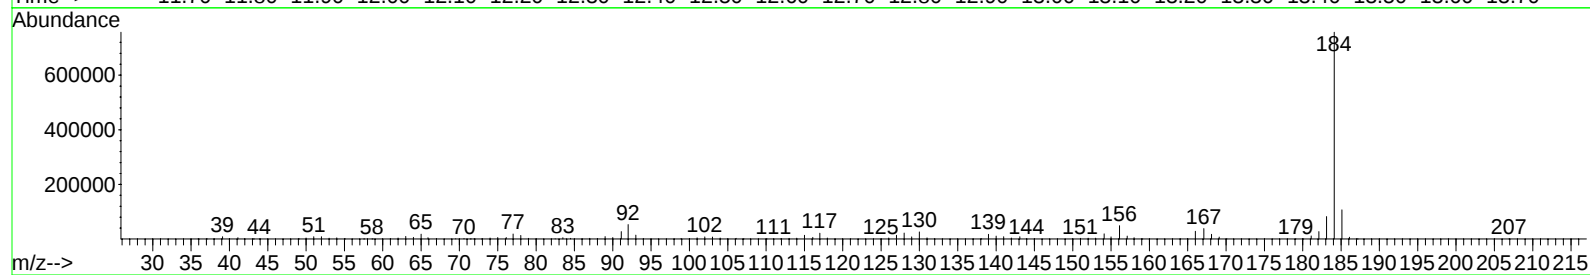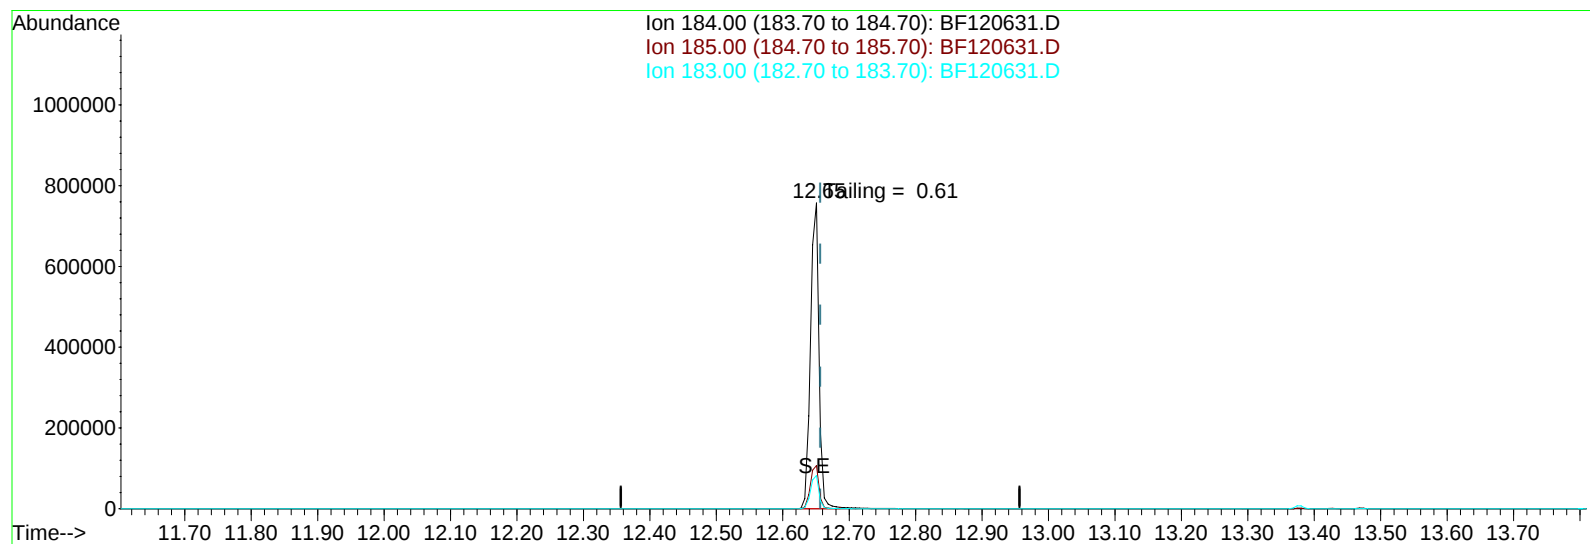

(77) Benzidine

12.651min (-0.006) 29905.41ng

response 680660

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.13
183.00	11.30	10.89
0.00	0.00	0.00