


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061720\
 Data File : BF120631.D
 Acq On : 17 Jun 2020 14:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 11:28:22 2020

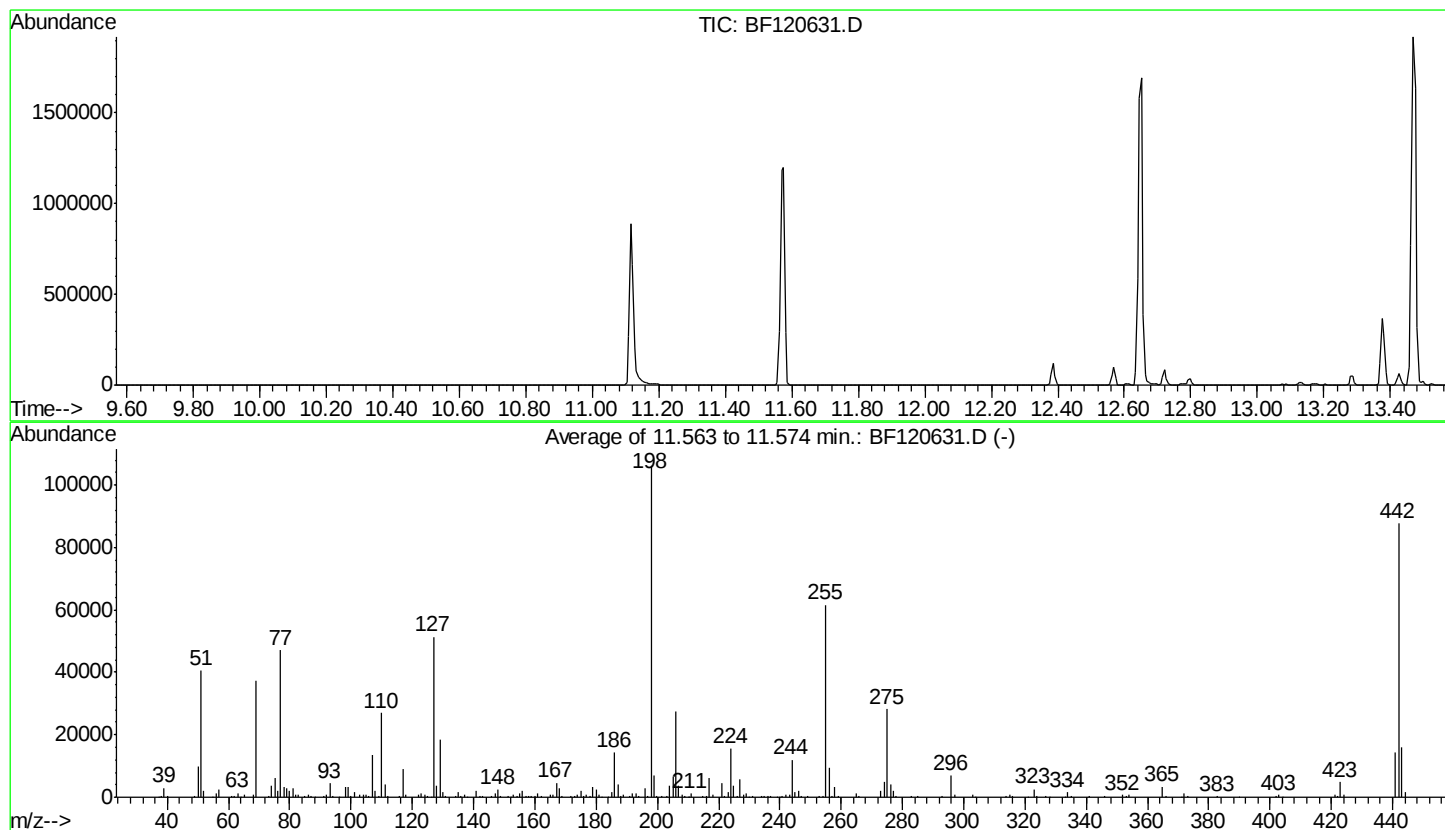

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	40509	PASS
68	69	0.00	2	1.7	642	PASS
69	198	0.00	100	35.1	37322	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	51298	PASS
197	198	0.00	2	0.6	587	PASS
198	198	100	100	100.0	106189	PASS
199	198	5	9	6.6	6983	PASS
275	198	10	60	26.6	28206	PASS
365	198	1	100	3.2	3444	PASS
441	198	0.01	100	13.6	14461	PASS
442	198	50	100	82.5	87637	PASS
443	442	15	24	18.5	16190	PASS