
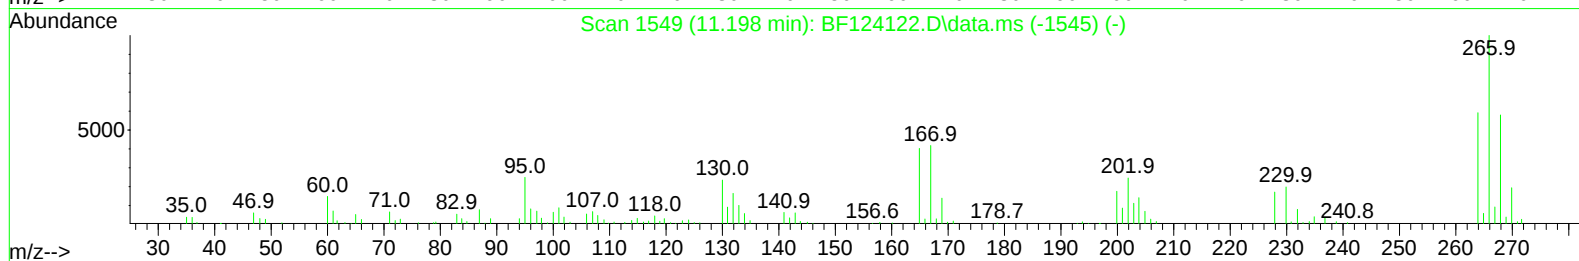
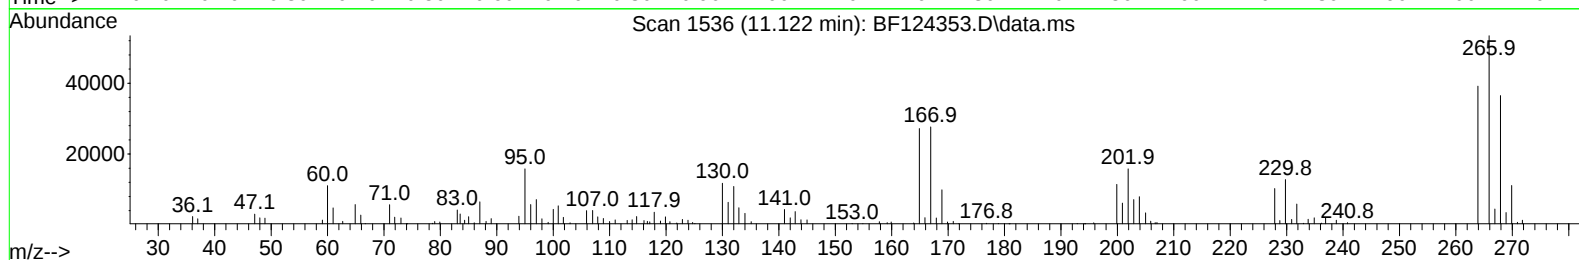


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124353.D
Acq On : 17 Jun 2021 9:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 11:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

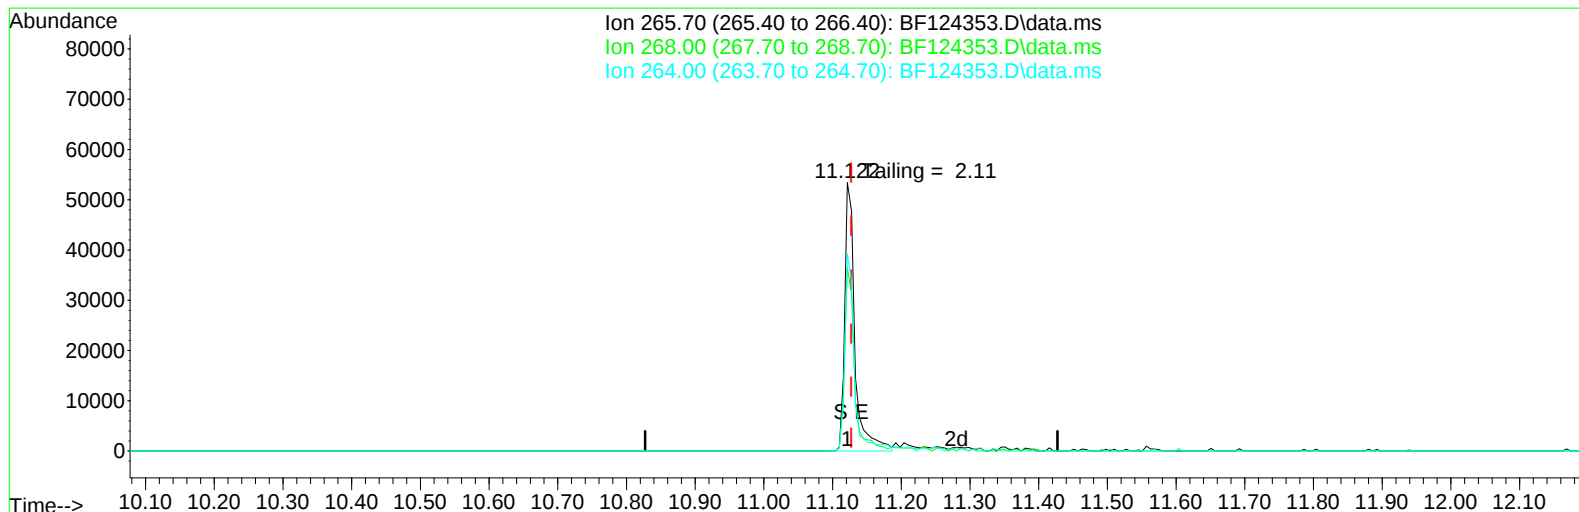

TIC: BF124353.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.006) 20768.59 ng

response 54914

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	68.32
264.00	65.70	73.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124353.D
Acq On : 17 Jun 2021 9:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 11:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

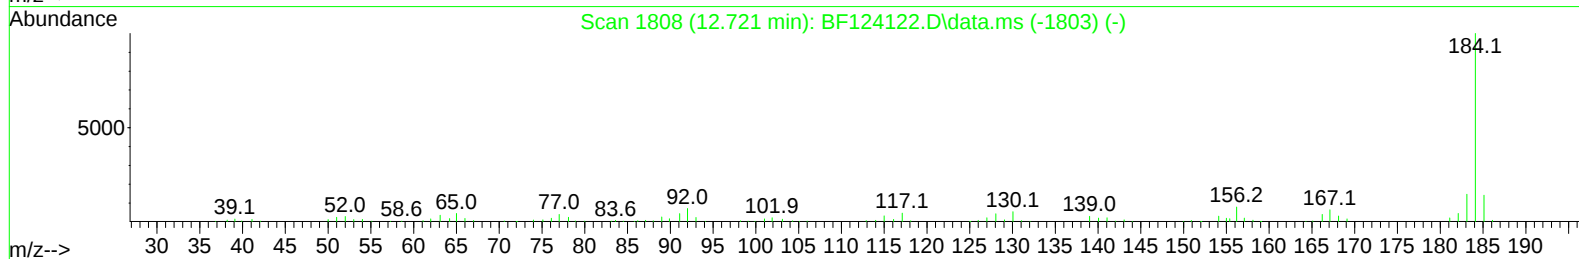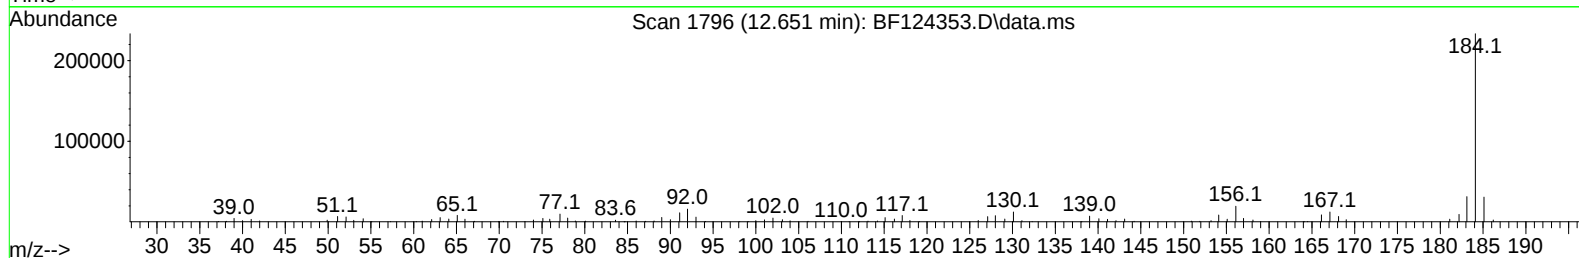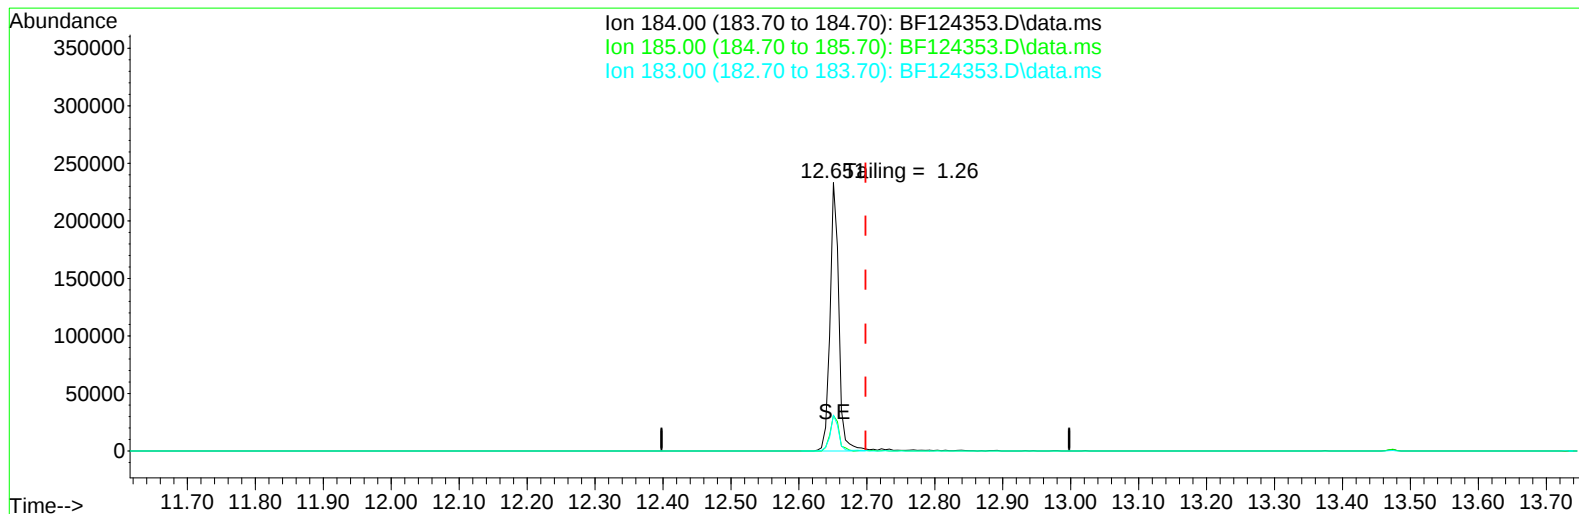

TIC: BF124353.D\data.ms

(77) Benzidine

12.651min (-0.047) 0.00 ng

response 212339

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.24
183.00	9.80	13.46#
0.00	0.00	0.00