

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
 Data File : BF124355.D
 Acq On : 17 Jun 2021 10:14
 Operator : JU/CG
 Sample : PB137159BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137159BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	497	500	505	rBV2	16307	23327	1.27%	0.222%
2	5.422	562	567	580	rBV	1433142	1423827	77.71%	13.559%
3	6.434	735	739	742	rBV	1374205	1343738	73.34%	12.796%
4	6.781	795	798	802	rBV	323552	270669	14.77%	2.578%
5	7.351	890	895	898	rBV	950965	941763	51.40%	8.968%
6	8.069	1013	1017	1020	rBV	387209	340212	18.57%	3.240%
7	9.145	1195	1200	1203	rBV	2066705	1832164	100.00%	17.447%
8	9.822	1311	1315	1319	rBV	526681	407020	22.22%	3.876%
9	10.616	1446	1450	1453	rBV	1375748	1167763	63.74%	11.120%
10	11.310	1564	1568	1576	rBV	504634	420146	22.93%	4.001%
11	12.904	1833	1839	1842	rBV	1934835	1815445	99.09%	17.288%
12	13.957	2014	2018	2022	rVB	319551	279238	15.24%	2.659%
13	15.409	2261	2265	2275	rVB	185621	235827	12.87%	2.246%




Sum of corrected areas: 10501139

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124355.D
Acq On : 17 Jun 2021 10:14
Operator : JU/CG
Sample : PB137159BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137159BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

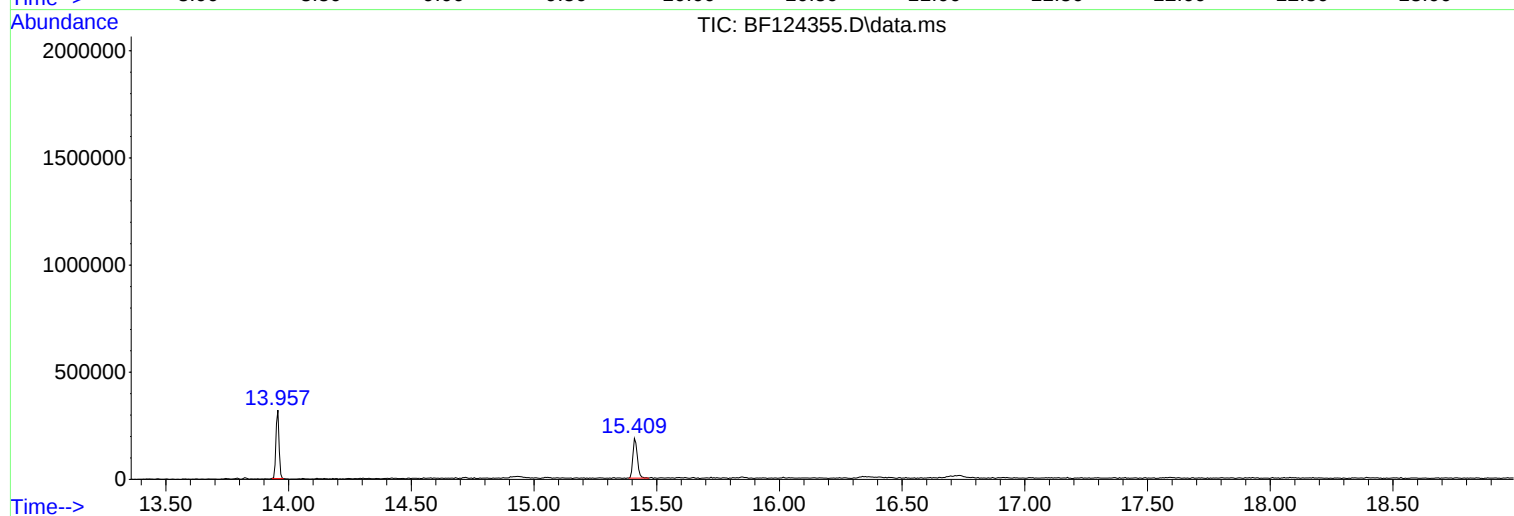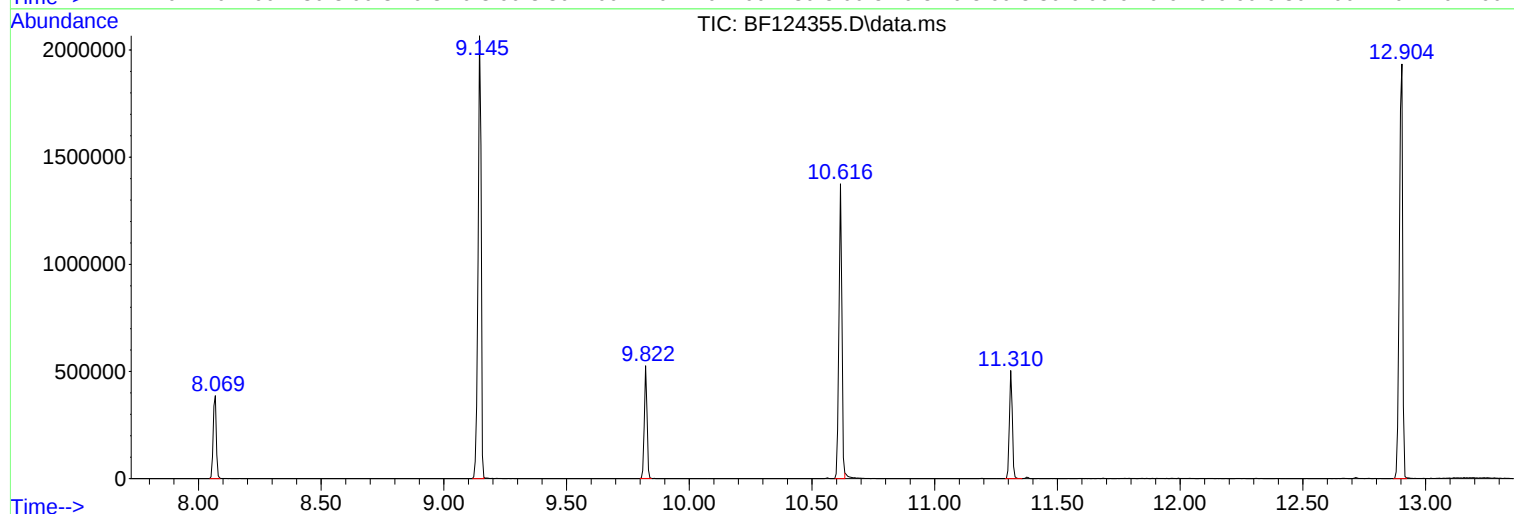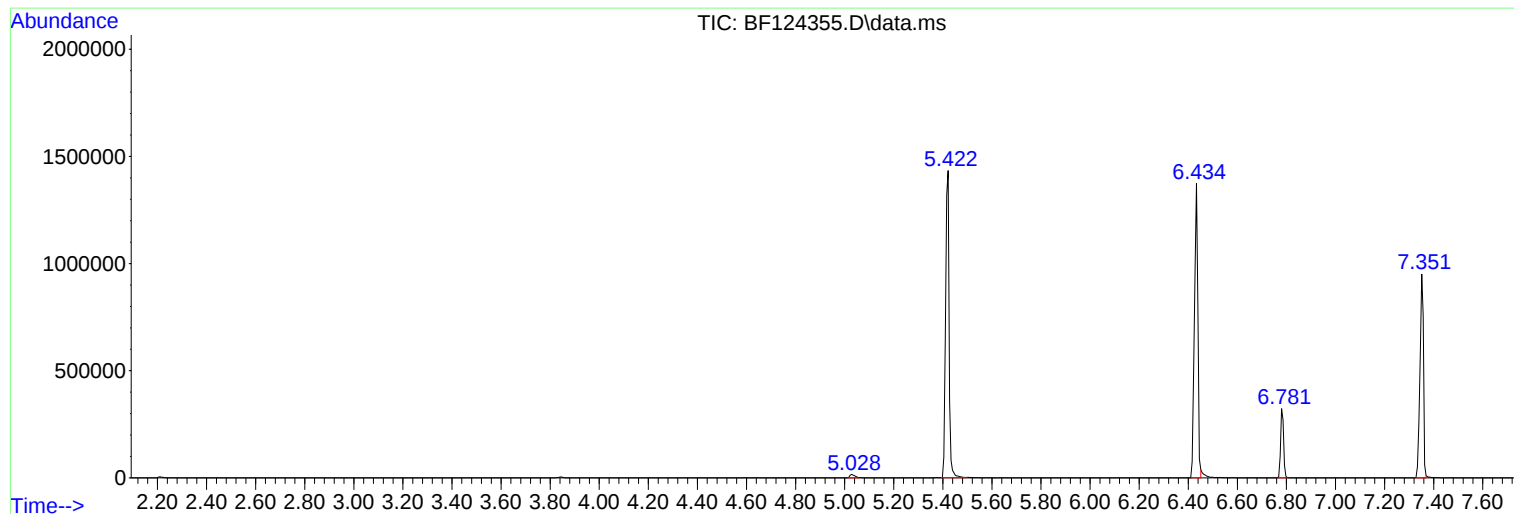

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124355.D
Acq On : 17 Jun 2021 10:14
Operator : JU/CG
Sample : PB137159BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137159BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124355.D
Acq On : 17 Jun 2021 10:14
Operator : JU/CG
Sample : PB137159BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137159BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------