

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
 Data File : BF124359.D
 Acq On : 17 Jun 2021 12:42
 Operator : JU/CG
 Sample : M2678-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SPLP-AMND-COMP-K(CL-16)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	490	493	497	rBV	19179	20122	1.11%	0.245%
2	5.404	561	564	577	rBV	513035	492797	27.11%	6.003%
3	6.428	735	738	750	rBV	263833	276456	15.21%	3.368%
4	6.781	795	798	804	rBB	304624	229090	12.60%	2.791%
5	6.851	807	810	815	rBV	20617	20237	1.11%	0.247%
6	7.351	890	895	898	rBV	949487	896828	49.34%	10.924%
7	8.069	1013	1017	1020	rBV	320163	278541	15.32%	3.393%
8	9.145	1196	1200	1203	rBV	2039698	1720271	94.64%	20.955%
9	9.822	1312	1315	1318	rBV	468137	341389	18.78%	4.159%
10	10.616	1446	1450	1453	rBV	1388050	1149563	63.25%	14.003%
11	11.310	1565	1568	1571	rBV	490805	374556	20.61%	4.563%
12	12.898	1834	1838	1841	rBV	1816600	1817618	100.00%	22.141%
13	13.957	2014	2018	2022	rVB	339025	305145	16.79%	3.717%
14	15.409	2260	2265	2271	rBV	203169	266769	14.68%	3.250%
15	15.851	2336	2340	2345	rVB4	13246	19964	1.10%	0.243%




Sum of corrected areas: 8209346

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124359.D
Acq On : 17 Jun 2021 12:42
Operator : JU/CG
Sample : M2678-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-AMND-COMP-K(CL-16)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

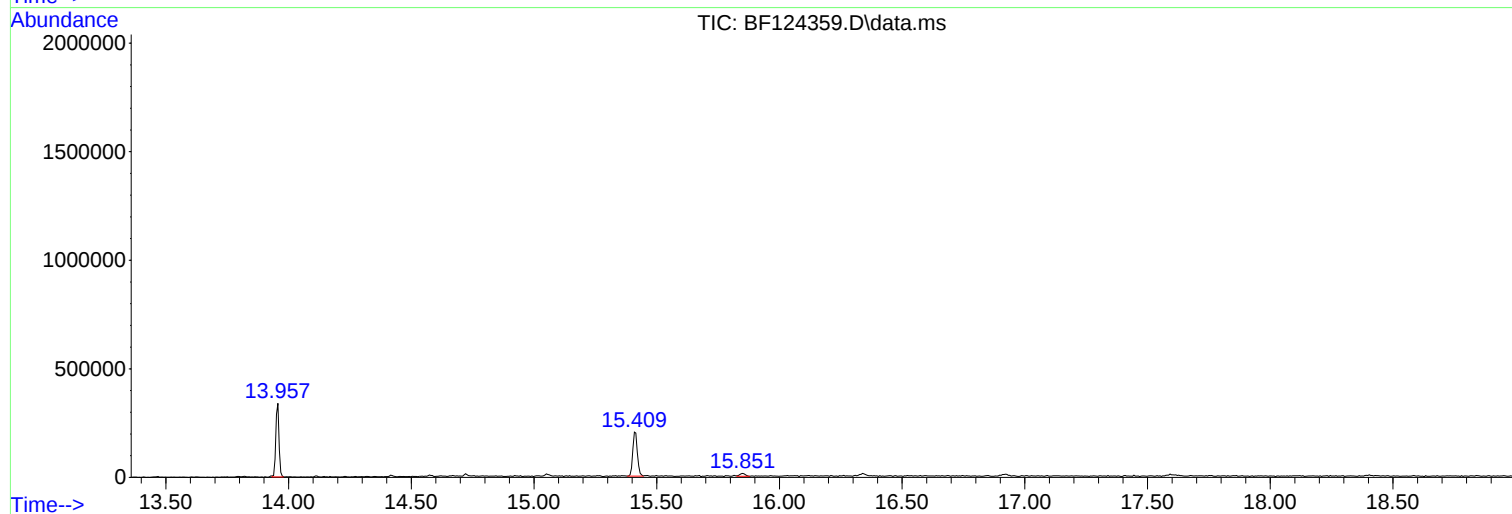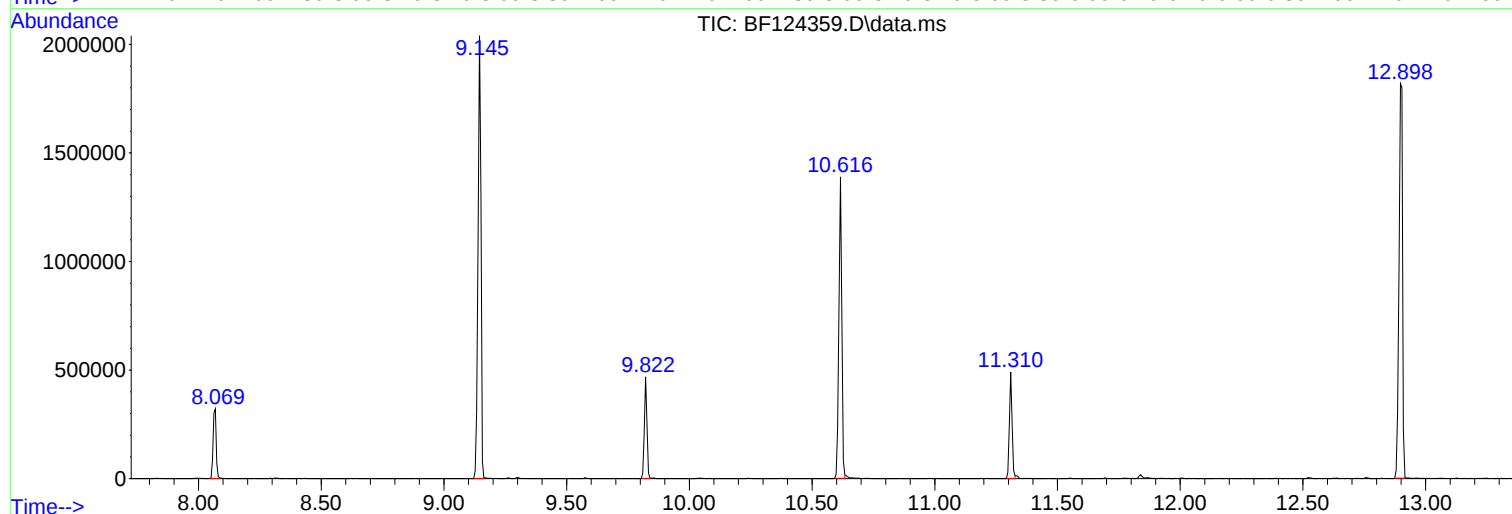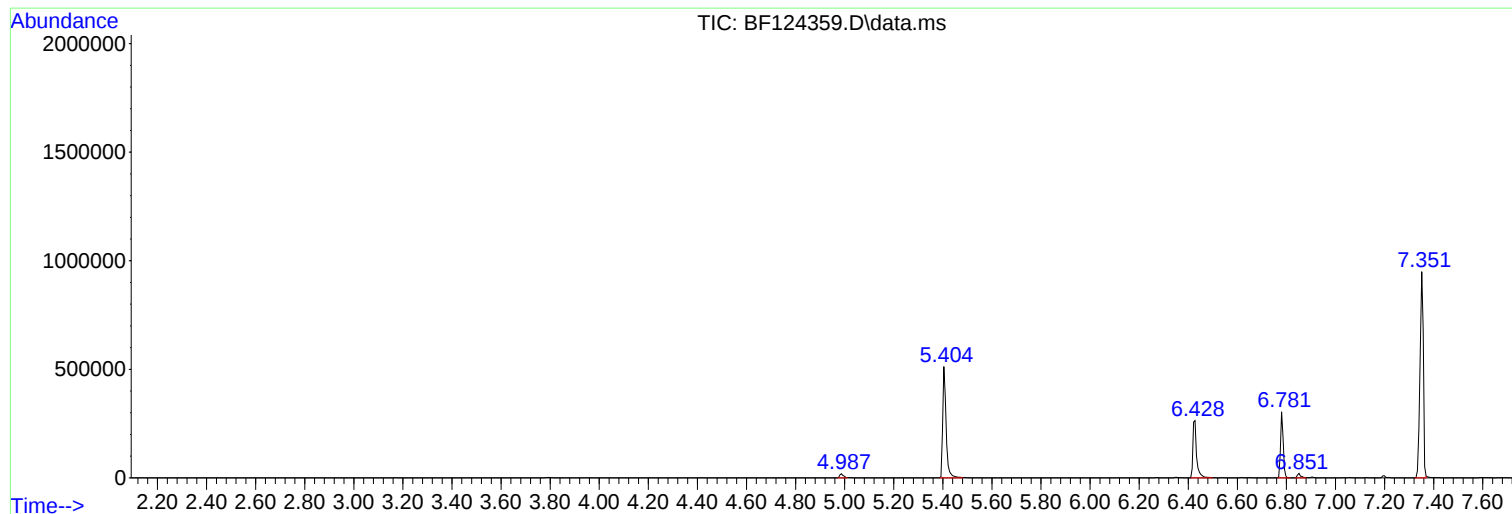

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124359.D
Acq On : 17 Jun 2021 12:42
Operator : JU/CG
Sample : M2678-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-AMND-COMP-K(CL-16)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124359.D
Acq On : 17 Jun 2021 12:42
Operator : JU/CG
Sample : M2678-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-AMND-COMP-K(CL-16)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------