


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
 Data File : BF124353.D
 Acq On : 17 Jun 2021 9:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 15 20:09:26 2021

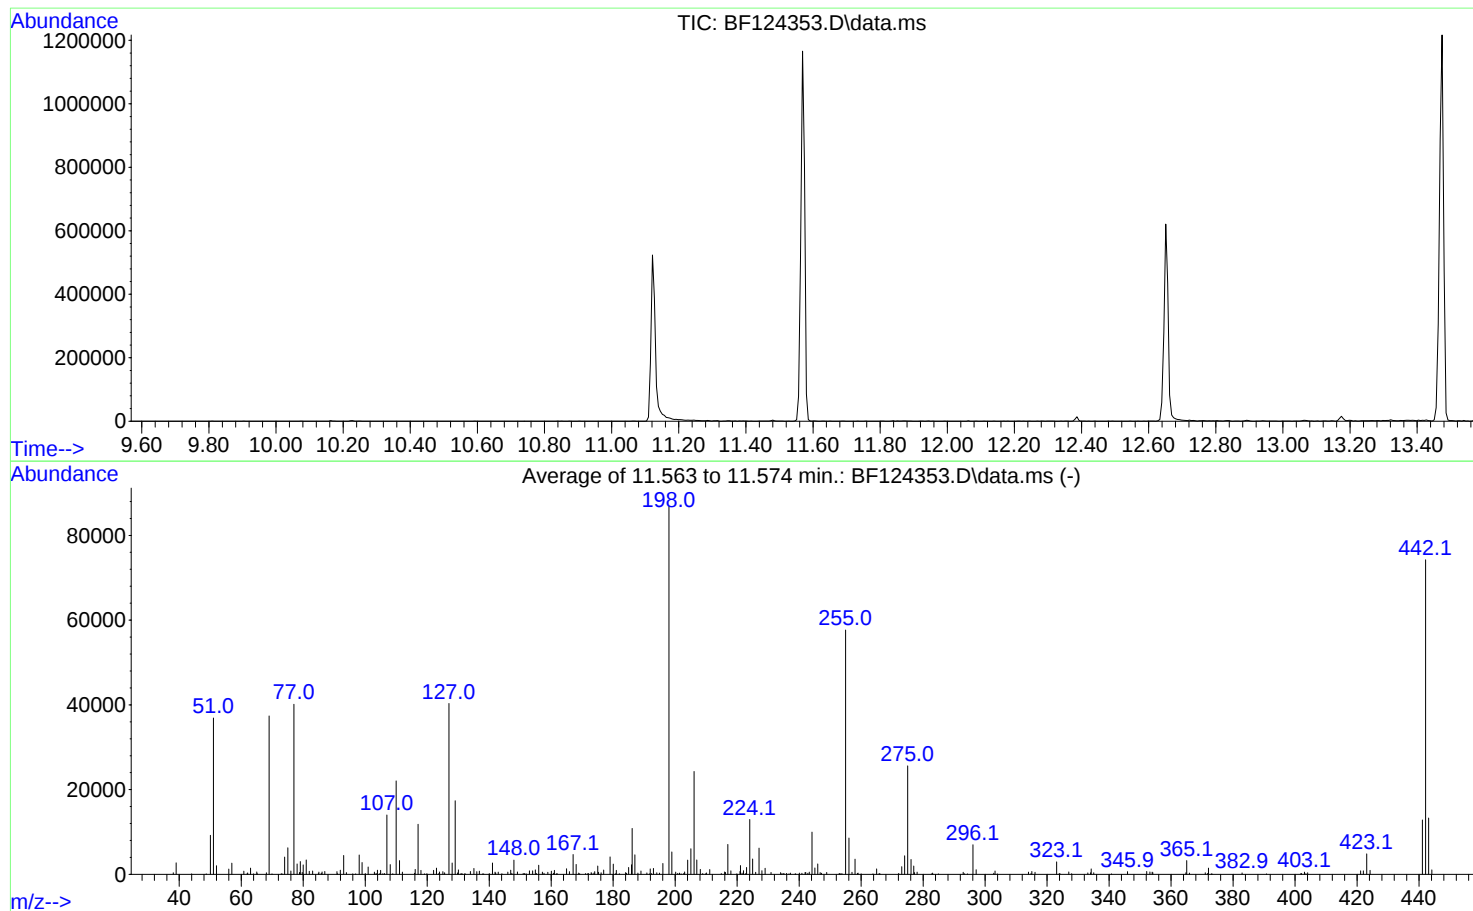




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	36896	PASS
68	69	0.00	2	1.1	396	PASS
69	198	0.00	100	43.1	37400	PASS
70	69	0.00	2	0.3	129	PASS
127	198	10	80	46.5	40328	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86819	PASS
199	198	5	9	6.1	5304	PASS
275	198	10	60	29.5	25620	PASS
365	198	1	100	3.7	3234	PASS
441	198	0.01	100	14.8	12845	PASS
442	442	50	100	100.0	74243	PASS
443	442	15	24	17.9	13284	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
 Data File : BF124353.D
 Acq On : 17 Jun 2021 9:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 11:30:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:09:26 2021
 Response via : Initial Calibration

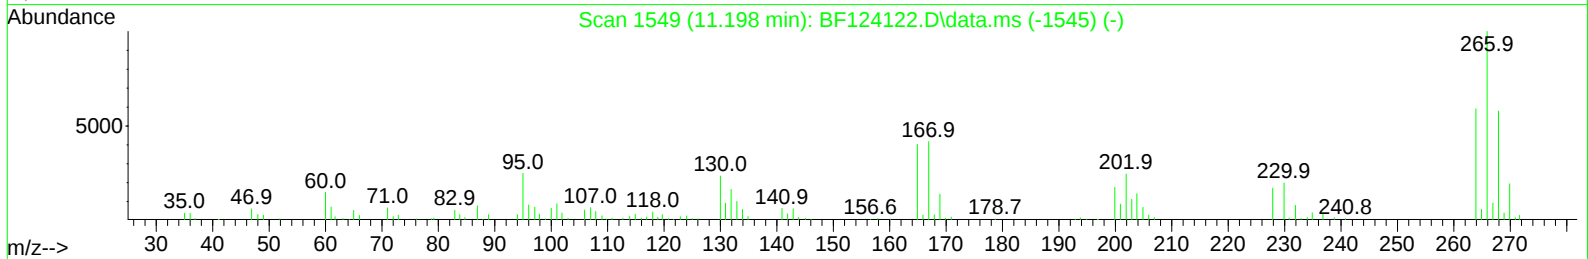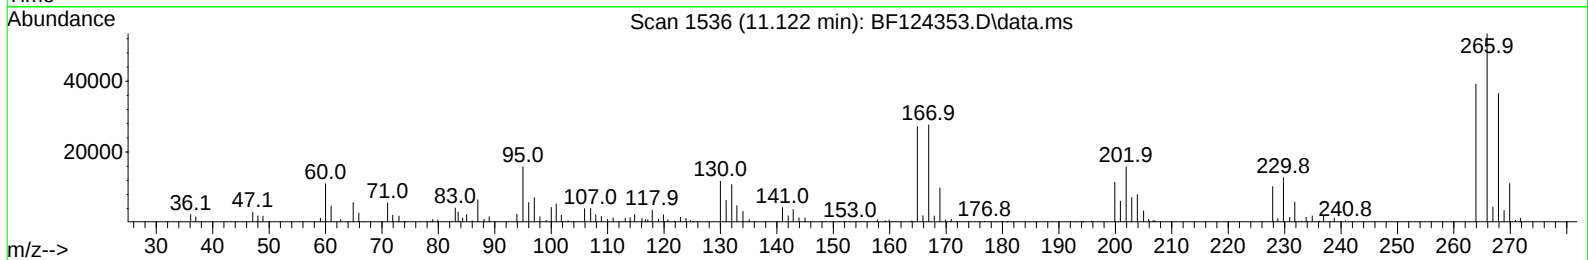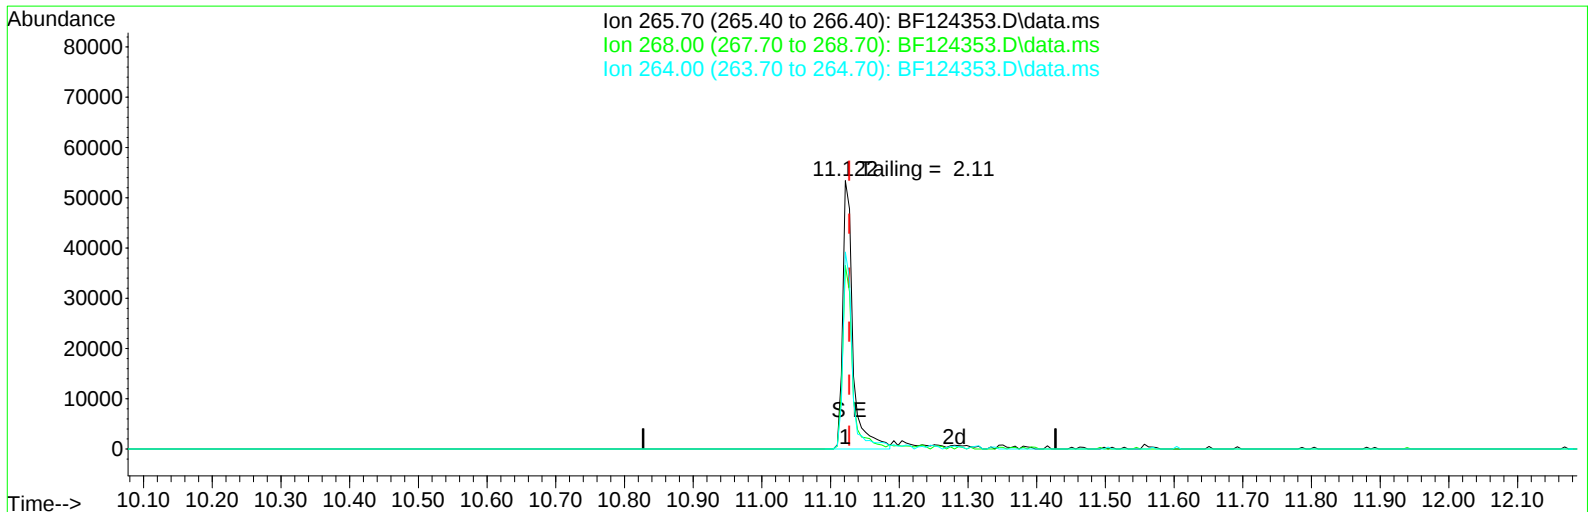

TIC: BF124353.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 20768.59 ng




response 54914

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	68.32
264.00	65.70	73.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061721\
Data File : BF124353.D
Acq On : 17 Jun 2021 9:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 17 11:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

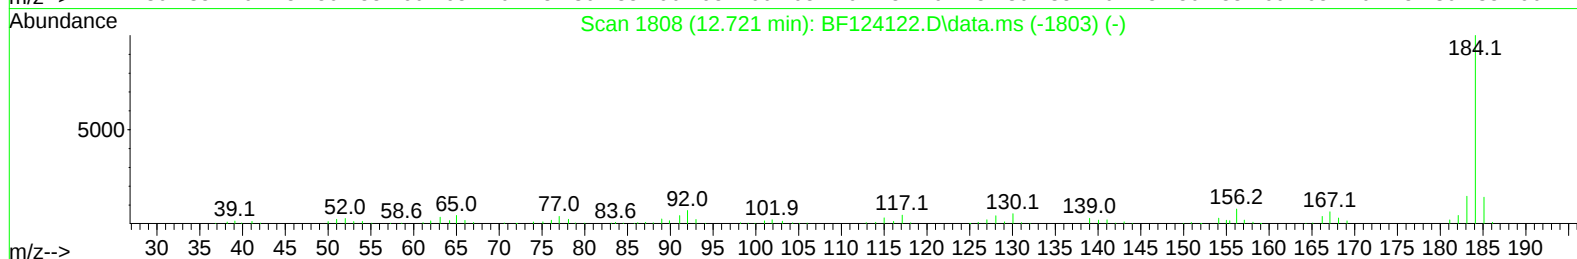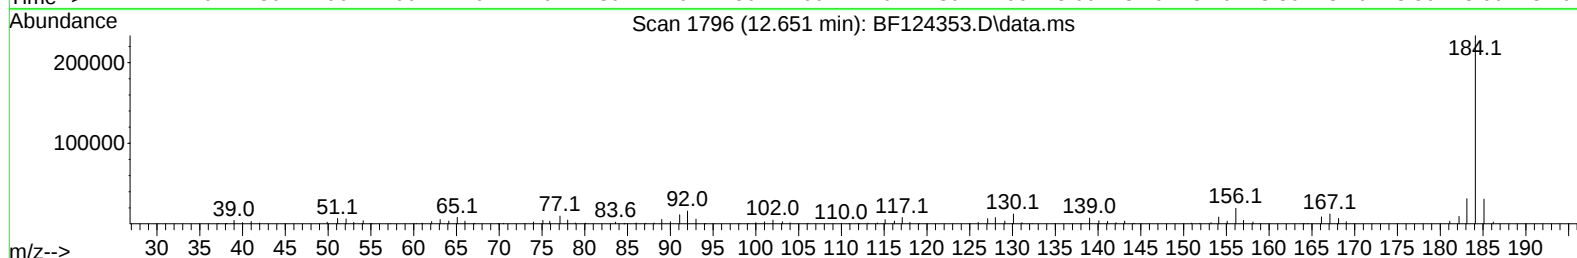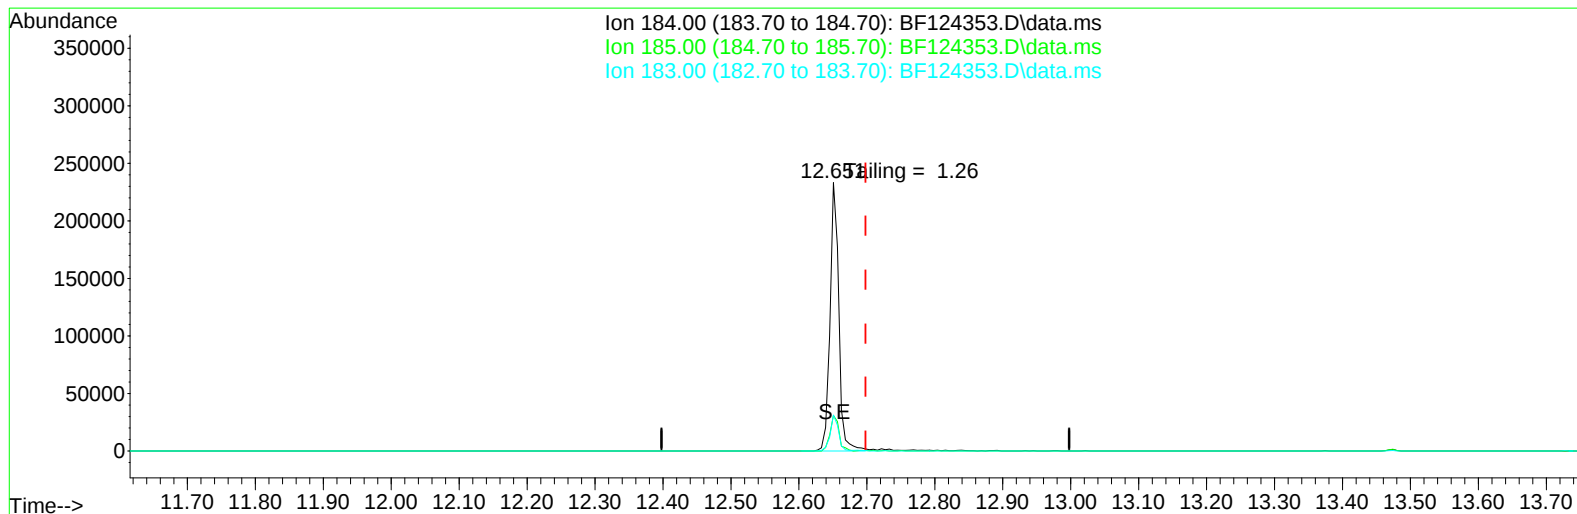

TIC: BF124353.D\data.ms

(77) Benzidine

12.651min (-0.047) 0.00 ng

response 212339

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.24
183.00	9.80	13.46#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/17/2021	BNA_F	<u>BF124353.D</u>
Compound Name	Response	Retention Time
DDT	192622	13.47
DDD	2390	13.17
DDE	150	12.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2540	195162	1.30