
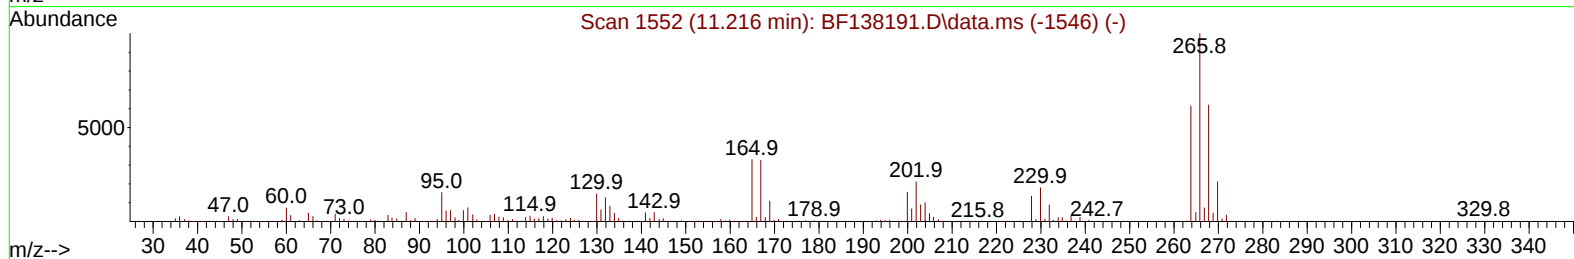
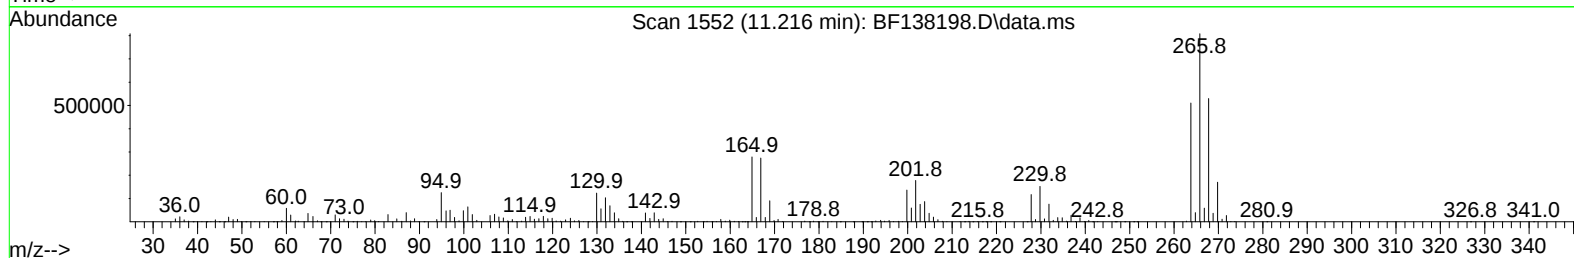


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138198.D
Acq On : 17 Jun 2024 11:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 13:10:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

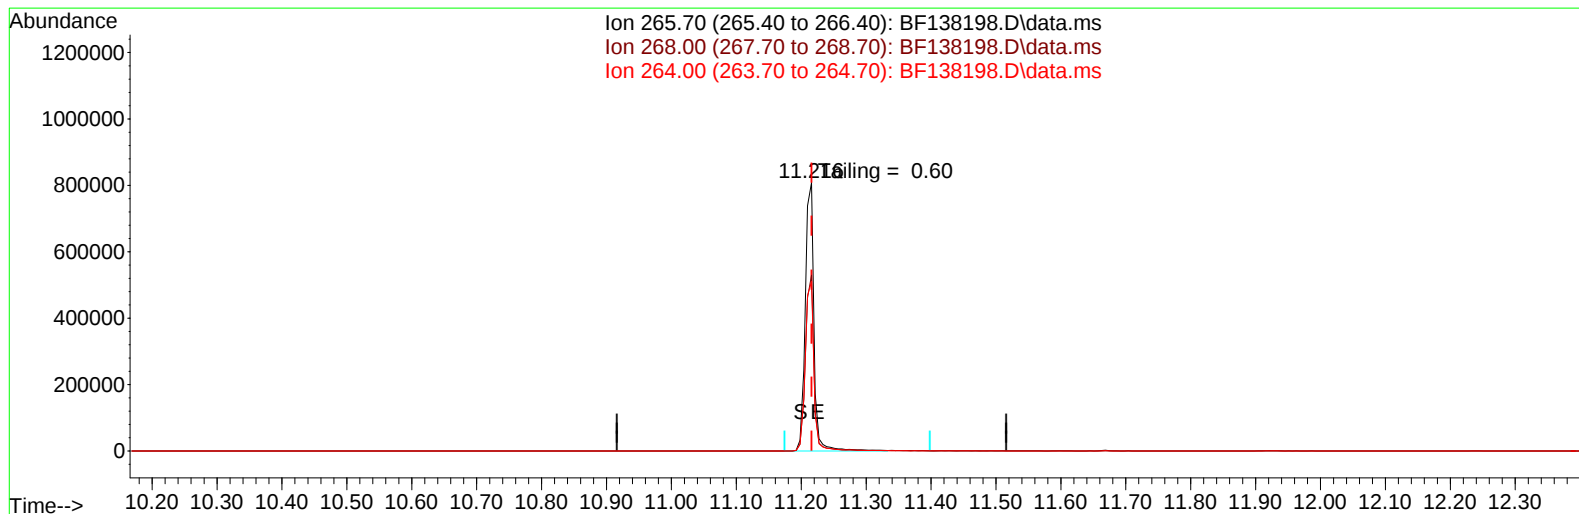

TIC: BF138198.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 375292.24 ng

response 759845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	65.51
264.00	61.50	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138198.D
Acq On : 17 Jun 2024 11:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 13:10:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

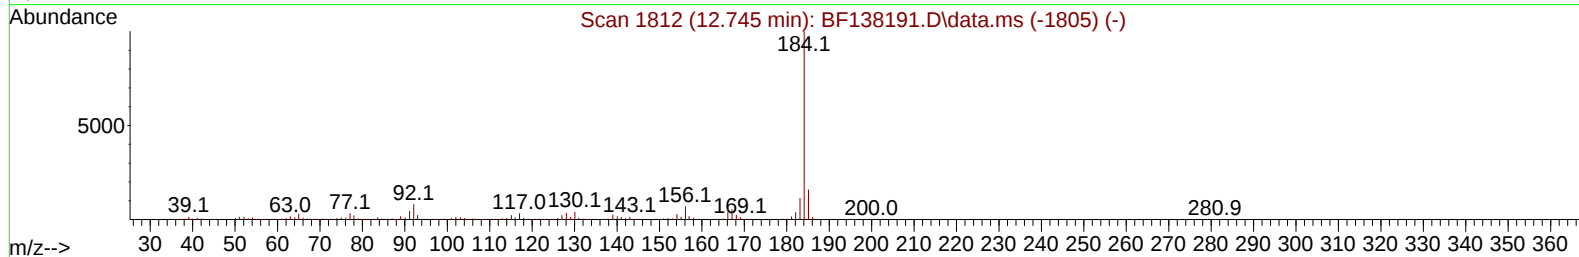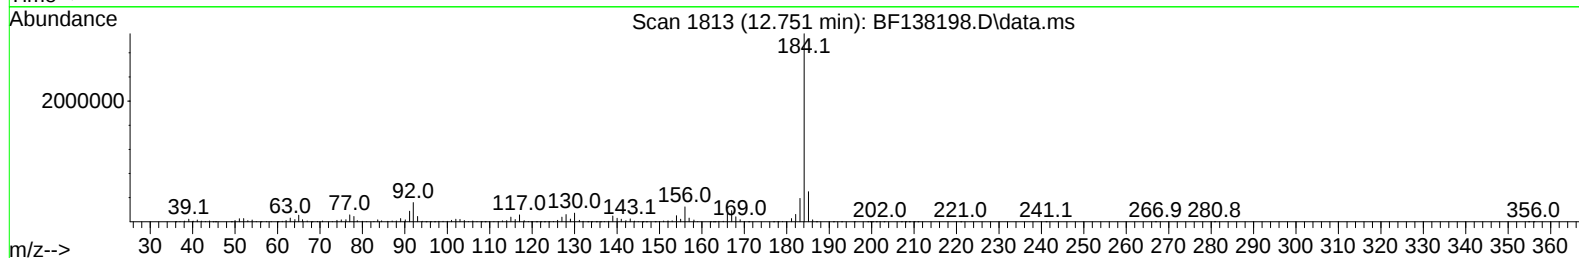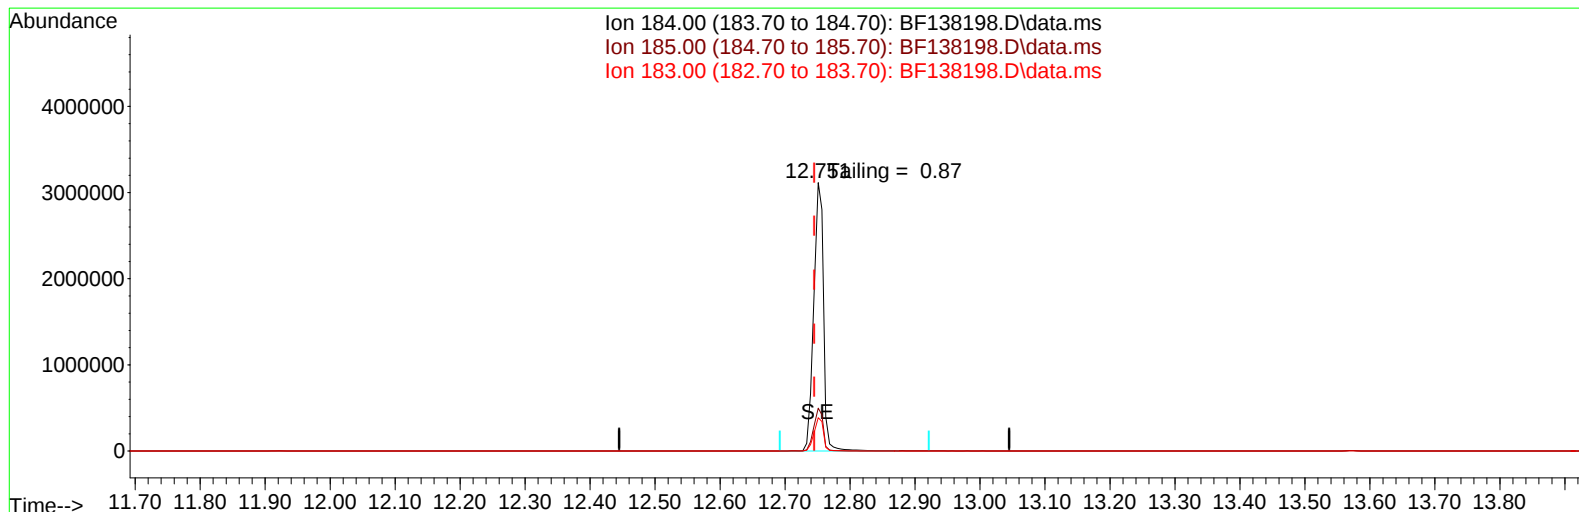

TIC: BF138198.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 125608.28 ng

response 3292214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	16.02
183.00	11.30	12.40
0.00	0.00	0.00