

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
 Data File : BF138200.D
 Acq On : 17 Jun 2024 13:05
 Operator : CG\JU
 Sample : PB161511BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB161511BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.293	21	35	43	rVB	223228	342402	2.51%	0.402%
2	5.139	511	519	528	rBV	441018	629783	4.62%	0.739%
3	5.528	579	585	588	rBV	9438271	10571954	77.54%	12.402%
4	6.522	747	754	756	rBV	8610769	10553554	77.41%	12.380%
5	6.892	813	817	820	rBV	3206686	2656694	19.49%	3.116%
6	7.451	906	912	915	rBV	5997553	6945445	50.94%	8.147%
7	8.169	1029	1034	1038	rBV	3482276	3607204	26.46%	4.231%
8	9.251	1211	1218	1221	rBV	12227909	13232325	97.06%	15.522%
9	9.927	1327	1333	1336	rBV	4453252	4218660	30.94%	4.949%
10	10.716	1460	1467	1470	rBV	8469140	7949233	58.31%	9.325%
11	11.410	1579	1585	1589	rBV	4932644	4355548	31.95%	5.109%
12	13.004	1850	1856	1859	rBV	13201266	13633644	100.00%	15.993%
13	14.045	2029	2033	2037	rBV	3885397	3419315	25.08%	4.011%
14	15.521	2278	2284	2296	rBV	2333309	2924000	21.45%	3.430%
15	17.168	2556	2564	2580	rVB5	48756	207282	1.52%	0.243%




Sum of corrected areas: 85247043

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138200.D
Acq On : 17 Jun 2024 13:05
Operator : CG\JU
Sample : PB161511BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161511BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

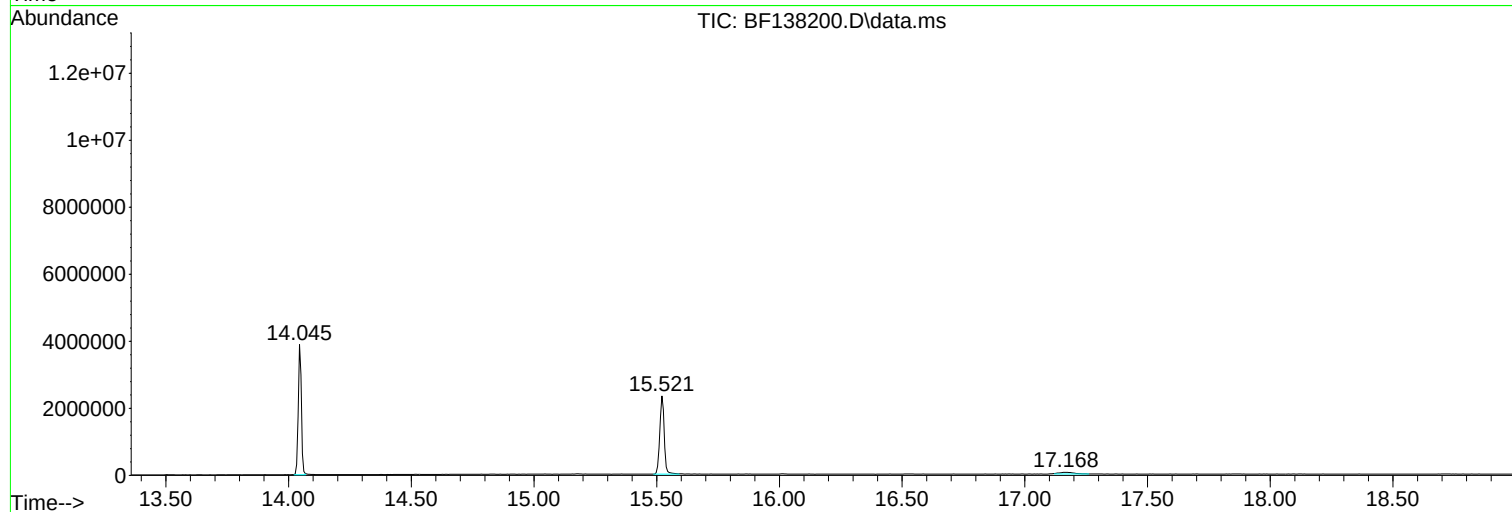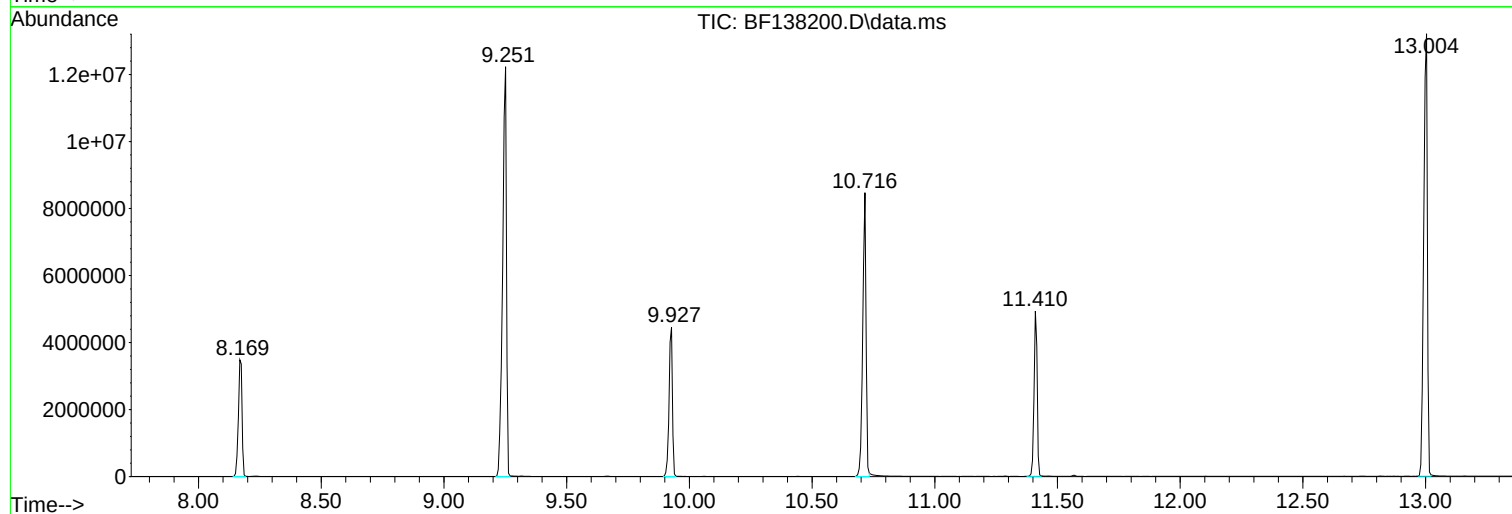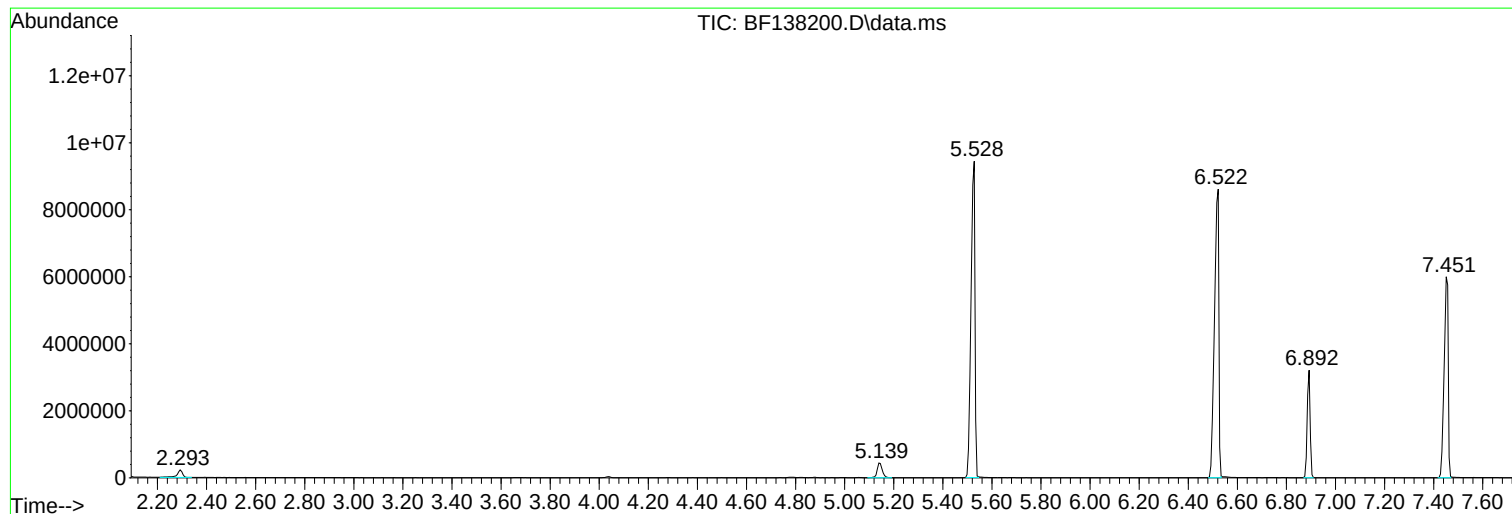

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138200.D
Acq On : 17 Jun 2024 13:05
Operator : CG\JU
Sample : PB161511BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161511BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.293	2.58 ng	342402	1,4-Dichlorobenzene-d4	6.892

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12

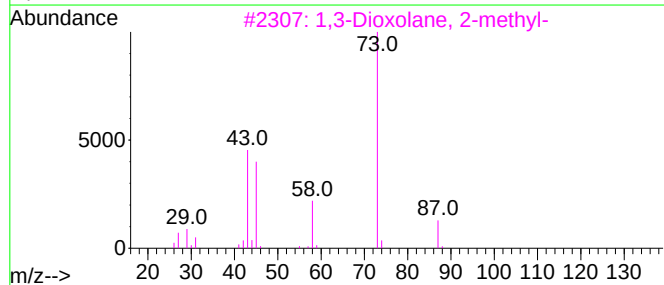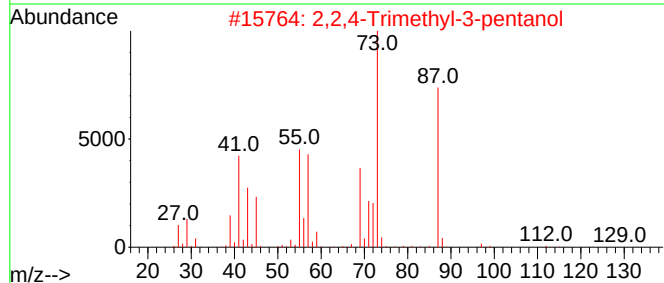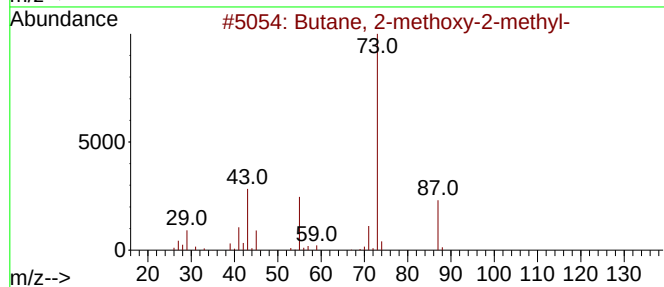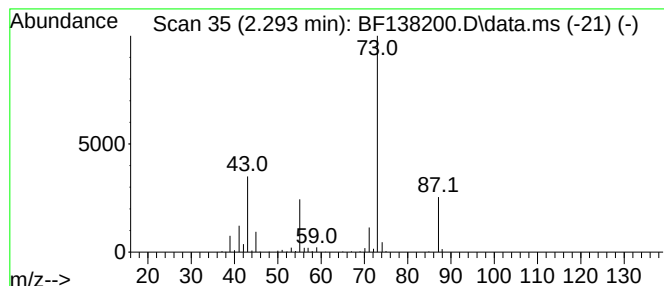

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138200.D
Acq On : 17 Jun 2024 13:05
Operator : CG\JU
Sample : PB161511BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB161511BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.139	4.74 ng	629783	1,4-Dichlorobenzene-d4			6.892
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	83
2	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	16
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	12
4	Acetone		58	C3H6O	000067-64-1	9
5	Butane		58	C4H10	000106-97-8	9

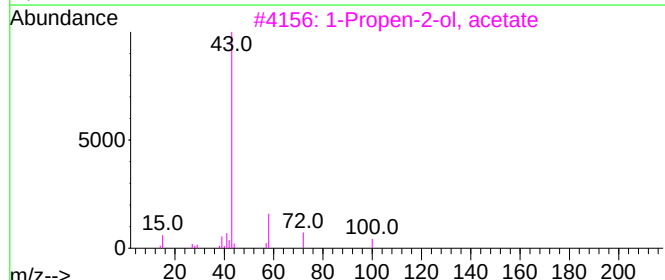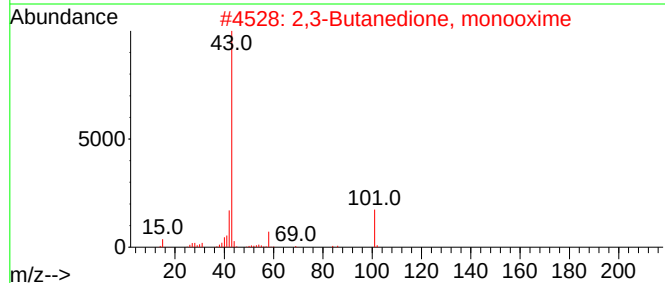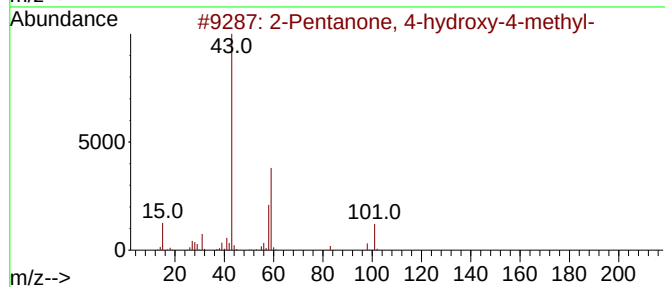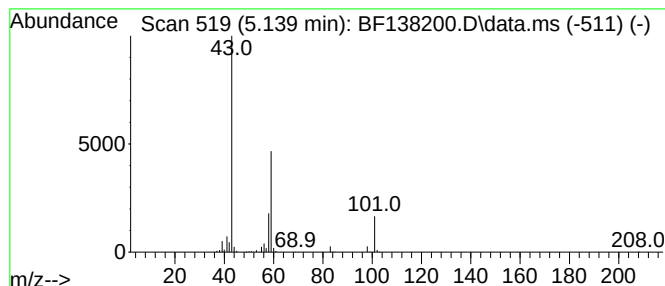

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138200.D
Acq On : 17 Jun 2024 13:05
Operator : CG\JU
Sample : PB161511BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB161511BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.293	2.6	ng	342402	1	6.892	2656690	20.0
2-Pentanone, 4-...	5.139	4.7	ng	629783	1	6.892	2656690	20.0