


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138198.D
Acq On : 17 Jun 2024 11:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

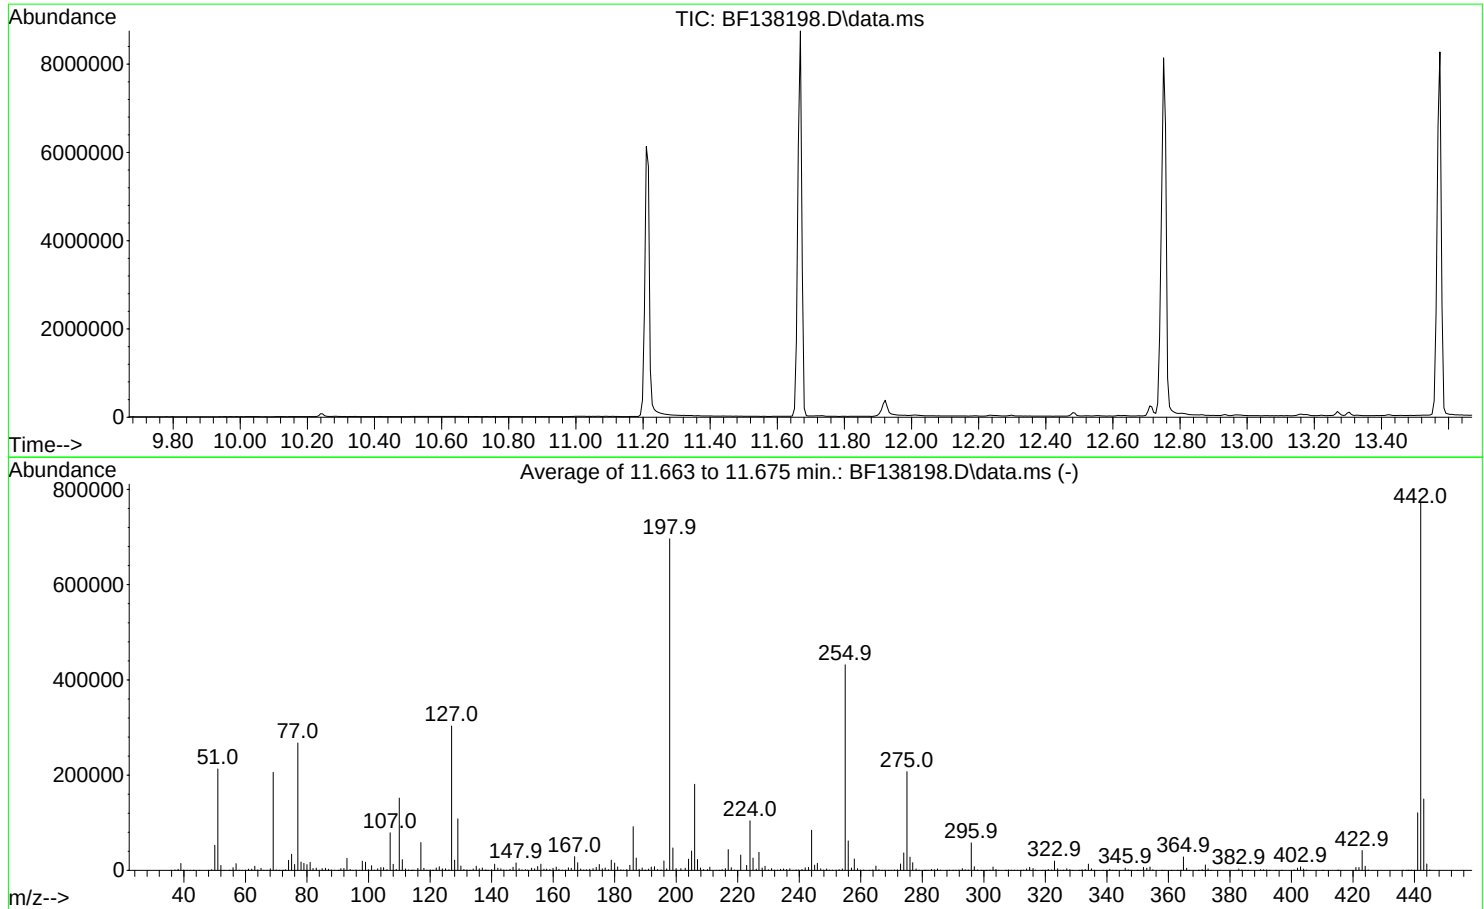




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	213133	PASS
68	69	0.00	2	1.6	3332	PASS
69	198	0.00	100	29.6	206103	PASS
70	69	0.00	2	0.5	1029	PASS
127	198	10	80	43.6	303277	PASS
197	198	0.00	2	0.4	3090	PASS
198	198	100	100	100.0	696192	PASS
199	198	5	9	6.7	46984	PASS
275	198	10	60	29.8	207387	PASS
365	198	1	100	4.1	28307	PASS
441	198	0.01	100	17.4	121037	PASS
442	442	50	100	100.0	772565	PASS
443	442	15	24	19.4	149901	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
 Data File : BF138198.D
 Acq On : 17 Jun 2024 11:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 13:10:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 01:52:47 2024
 Response via : Initial Calibration

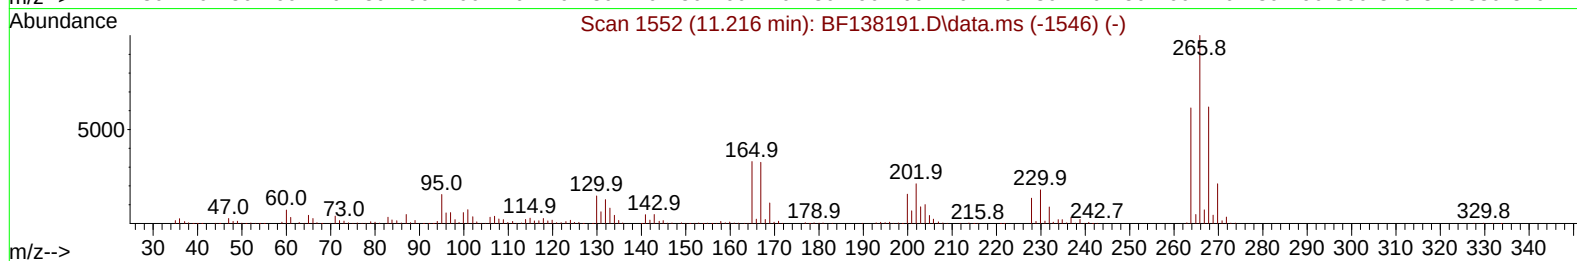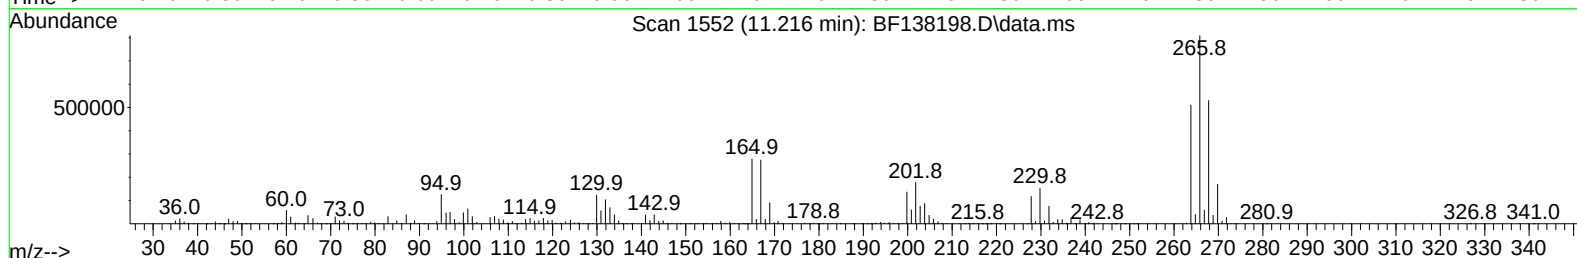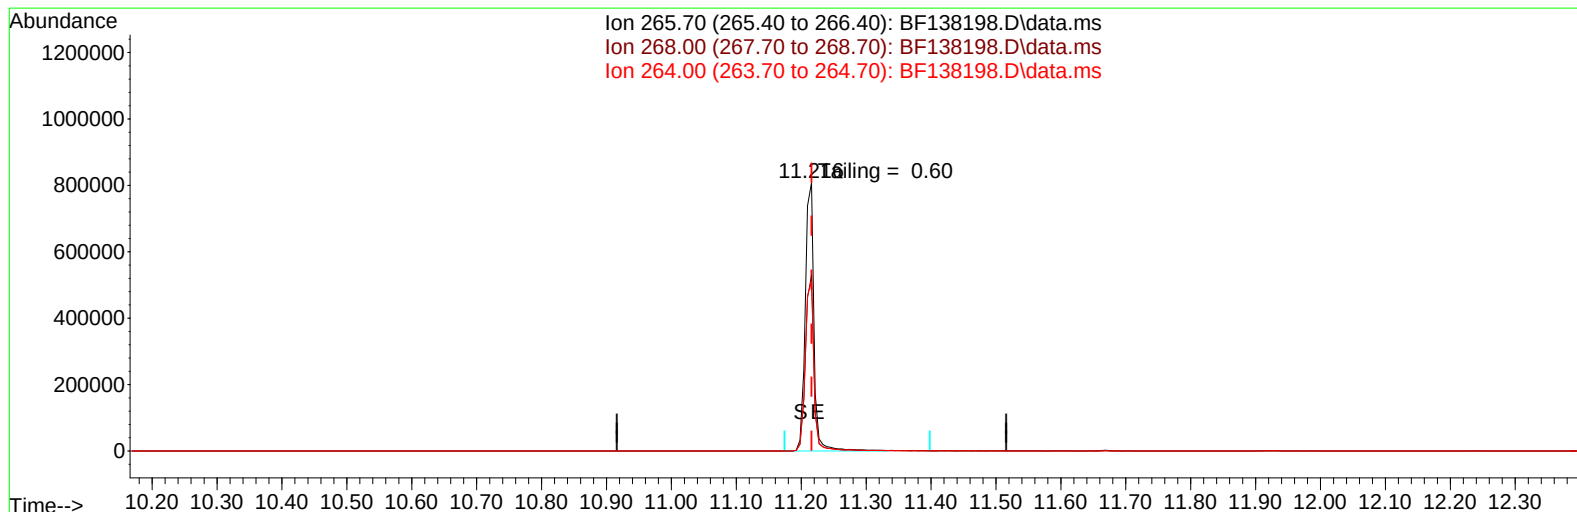

TIC: BF138198.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 375292.24 ng




response 759845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	65.51
264.00	61.50	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061724\
Data File : BF138198.D
Acq On : 17 Jun 2024 11:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 17 13:10:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

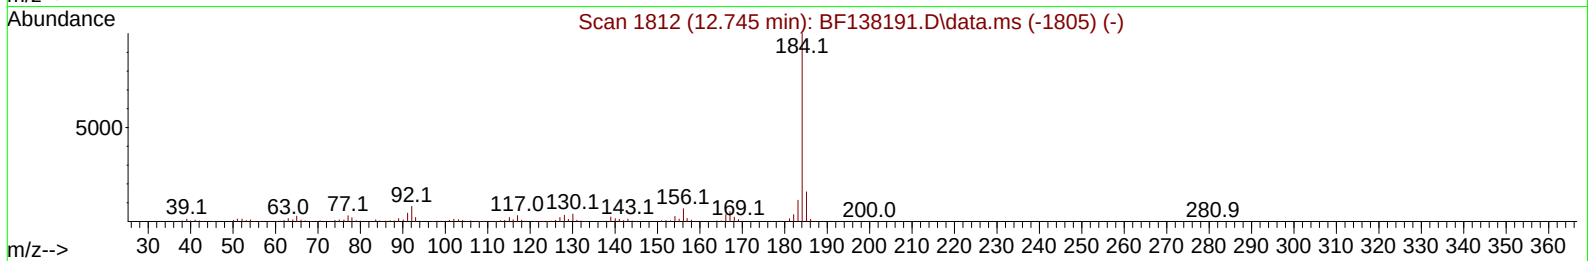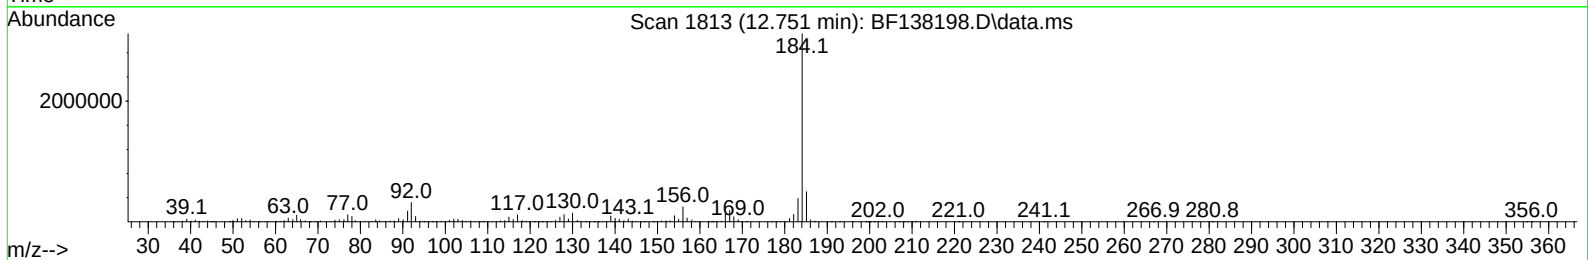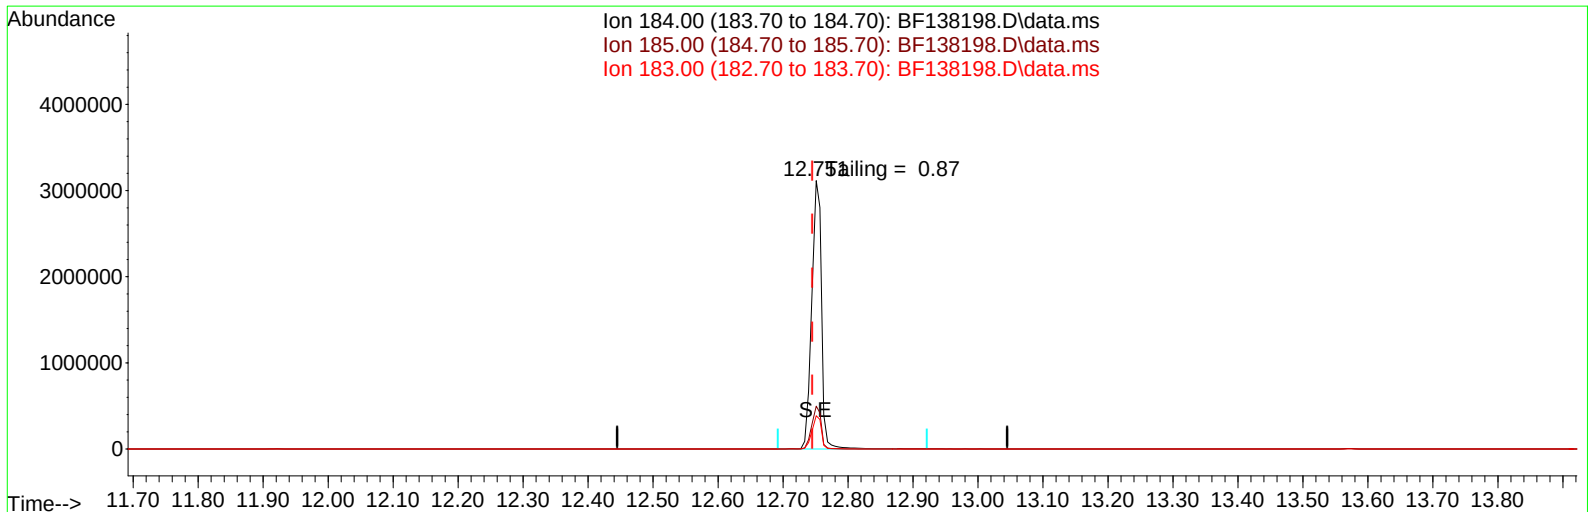

TIC: BF138198.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 125608.28 ng

response 3292214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	16.02
183.00	11.30	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/17/2024	BNA_F	<u>BF138198.D</u>
Compound Name	Response	Retention Time
DDT	1298501	13.574
DDD	22769	13.269
DDE	2202	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24971	1323472	1.89

Instrument :
BNA_F
ClientSampleId :
DFTPP