
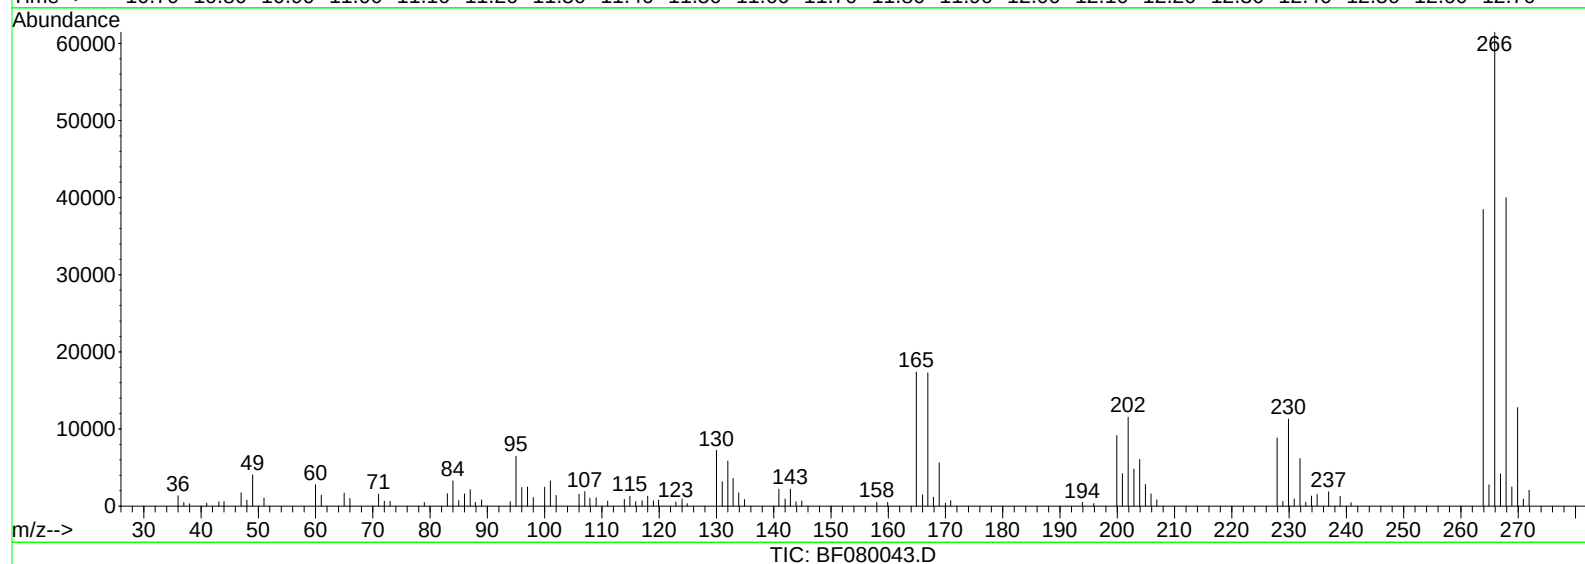


Data Path : Z:\HPCHEM1\BNA F\Data\BF061815\
Data File : BF080043.D
Acq On : 18 Jun 2015 11:38
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:22:46 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 17 16:41:53 2015
Response via : Initial Calibration

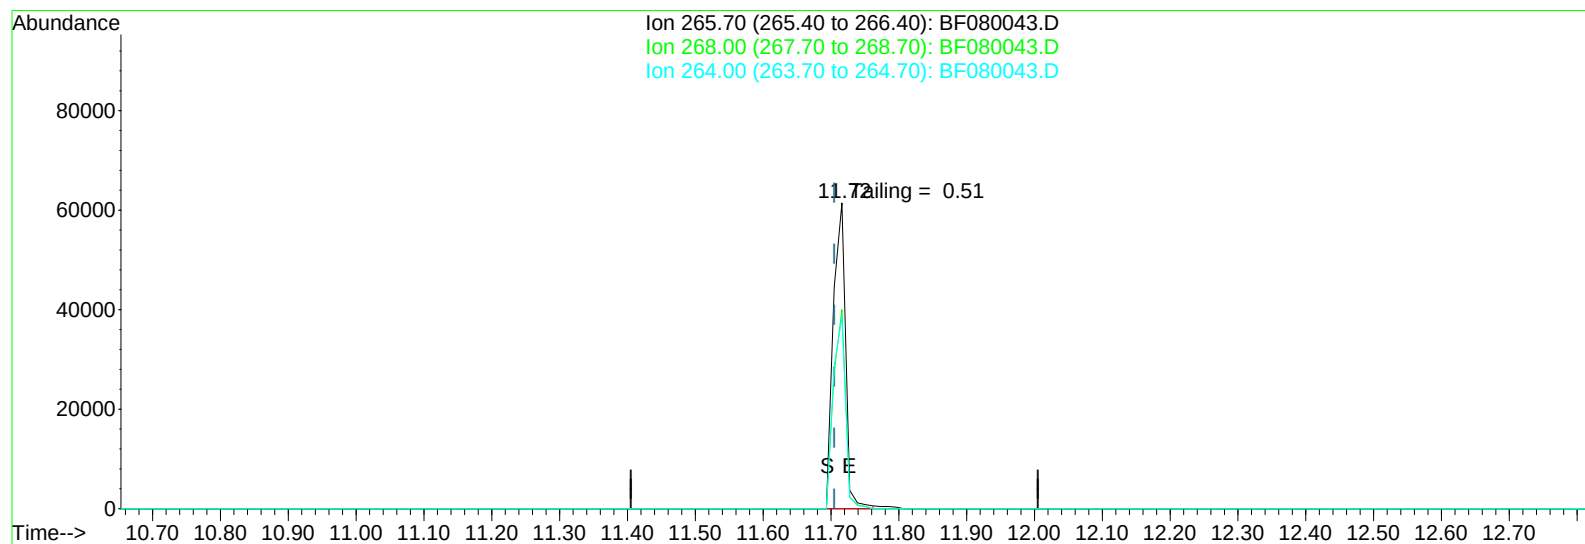

(69) Pentachlorophenol (C)



11.716min (+0.011) 0.00ng

response 77788

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	65.07
264.00	62.70	62.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF061815\
Data File : BF080043.D
Acq On : 18 Jun 2015 11:38
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:22:46 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 17 16:41:53 2015
Response via : Initial Calibration

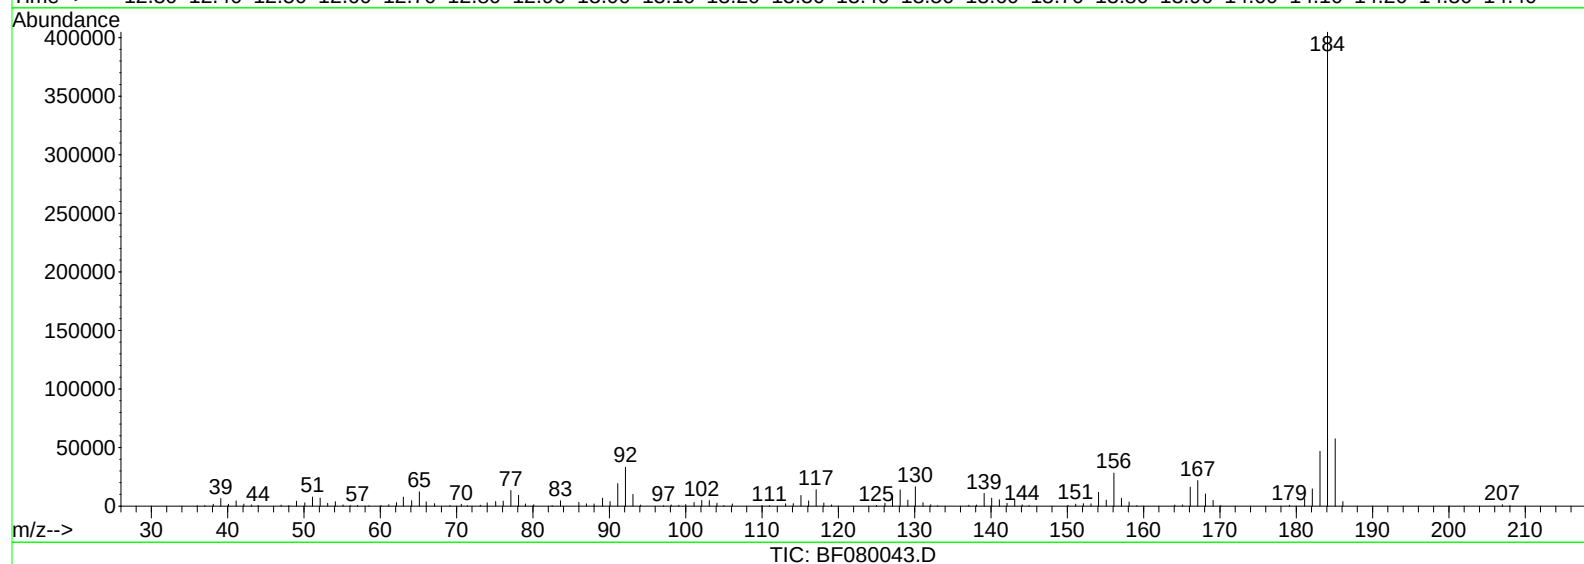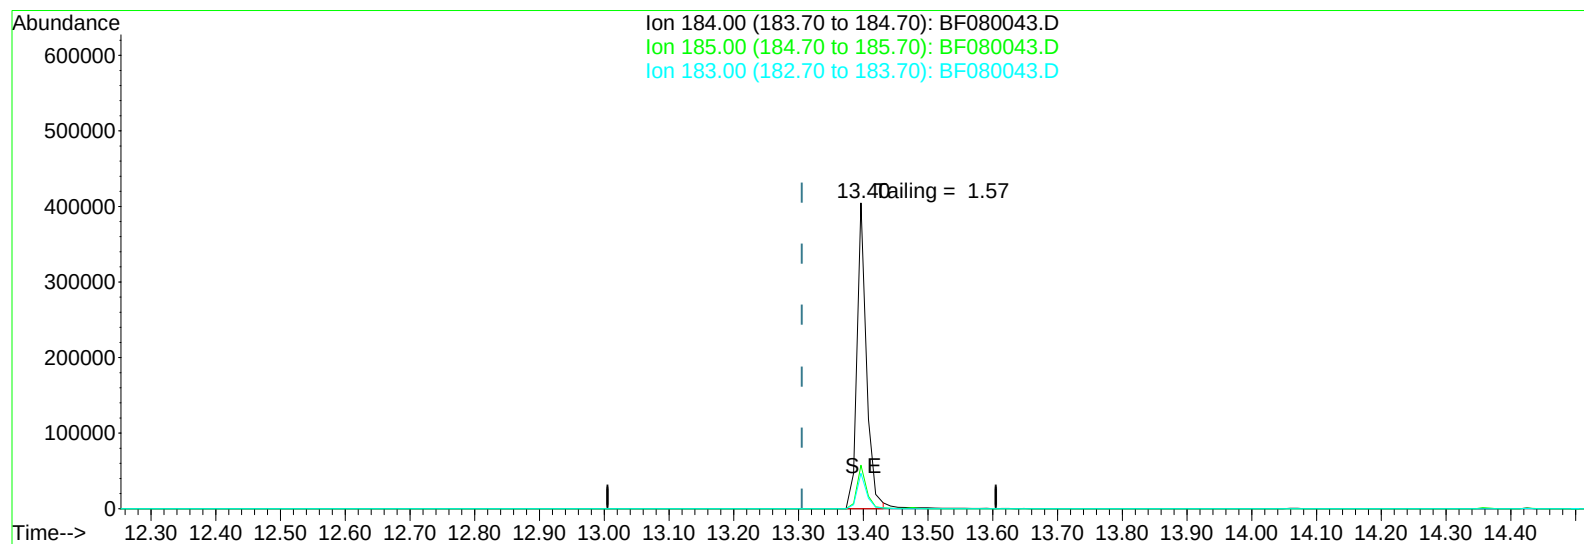

(76) Benzidine

13.396min (+0.091) 0.00ng

response 417182

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.19
183.00	9.50	11.56#
0.00	0.00	0.00