

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
 Data File : BF080045.D
 Acq On : 18 Jun 2015 14:35
 Operator : TP/IZ
 Sample : PB84072BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB84072BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.556	213	216	220	rBV	101116	103245	4.21%	0.679%
2	5.944	248	250	253	rBV	1613799	1387532	56.58%	9.125%
3	6.939	334	337	339	rBV	1579656	1494345	60.94%	9.828%
4	7.099	349	351	353	rBV	1835279	1497321	61.06%	9.847%
5	7.339	369	372	374	rBV	257495	316261	12.90%	2.080%
6	7.487	383	385	388	rBV	798050	1086191	44.30%	7.143%
7	7.887	418	420	422	rBV	1101152	879066	35.85%	5.781%
8	8.630	483	485	487	rVB	351579	432448	17.64%	2.844%
9	9.704	576	579	581	rBV	1943596	1875823	76.50%	12.337%
10	10.402	637	640	642	rVB	504284	533103	21.74%	3.506%
11	11.202	708	710	713	rBV	1192149	1188169	48.45%	7.814%
12	11.956	774	776	779	rBV	697326	620604	25.31%	4.081%
13	13.842	938	941	943	rBV	1942382	2452151	100.00%	16.127%
14	15.282	1065	1067	1070	rBV	495758	690833	28.17%	4.543%
15	17.397	1249	1252	1256	rBV	432385	648371	26.44%	4.264%


Sum of corrected areas: 15205463

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080045.D
Acq On : 18 Jun 2015 14:35
Operator : TP/IZ
Sample : PB84072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84072BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

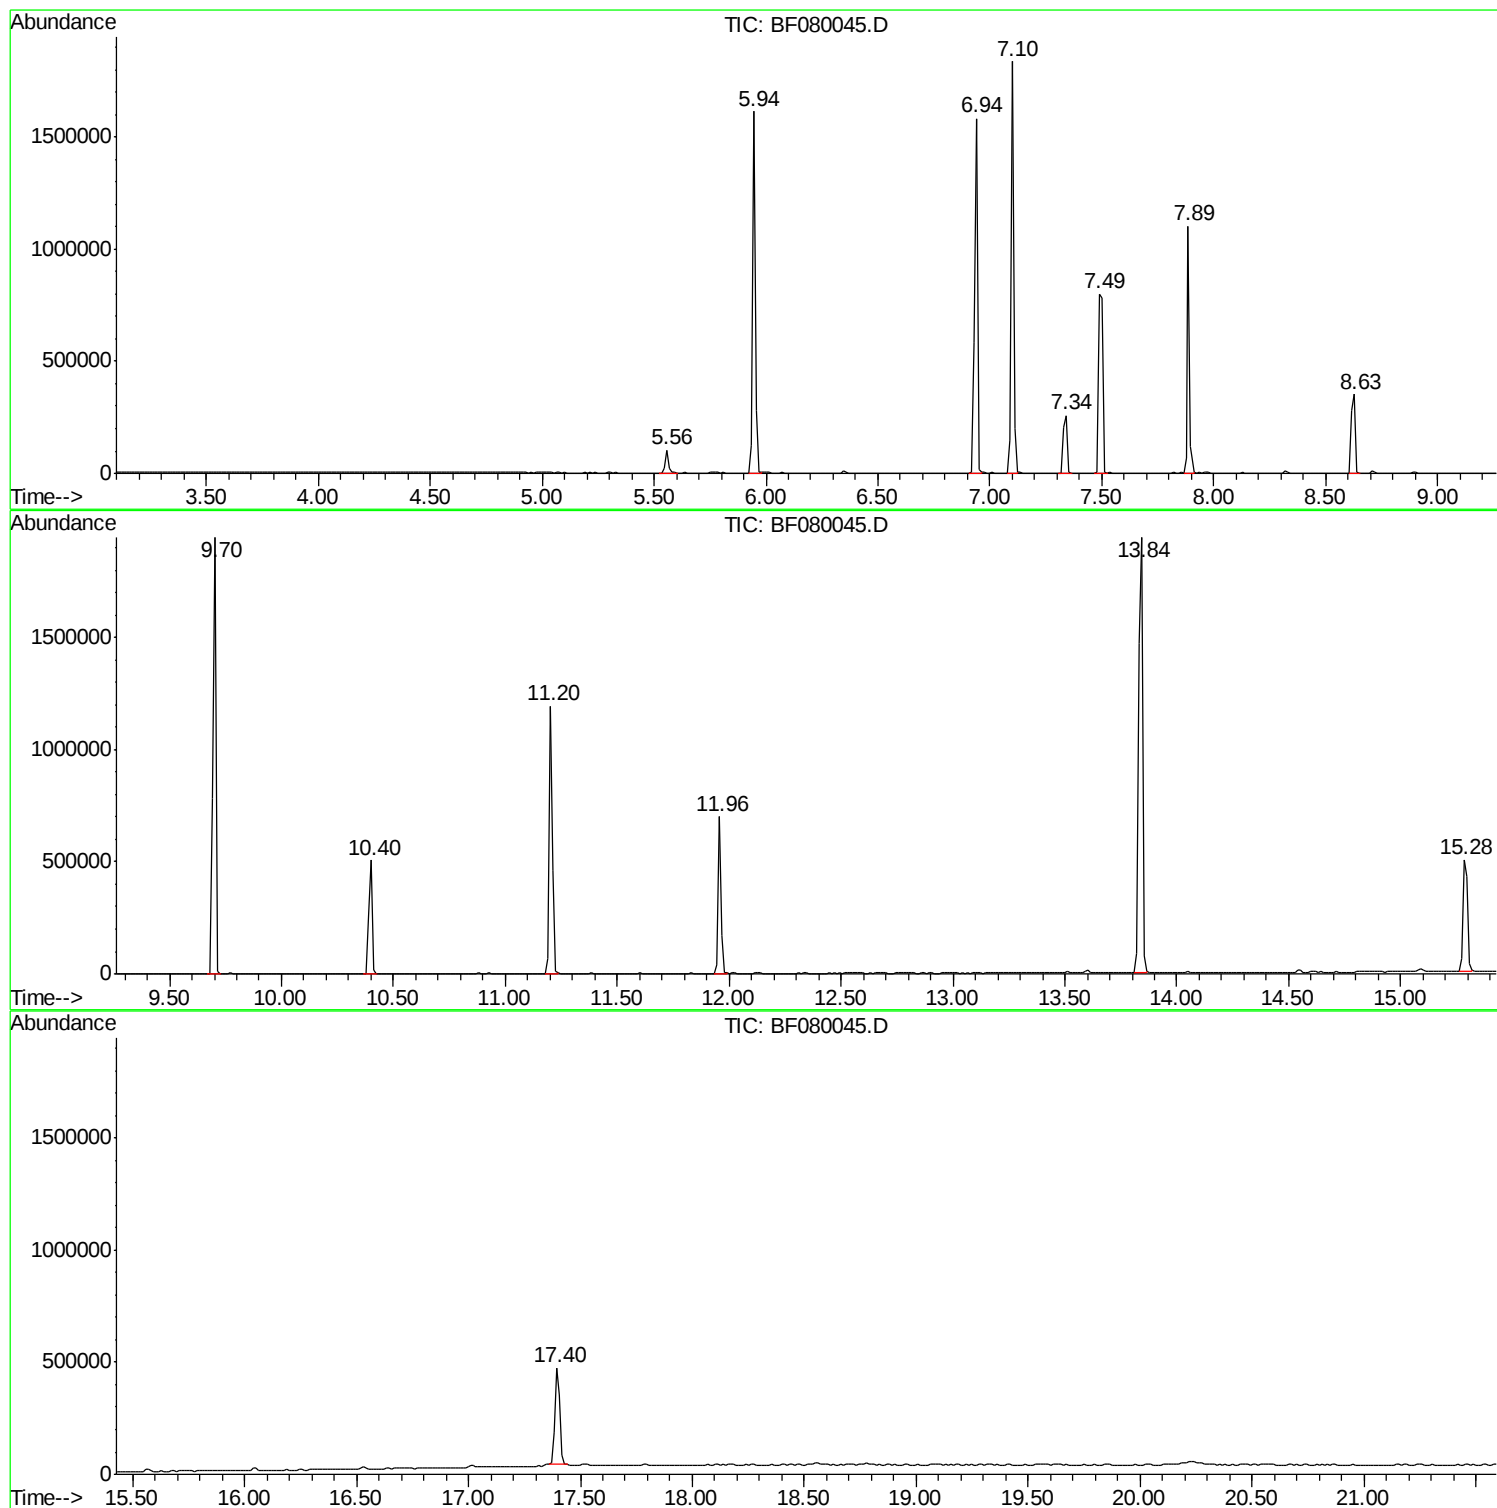

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080045.D
Acq On : 18 Jun 2015 14:35
Operator : TP/IZ
Sample : PB84072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84072BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.56	6.53 ng	103245	1,4-Dichlorobenzene-d4	7.34

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
4			3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	9
5			3-Heptanol	116	C7H16O	000589-82-2	9

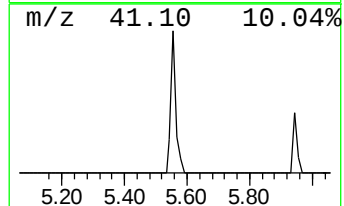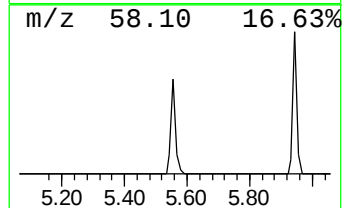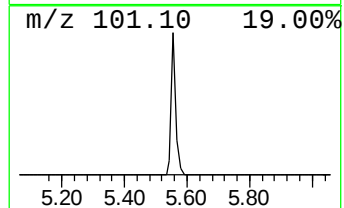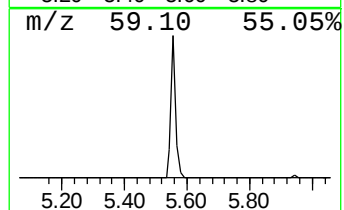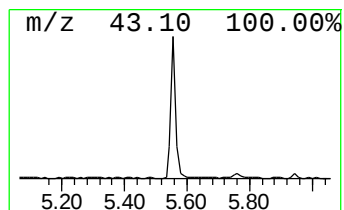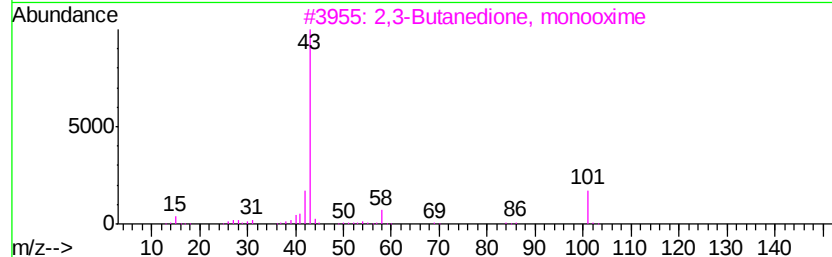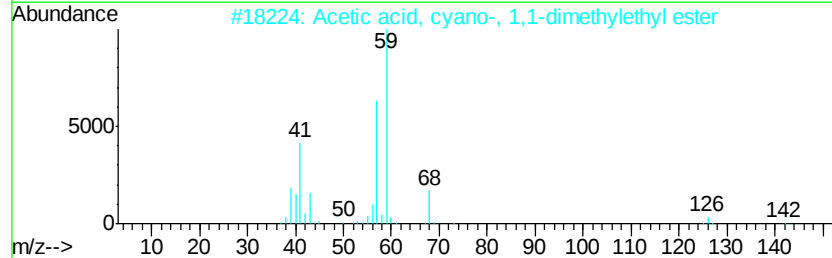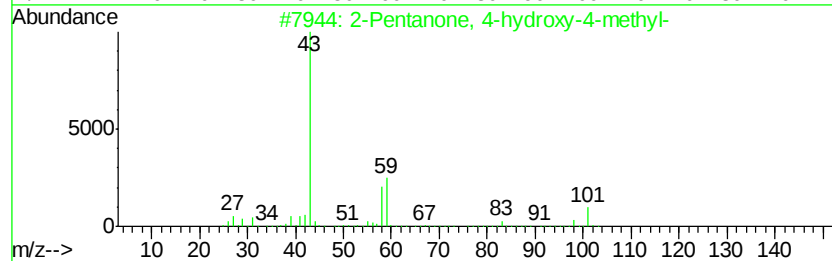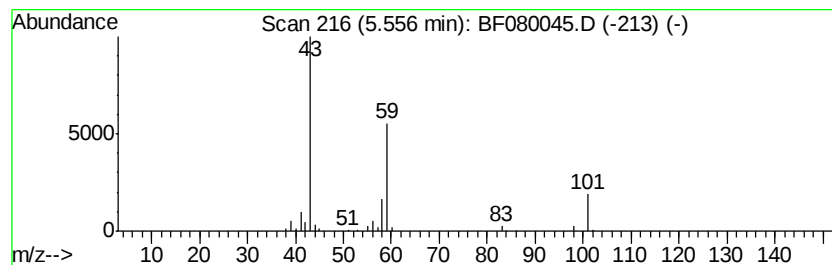

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080045.D
Acq On : 18 Jun 2015 14:35
Operator : TP/IZ
Sample : PB84072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84072BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.10 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.10	94.69 ng	1497320	1,4-Dichlorobenzene-d4	7.34

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

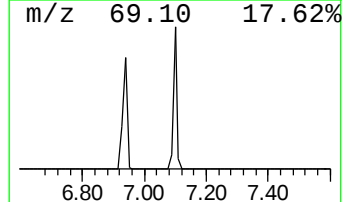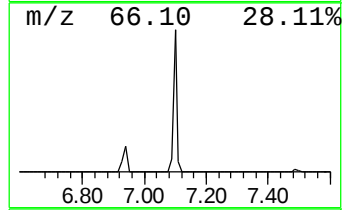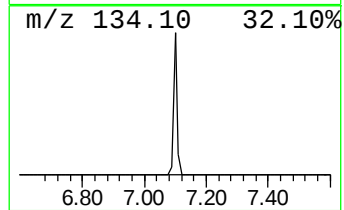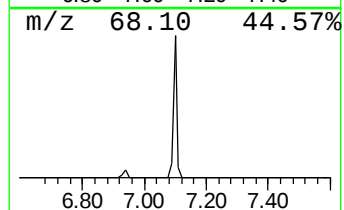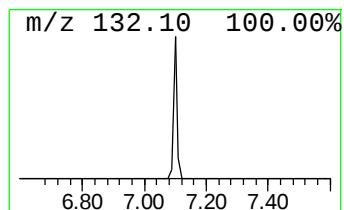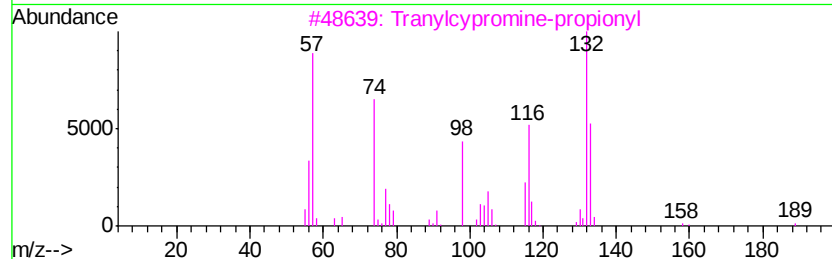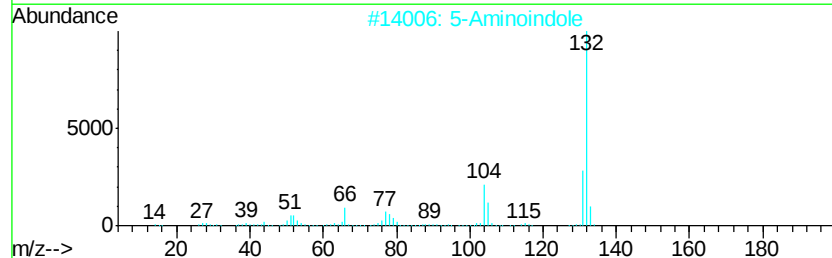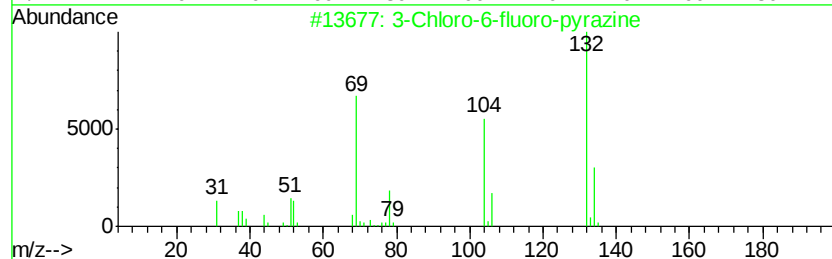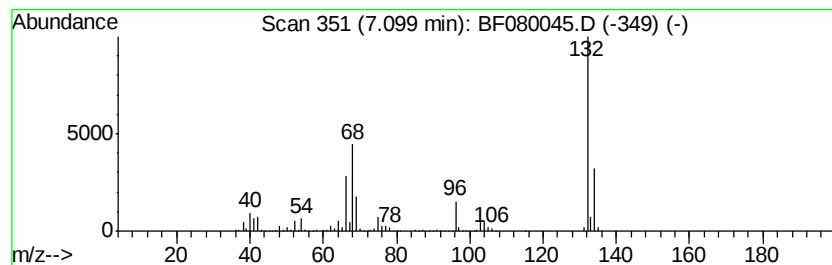

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080045.D
Acq On : 18 Jun 2015 14:35
Operator : TP/IZ
Sample : PB84072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84072BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.56	6.5	ng	103245	1	7.34	316261	20.0
unknown7.10	7.10	94.7	ng	1497320	1	7.34	316261	20.0