

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
 Data File : BF080047.D
 Acq On : 18 Jun 2015 15:33
 Operator : TP/IZ
 Sample : G2656-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.544	214	215	222	rVB	96520	114561	17.82%	2.094%
2	5.944	247	250	252	rBV	334426	304316	47.34%	5.564%
3	6.344	283	285	287	rVB	11647	9423	1.47%	0.172%
4	6.927	334	336	339	rVB	343474	301522	46.90%	5.513%
5	7.099	348	351	353	rBV	425123	367044	57.10%	6.710%
6	7.327	370	371	374	rVB	202868	235547	36.64%	4.306%
7	7.487	383	385	387	rVB	309564	288844	44.93%	5.281%
8	7.887	418	420	422	rBV	274724	225848	35.13%	4.129%
9	8.619	482	484	487	rVB	305979	327560	50.96%	5.989%
10	9.693	576	578	581	rBV	435671	474089	73.75%	8.668%
11	10.390	637	639	642	rBV2	331150	394784	61.41%	7.218%
12	11.099	699	701	703	rBV	11266	11108	1.73%	0.203%
13	11.191	707	709	711	rBV	346008	317498	49.39%	5.805%
14	11.922	770	773	775	rVB	462288	458097	71.26%	8.375%
15	13.694	925	928	931	rBV	712450	642837	100.00%	11.753%
16	14.837	1025	1028	1029	rBV	7463	10633	1.65%	0.194%
17	15.054	1044	1047	1050	rVB	448958	499998	77.78%	9.141%
18	17.031	1216	1220	1223	rBV	312673	486020	75.61%	8.886%


Sum of corrected areas: 5469729

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080047.D
Acq On : 18 Jun 2015 15:33
Operator : TP/IZ
Sample : G2656-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN001

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

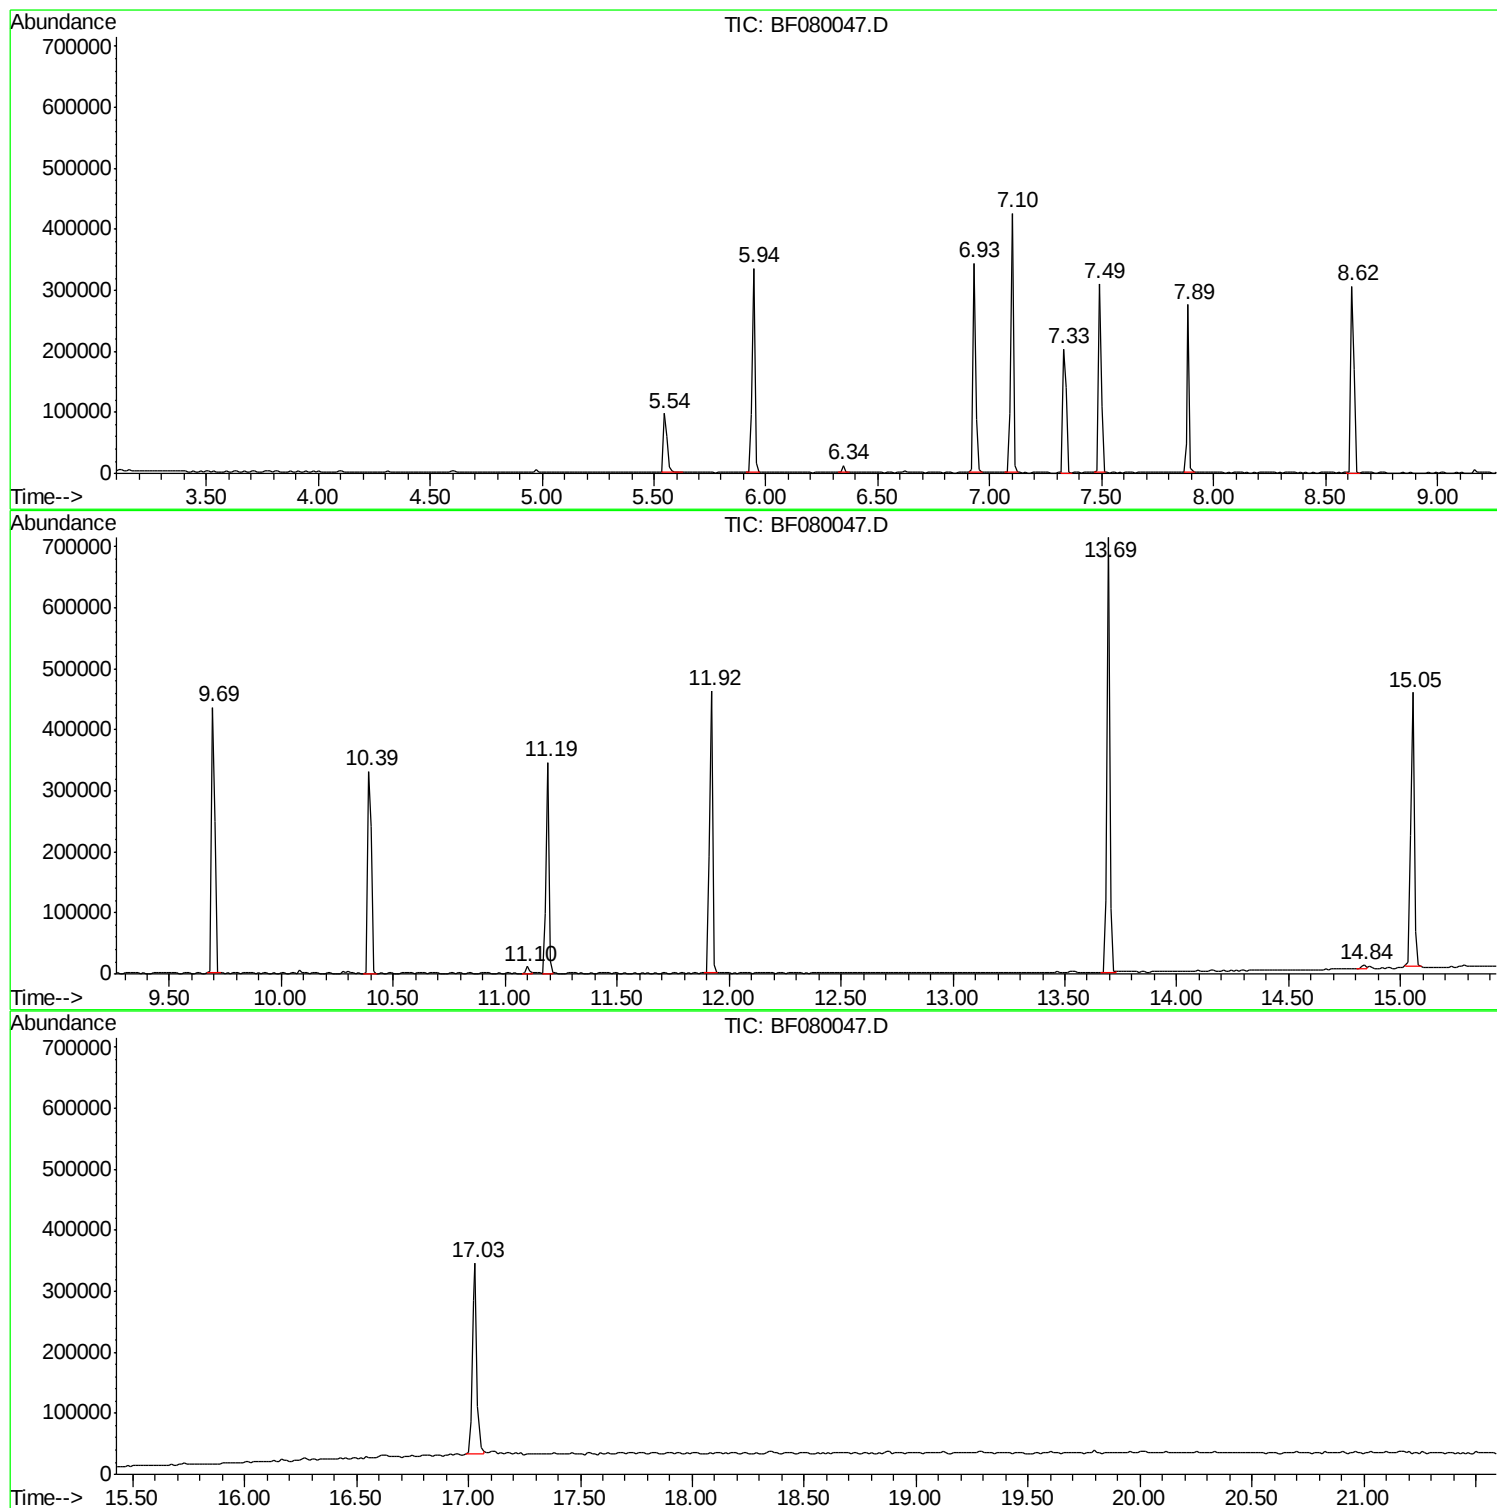

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080047.D
Acq On : 18 Jun 2015 15:33
Operator : TP/IZ
Sample : G2656-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN001










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.54	9.73 ng	114561	1,4-Dichlorobenzene-d4	7.33

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	40
3			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	30
5			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28

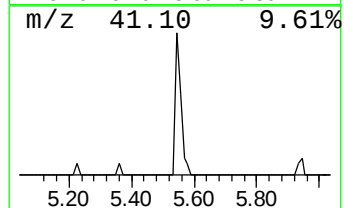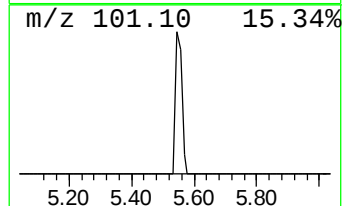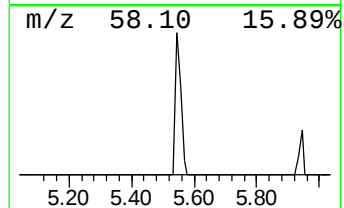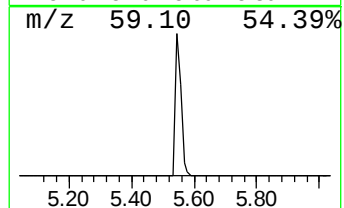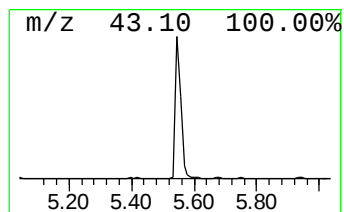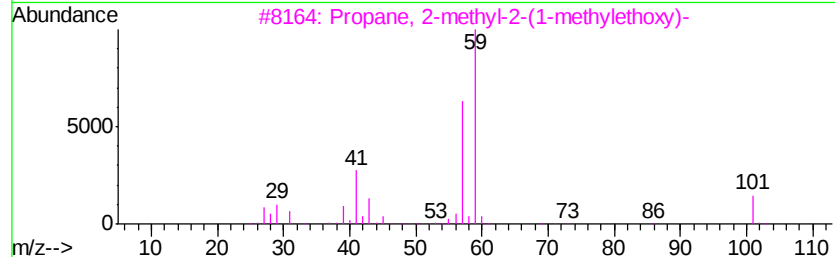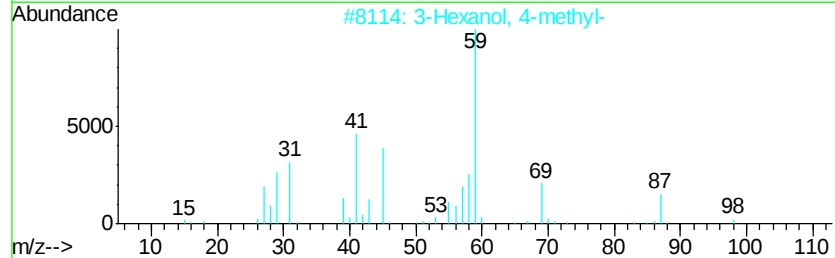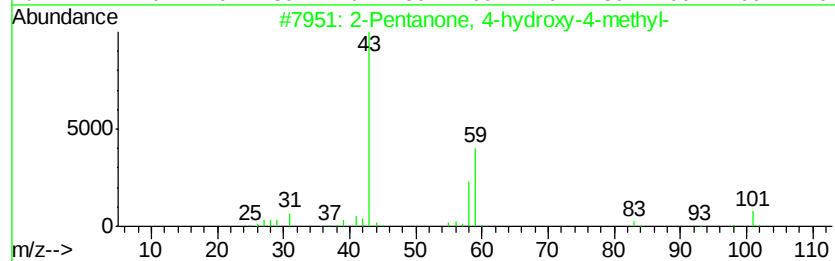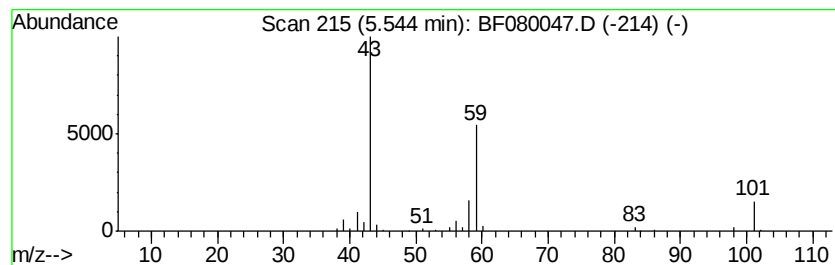

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080047.D
Acq On : 18 Jun 2015 15:33
Operator : TP/IZ
Sample : G2656-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN001










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.10 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.10	31.17 ng	367044	1,4-Dichlorobenzene-d4	7.33

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

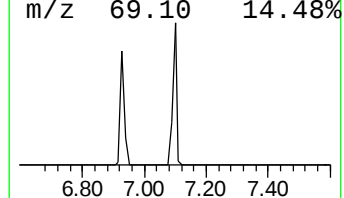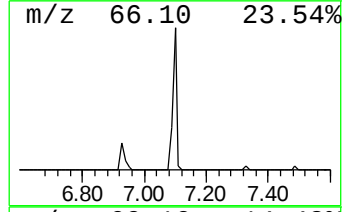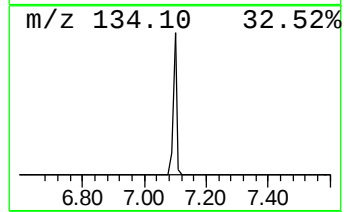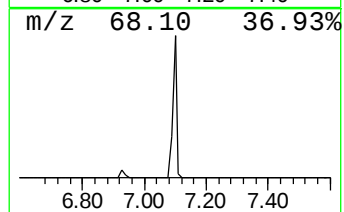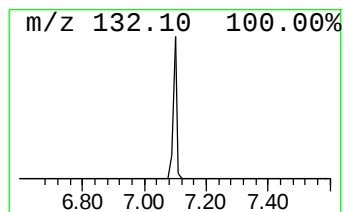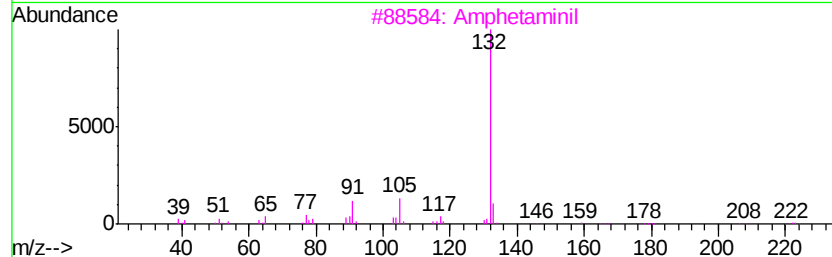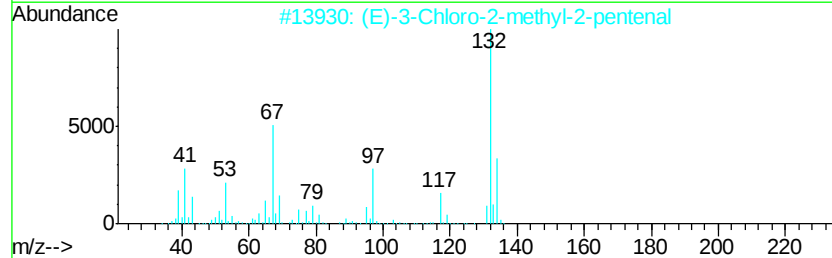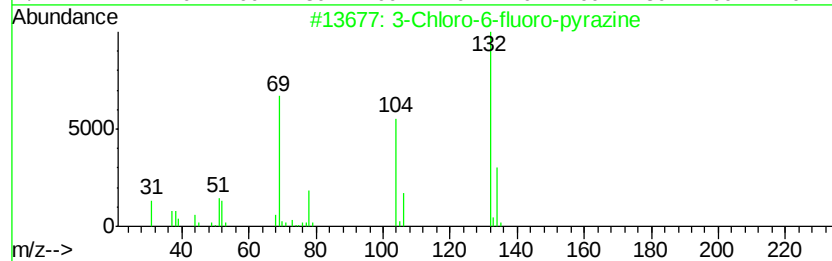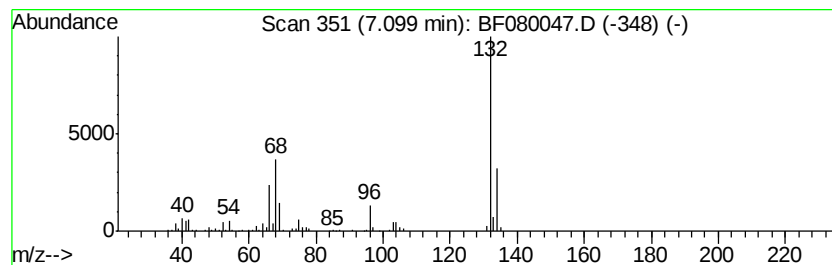

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061815\
Data File : BF080047.D
Acq On : 18 Jun 2015 15:33
Operator : TP/IZ
Sample : G2656-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN001

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.54	9.7	ng	114561	1	7.33	235547	20.0
unknown7.10	7.10	31.2	ng	367044	1	7.33	235547	20.0