

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061816\
 Data File : BF088135.D
 Acq On : 18 Jun 2016 15:43
 Operator : UM/SJ
 Sample : H3501-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SED2-0-6

Quant Time: Jun 20 05:20:10 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 17 16:09:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	104446	20.00	ng	-0.01
21) Naphthalene-d8	7.98	136	383519	20.00	ng	-0.01
38) Acenaphthene-d10	9.72	164	158743	20.00	ng	-0.01
63) Phenanthrene-d10	11.20	188	246949	20.00	ng	-0.01
75) Chrysene-d12	13.83	240	204184	20.00	ng	-0.02
86) Perylene-d12	15.21	264	159840	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	665823	108.98	ng	0.01
7) Phenol-d6	6.35	99	901621	121.77	ng	0.00
23) Nitrobenzene-d5	7.26	82	428320	65.22	ng	-0.02
41) 2,4,6-Tribromophenol	10.51	330	127386	76.00	ng	-0.01
44) 2-Fluorobiphenyl	9.05	172	832107	82.16	ng	-0.02
78) Terphenyl-d14	12.79	244	643648	71.73	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.45	163	135138	11.75	ng	99
83) Bis(2-ethylhexyl)phthalate	13.82	149	27956	3.43	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061816\
Data File : BF088135.D
Acq On : 18 Jun 2016 15:43
Operator : UM/SJ
Sample : H3501-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SED2-0-6

Quant Time: Jun 20 05:20:10 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 17 16:09:13 2016
Response via : Initial Calibration

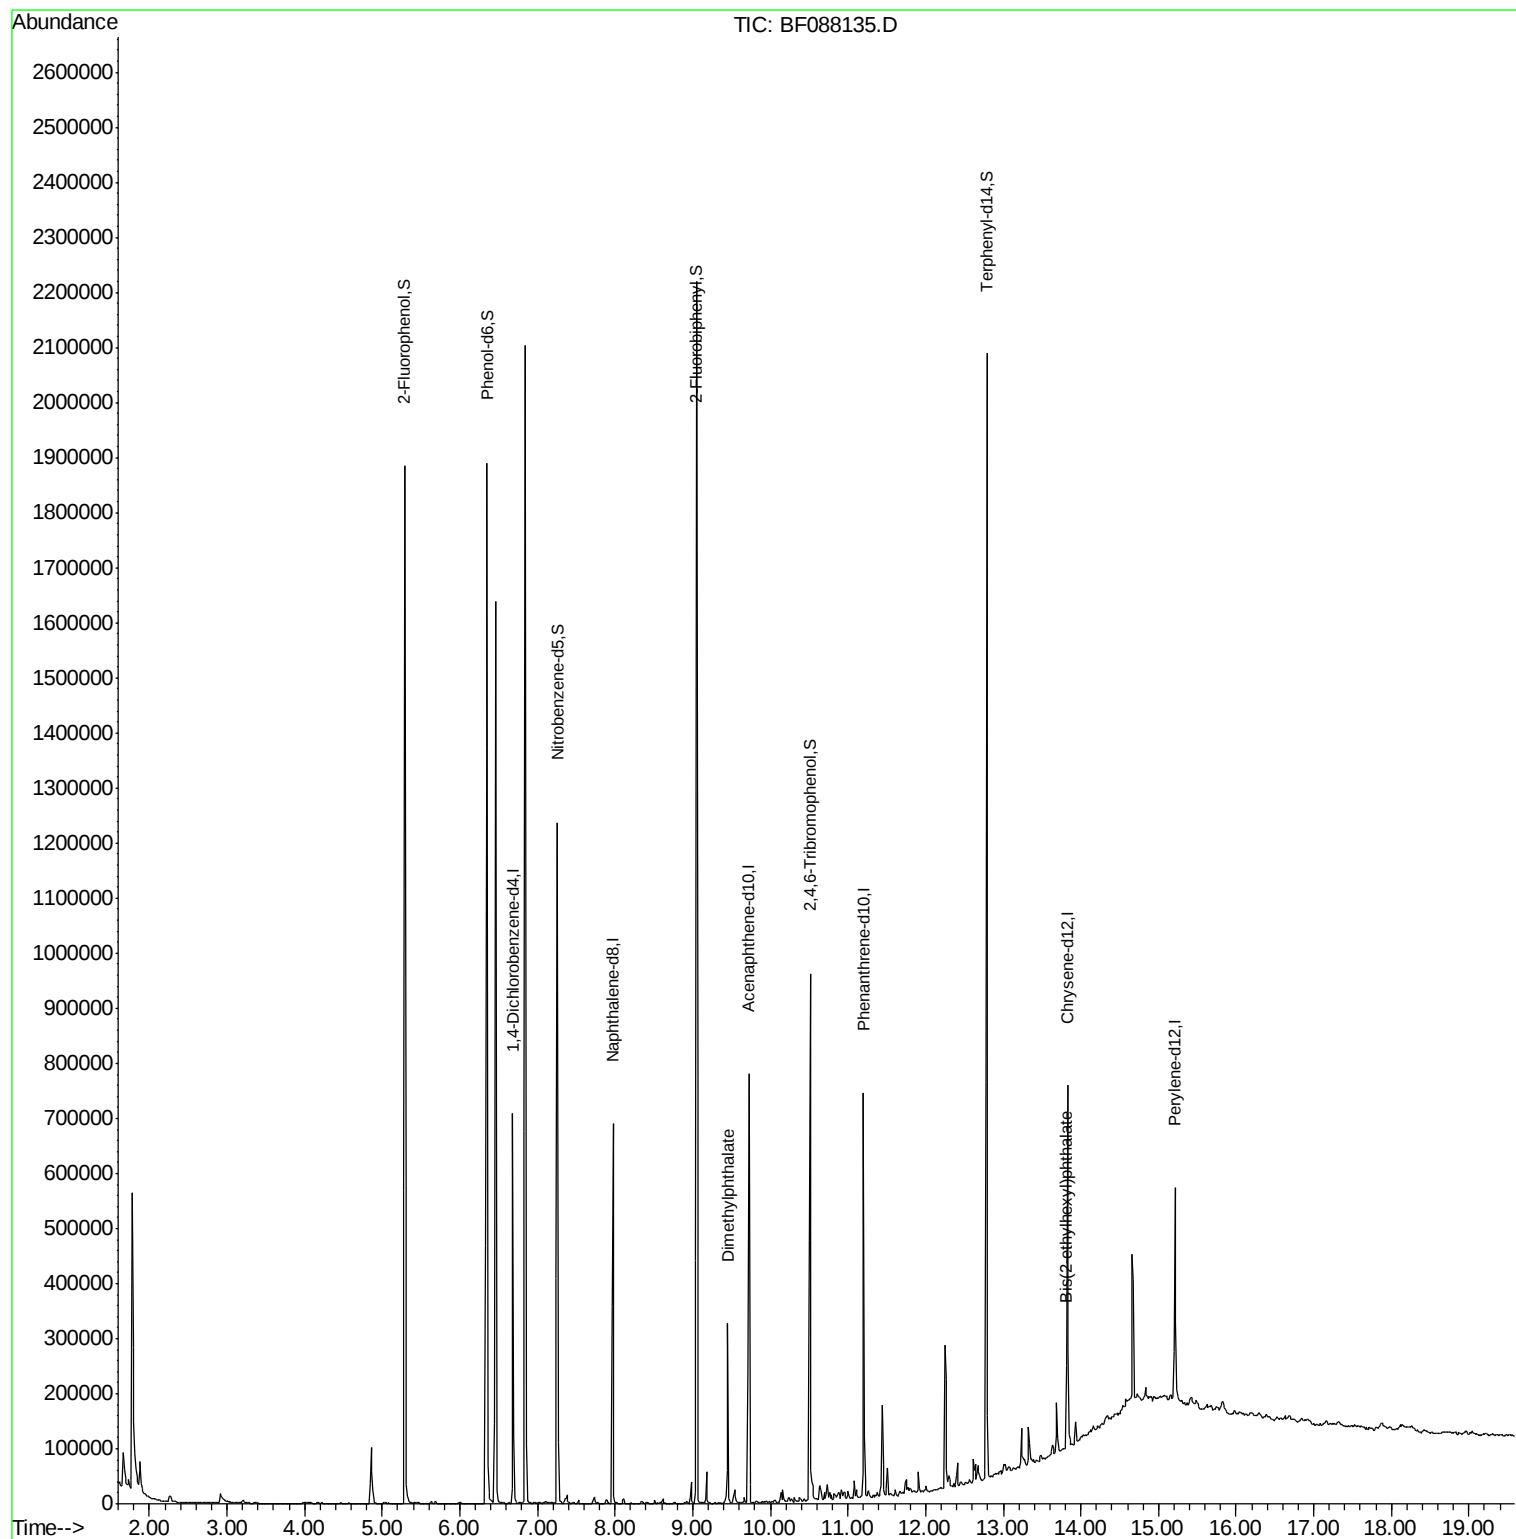

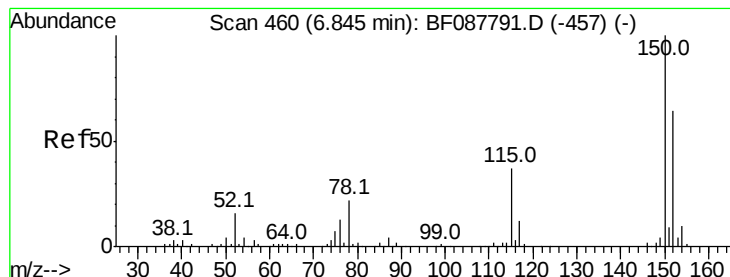

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.68 min Scan# 446

Delta R.T. -0.01 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43

Instrument :

BNA_F

ClientSampleId :

SED2-0-6


Tot Ion:152 Resp: 104446

Ion Ratio Lower Upper

152 100

150 158.0 123.8 185.6




115 63.5 39.6 59.4#

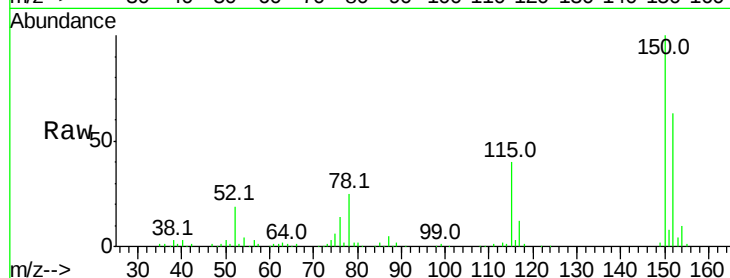

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

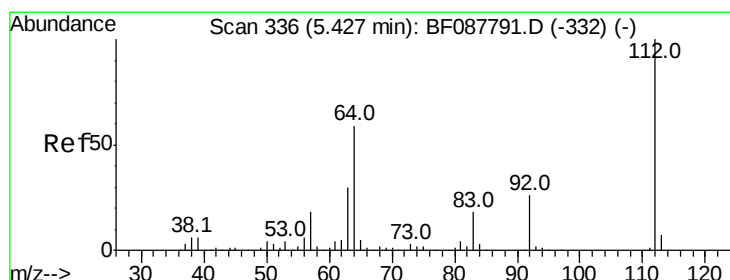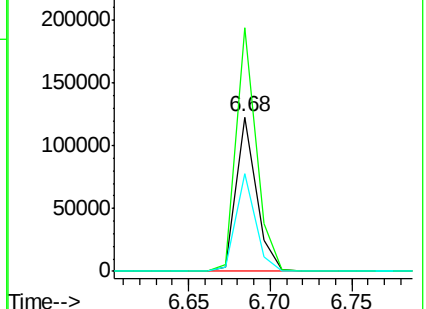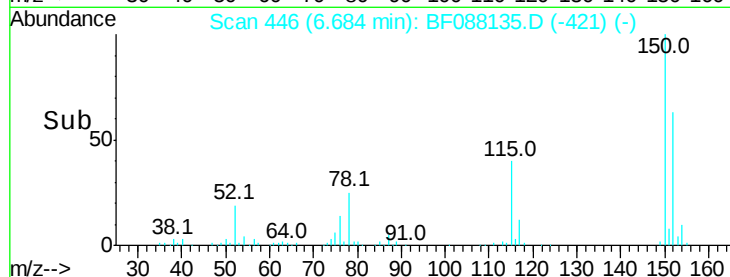

#5

2-Fluorophenol

Concen: 108.98 ng

RT: 5.29 min Scan# 324

Delta R.T. 0.01 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43


Tgt Ion:112 Resp: 665823

Ion Ratio Lower Upper

112 100

64 56.2 42.2 63.2



63 29.1 21.8 32.8

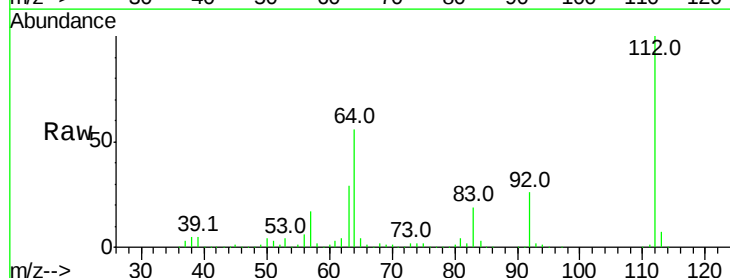

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

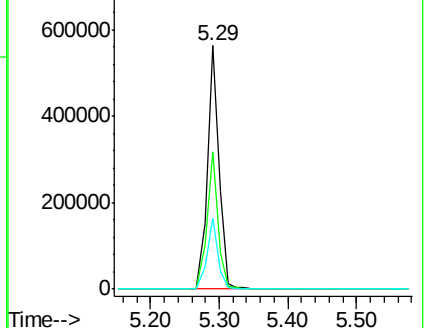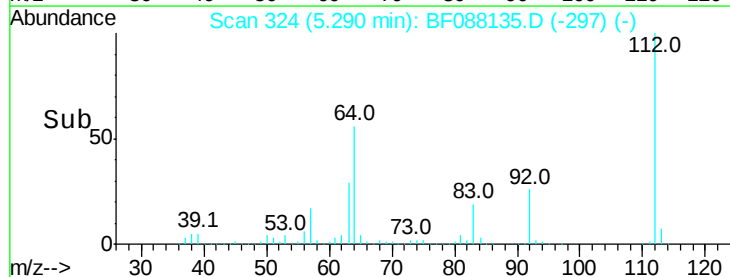



#7

Phenol-d6

Concen: 121.77 ng

RT: 6.35 min Scan# 417

Delta R.T. -0.00 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43

Instrument :

BNA_F

ClientSampleId :

SED2-0-6


Tot Ion: 99 Resp: 901621

Ion Ratio Lower Upper

99 100

42 14.5 12.2 18.2

71 33.4 23.4 35.0

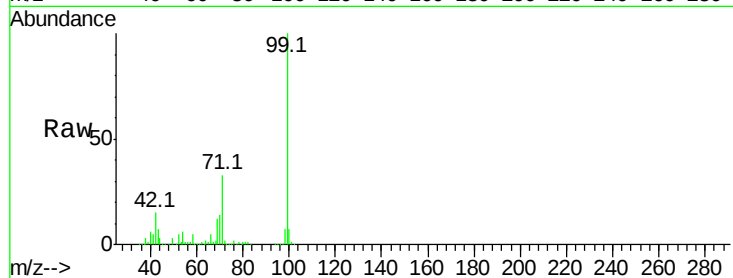

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

1000000

800000

600000



400000

200000

0

6.35

Time-->

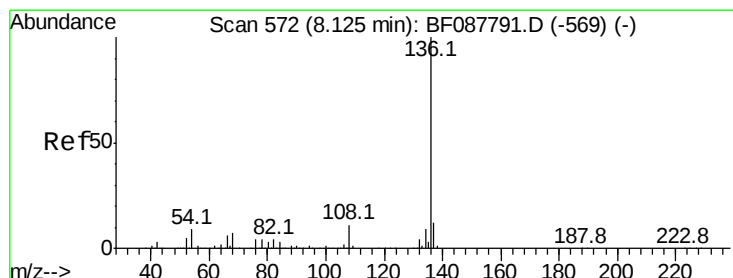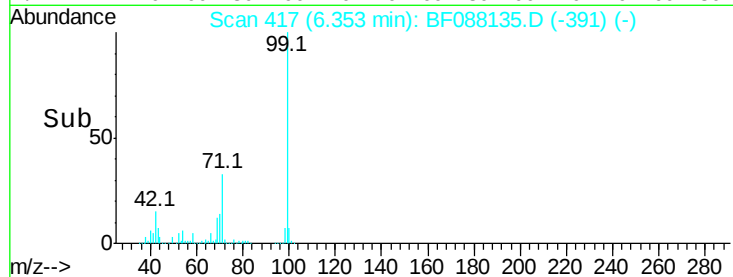

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.98 min Scan# 559

Delta R.T. -0.01 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43

Tgt Ion: 136 Resp: 383519


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 5.1 6.6 10.0#

68 4.5 5.1 7.7#

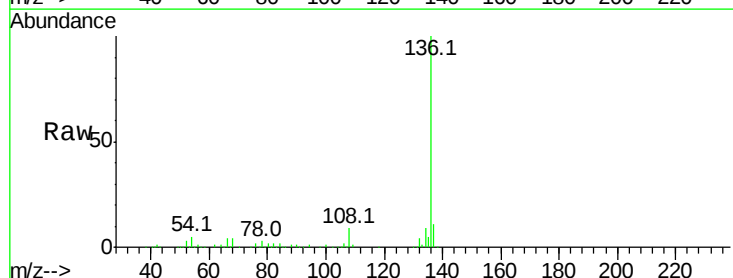

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

600000

500000

400000

300000


200000


100000

0

7.98

Time-->




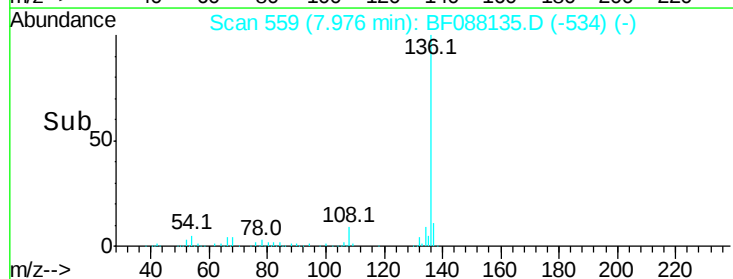


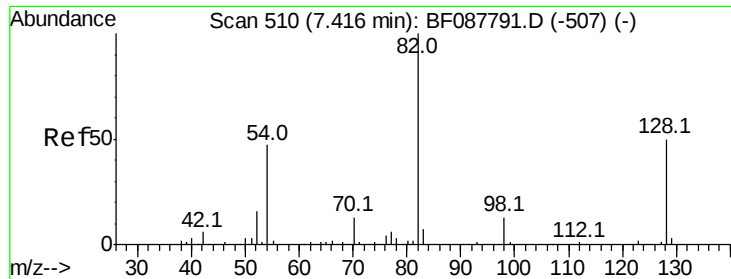

#23
Nitrobenzene-d5
Concen: 65.22 ng
RT: 7.26 min Scan# 496
Delta R.T. -0.02 min
Lab File: BF088135.D
Acq: 18 Jun 2016 15:43




Instrument :
BNA_F
ClientSampleId :
SED2-0-6


Tot Ion	82	Resp	428320
Ion Ratio	Lower	Upper	
82	100		
128	47.7	35.9	53.9
54	46.8	40.9	61.3

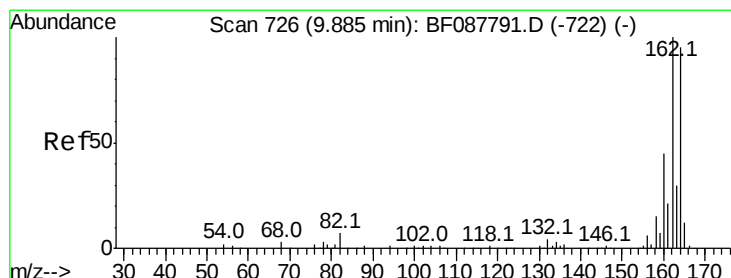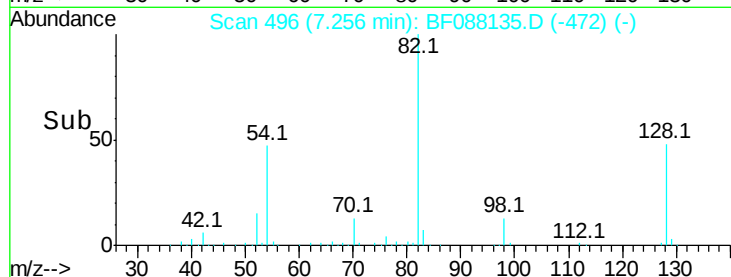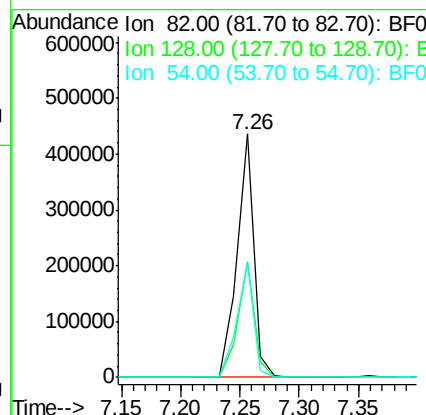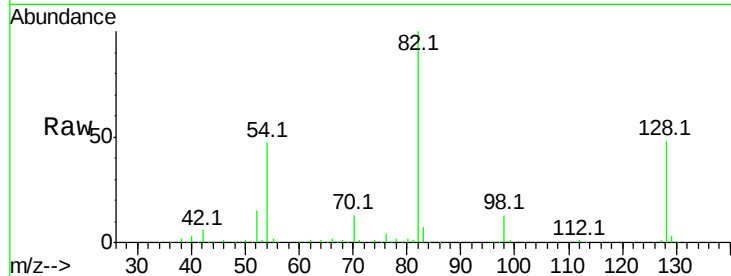

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.72 min Scan# 712
Delta R.T. -0.01 min
Lab File: BF088135.D
Acq: 18 Jun 2016 15:43

Tgt Ion	164	Resp	158743
Ion Ratio	Lower	Upper	
164	100		
162	105.1	85.4	128.2
160	47.7	39.5	59.3

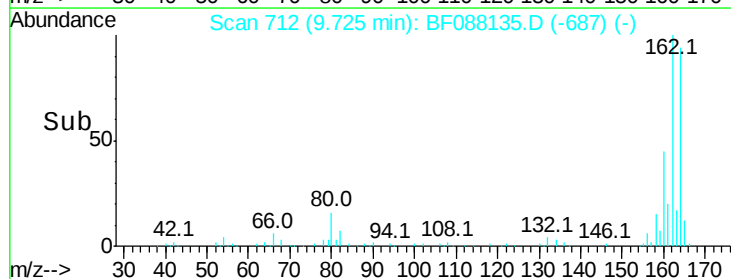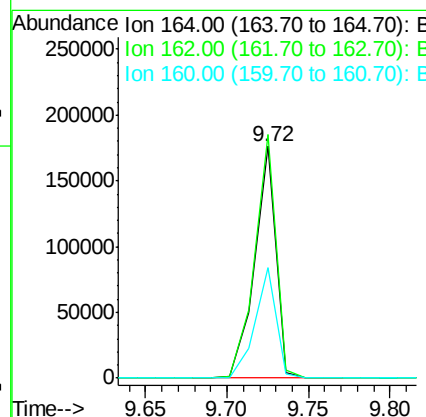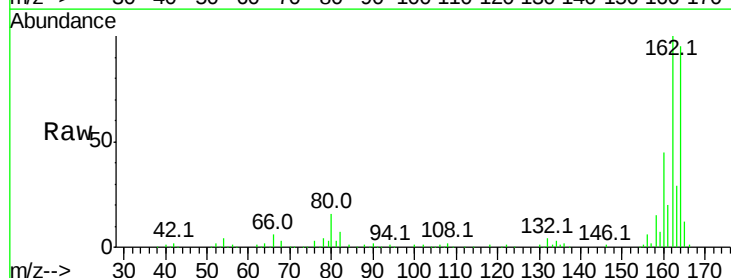


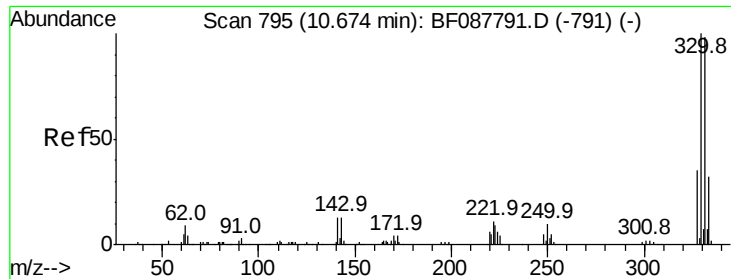




#41
 2,4,6-Tribromophenol
 Concen: 76.00 ng
 RT: 10.51 min Scan# 781
 Delta R.T. -0.01 min
 Lab File: BF088135.D
 Acq: 18 Jun 2016 15:43

Instrument :
 BNA_F
 ClientSampleId :
 SED2-0-6

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	0.0	0.0#
141	39.4	0.0	0.0#

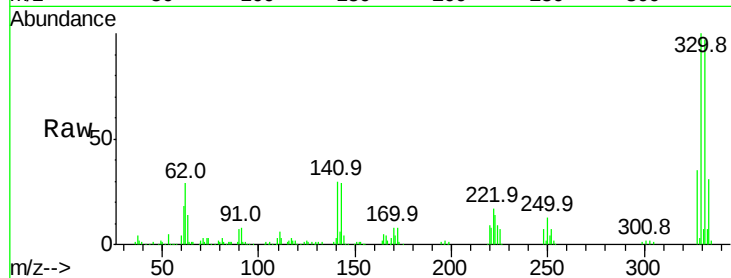


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

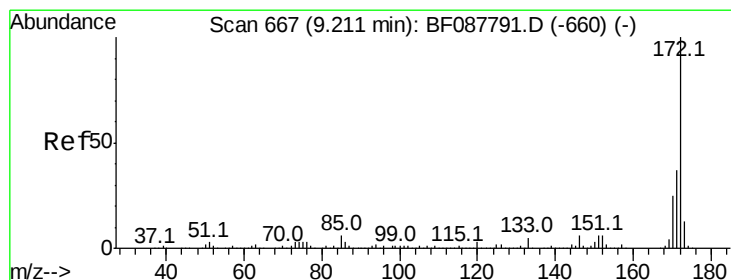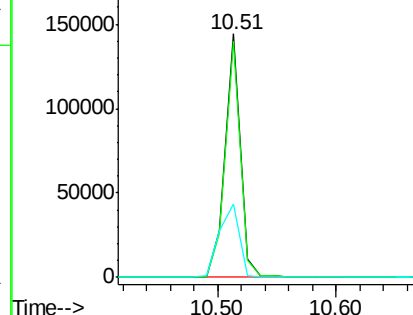
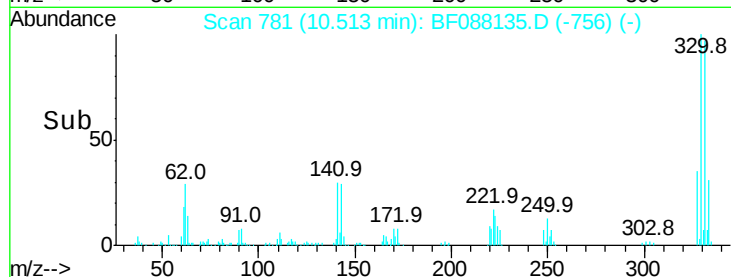



#44
 2-Fluorobiphenyl
 Concen: 82.16 ng
 RT: 9.05 min Scan# 653
 Delta R.T. -0.02 min
 Lab File: BF088135.D
 Acq: 18 Jun 2016 15:43

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.6	43.0
170	23.9	19.2	28.8

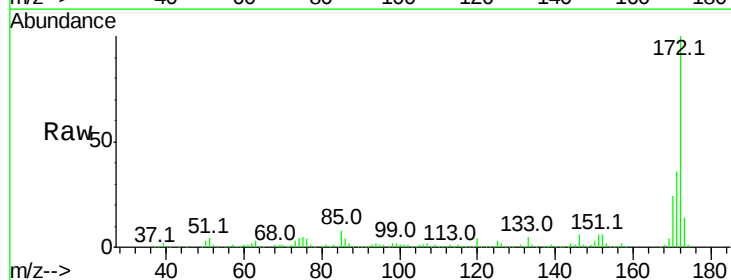

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

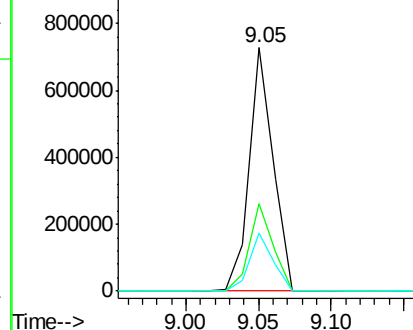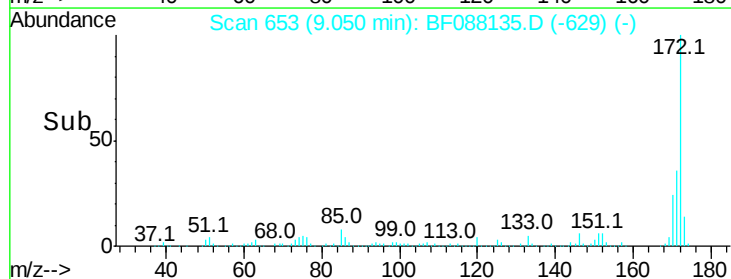

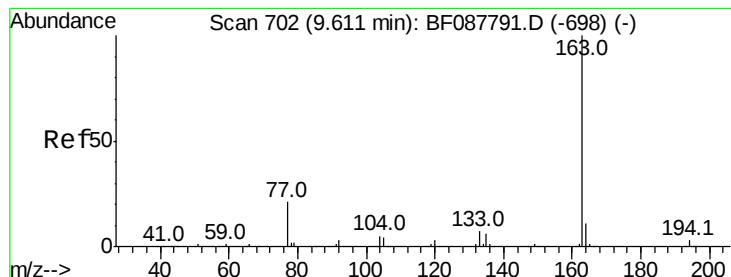

#49

Dimethylphthalate

Concen: 11.75 ng

RT: 9.45 min Scan# 688

Delta R.T. -0.02 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43

Instrument :

BNA_F

ClientSampled :

SED2-0-6


Tot Ion:163 Resp: 135138

Ion Ratio Lower Upper

163 100

194 3.4 2.8 4.2




164 9.8 8.3 12.5

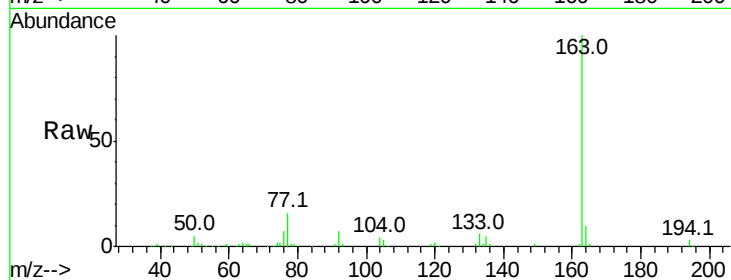

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

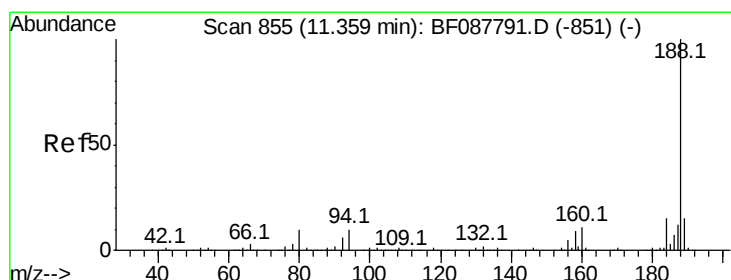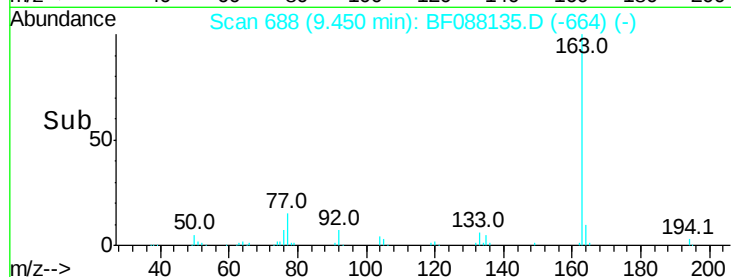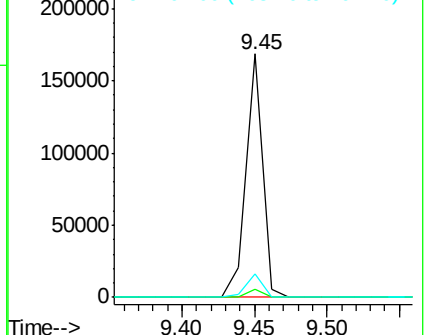

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.20 min Scan# 841

Delta R.T. -0.01 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43


Tgt Ion:188 Resp: 246949

Ion Ratio Lower Upper

188 100

94 10.9 9.0 13.6



80 11.2 10.0 15.0

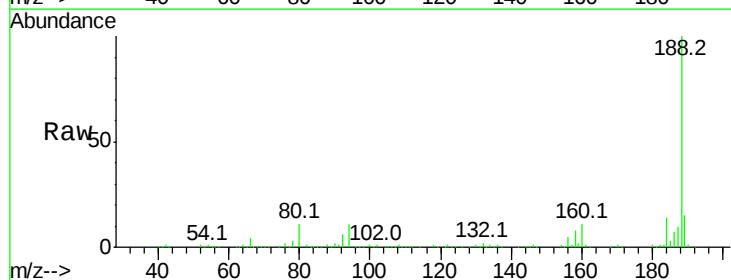


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

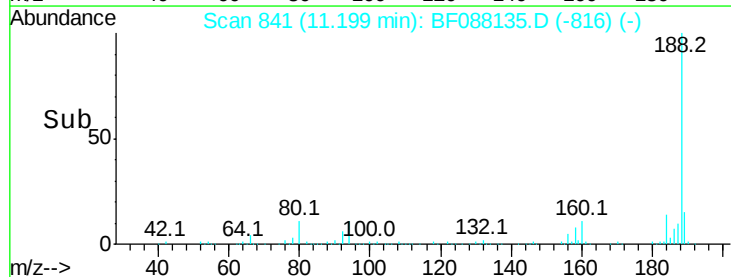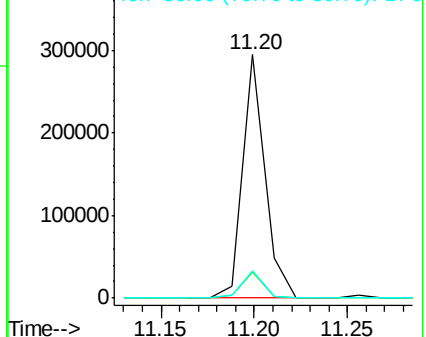

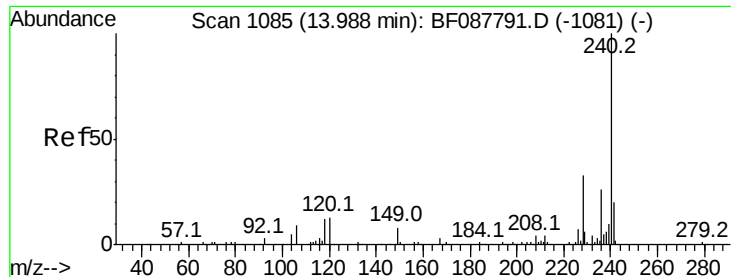

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.83 min Scan# 1071

Delta R.T. -0.02 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43

Instrument :

BNA_F

ClientSampleId :

SED2-0-6


Tot Ion:240 Resp: 204184

Ion Ratio Lower Upper

240 100

120 15.1 6.8 10.2#




236 25.7 20.2 30.2

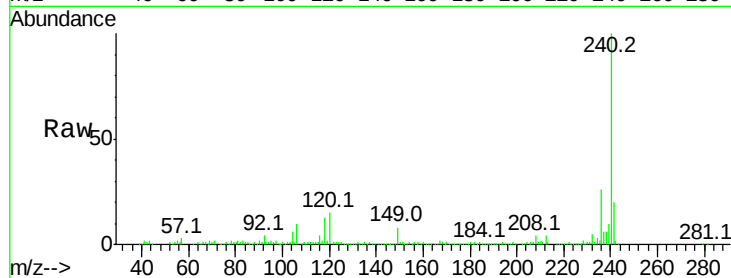

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

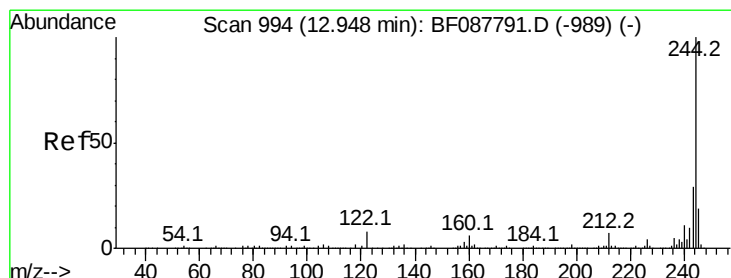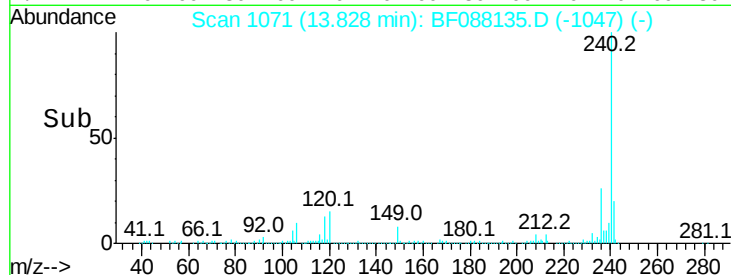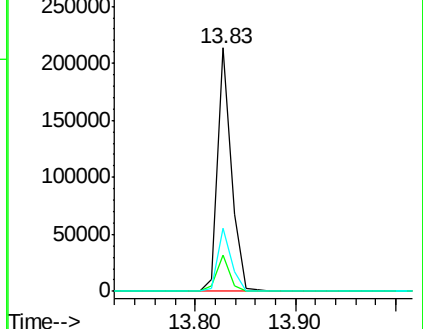

#78

Terphenyl-d14

Concen: 71.73 ng

RT: 12.79 min Scan# 980

Delta R.T. -0.01 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43


Tgt Ion:244 Resp: 643648

Ion Ratio Lower Upper

244 100

212 7.5 6.0 9.0



122 12.9 11.2 16.8

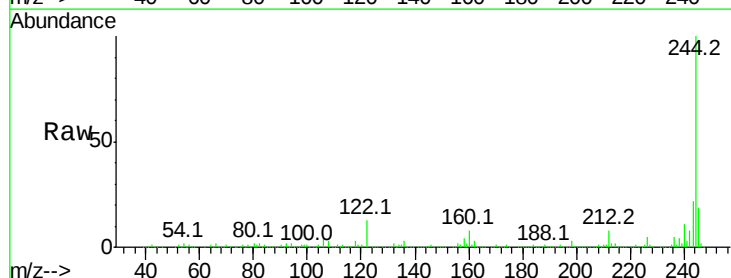


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

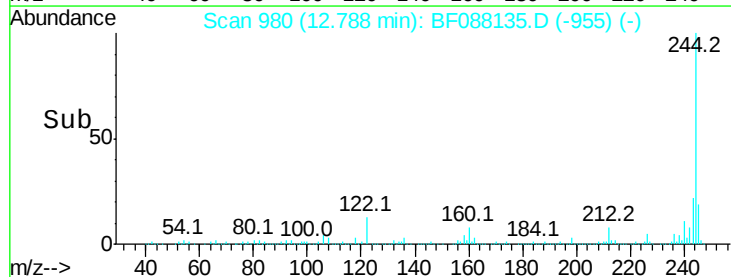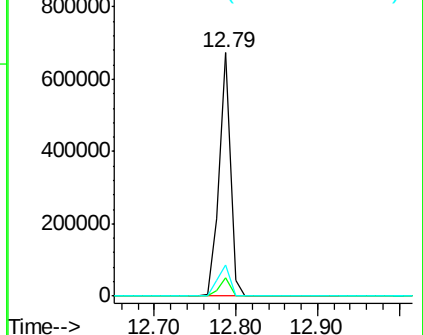

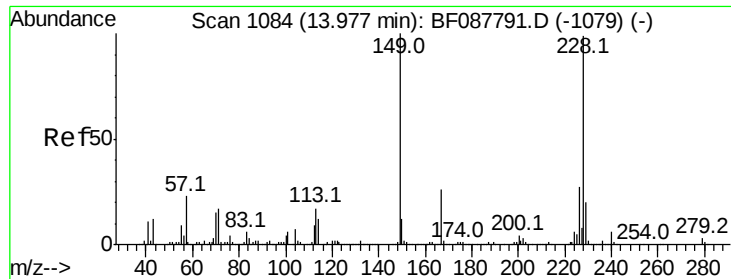

#83

Bis(2-ethylhexyl)phthalate

Concen: 3.43 ng

RT: 13.82 min Scan# 1070

Delta R.T. -0.02 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43

Instrument :

BNA_F

ClientSampleId :

SED2-0-6


Tot Ion:149 Resp: 27956

Ion Ratio Lower Upper




149 100

167 25.3 20.5 30.7

279 2.4 2.0 3.0

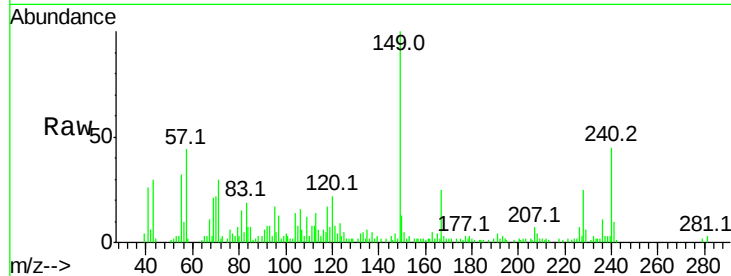

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

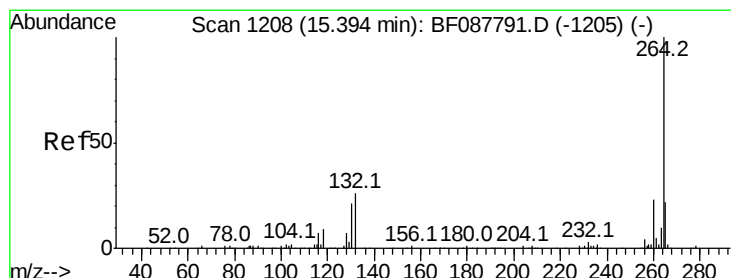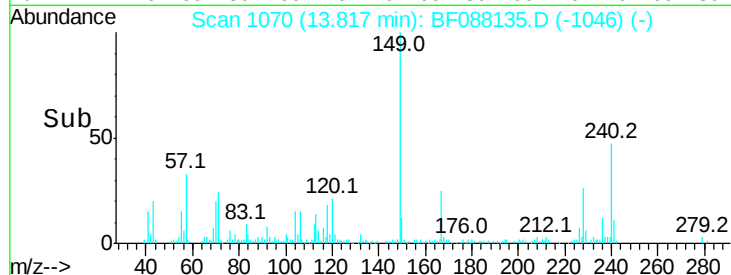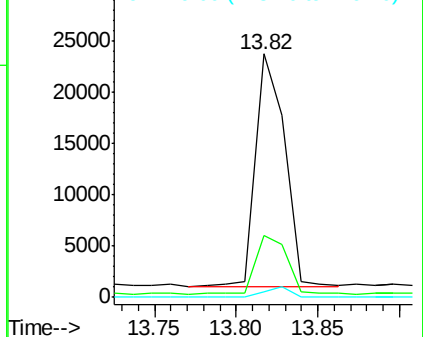

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.21 min Scan# 1192

Delta R.T. -0.01 min

Lab File: BF088135.D

Acq: 18 Jun 2016 15:43


Tgt Ion:264 Resp: 159840

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 21.7 16.9 25.3

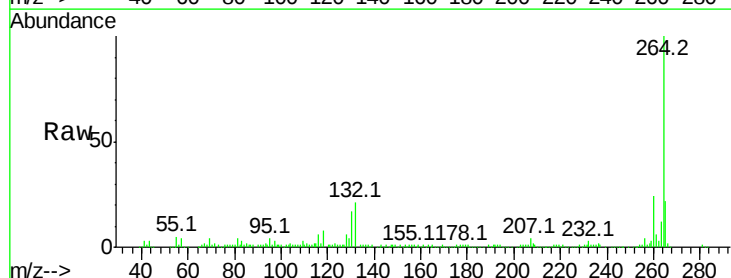

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

