

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061816\
 Data File : BF088146.D
 Acq On : 18 Jun 2016 21:01
 Operator : UM/SJ
 Sample : H3580-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 08-B5(0-8)C

Quant Time: Jun 20 05:51:01 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 17 16:09:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	94869	20.00	ng	-0.01
21) Naphthalene-d8	7.98	136	338138	20.00	ng	-0.01
38) Acenaphthene-d10	9.72	164	135306	20.00	ng	-0.01
63) Phenanthrene-d10	11.20	188	213867	20.00	ng	-0.01
75) Chrysene-d12	13.83	240	177871	20.00	ng	-0.02
86) Perylene-d12	15.21	264	135175	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	601759	108.44	ng	0.01
7) Phenol-d6	6.34	99	638958	95.01	ng	-0.01
23) Nitrobenzene-d5	7.26	82	395714	68.34	ng	-0.02
41) 2,4,6-Tribromophenol	10.51	330	103472	72.42	ng	-0.01
44) 2-Fluorobiphenyl	9.05	172	633952	72.81	ng	-0.02
78) Terphenyl-d14	12.79	244	479246	61.31	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.45	163	256338	26.15	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061816\
Data File : BF088146.D
Acq On : 18 Jun 2016 21:01
Operator : UM/SJ
Sample : H3580-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
08-B5(0-8)C

Quant Time: Jun 20 05:51:01 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 17 16:09:13 2016
Response via : Initial Calibration

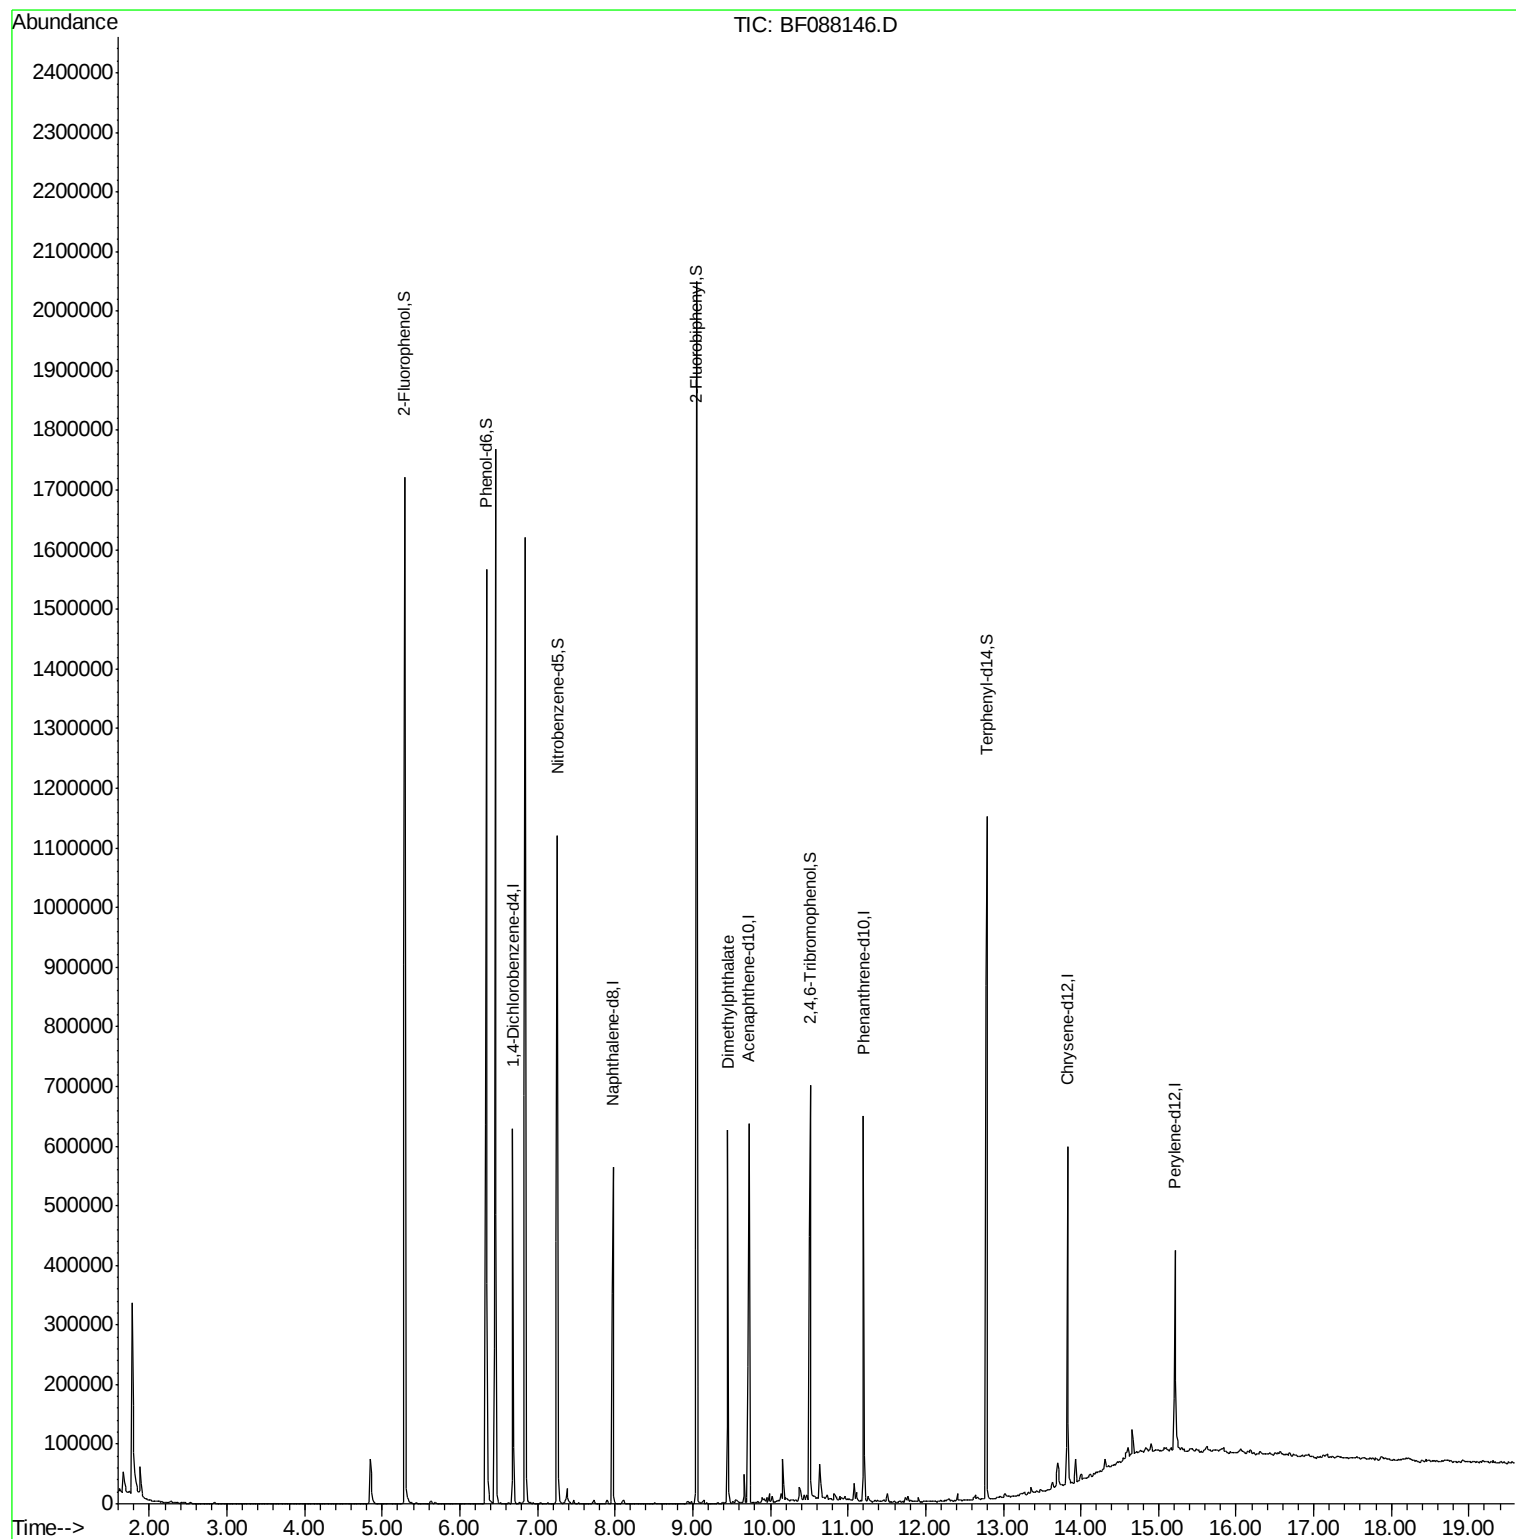

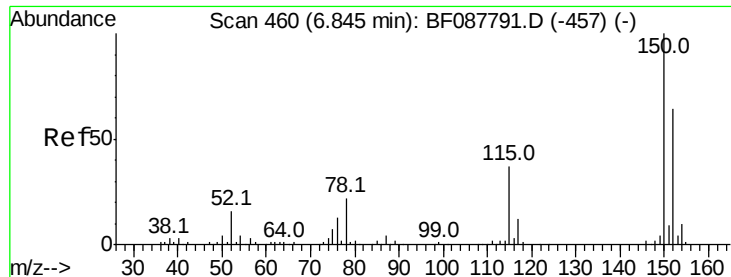

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.68 min Scan# 446

Delta R.T. -0.01 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01

Instrument :

BNA_F

ClientSampleId :

08-B5(0-8)C


Tot Ion:152 Resp: 94869

Ion Ratio Lower Upper

152 100

150 155.1 123.8 185.6




115 60.0 39.6 59.4#

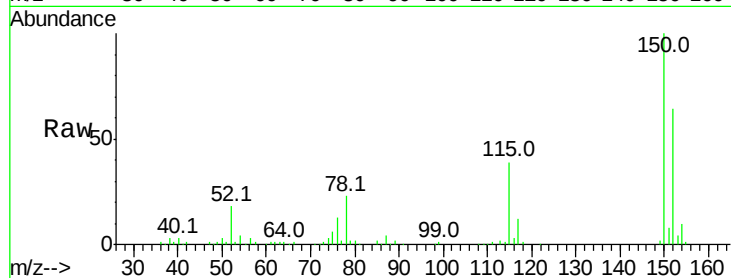

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

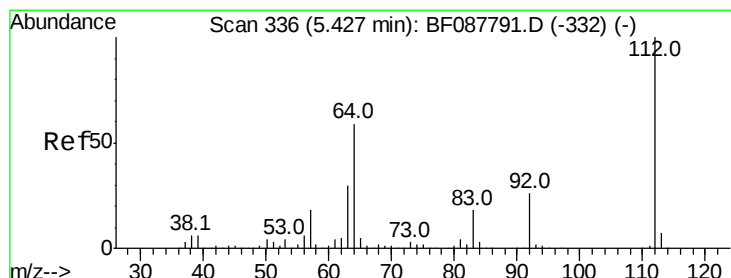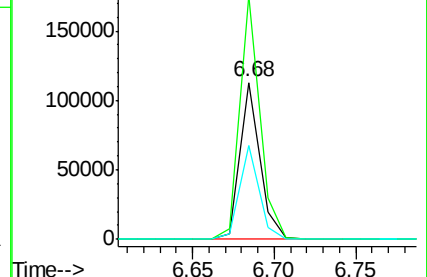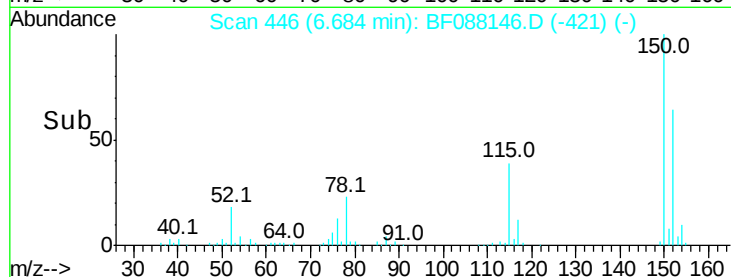

#5

2-Fluorophenol

Concen: 108.44 ng

RT: 5.29 min Scan# 324

Delta R.T. 0.01 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01


Tgt Ion:112 Resp: 601759

Ion Ratio Lower Upper

112 100

64 51.2 42.2 63.2



63 26.5 21.8 32.8

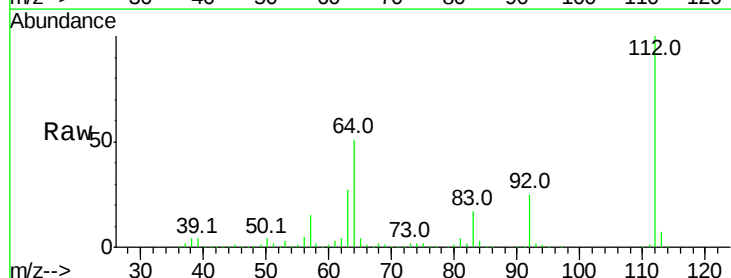

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

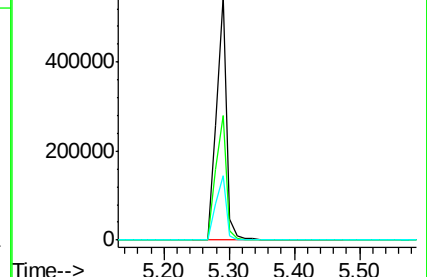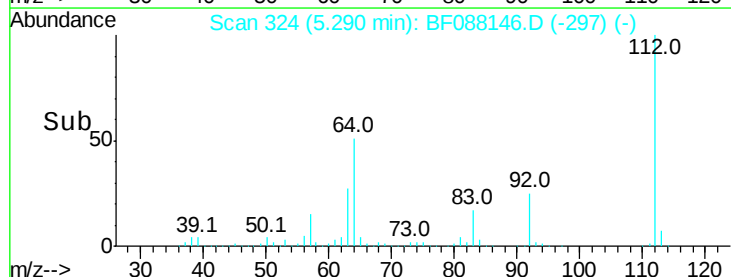



#7

Phenol-d6

Concen: 95.01 ng

RT: 6.34 min Scan# 416

Delta R.T. -0.01 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01

Instrument :

BNA_F

ClientSampleId :

08-B5(0-8)C


Tot Ion: 99 Resp: 638958

Ion Ratio Lower Upper


99 100

42 15.9 12.2 18.2



71 34.1 23.4 35.0

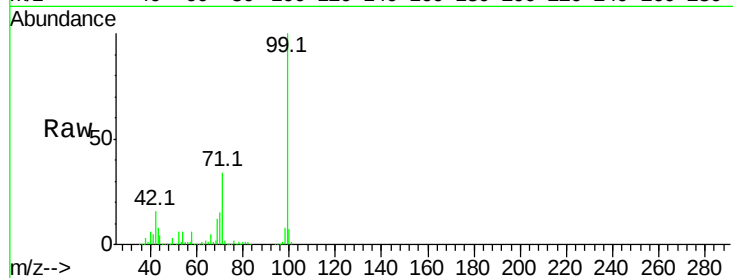

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

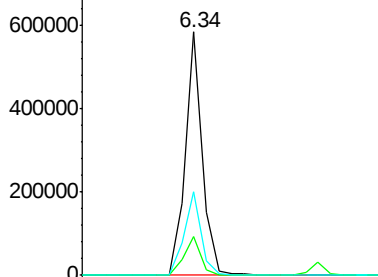

Time-->

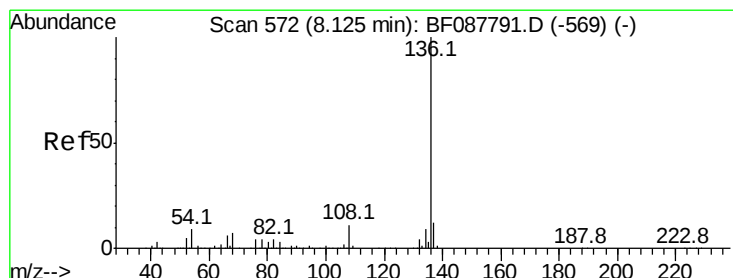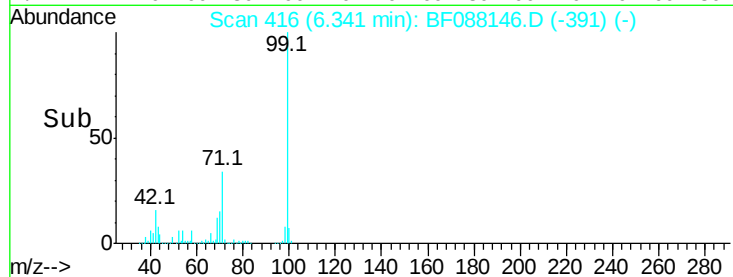

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.98 min Scan# 559

Delta R.T. -0.01 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01

Tgt Ion: 136 Resp: 338138


Ion Ratio Lower Upper

136 100


137 10.5 9.1 13.7

54 5.0 6.6 10.0#


68 4.5 5.1 7.7#

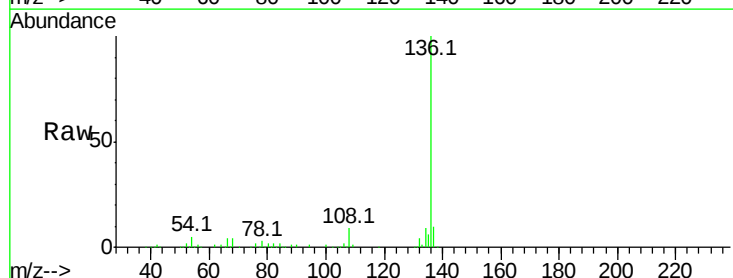


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

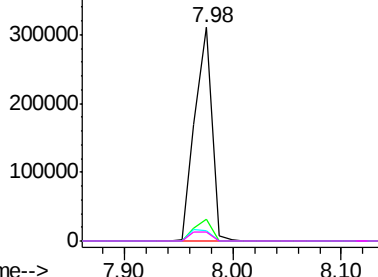

Time-->




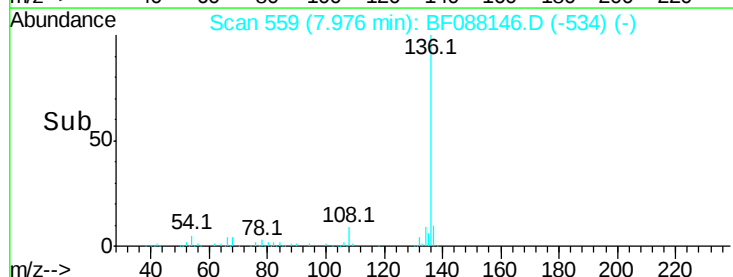


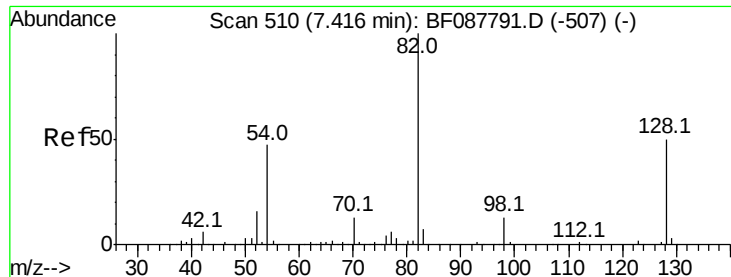

#23
 Nitrobenzene-d5
 Concen: 68.34 ng
 RT: 7.26 min Scan# 496
 Delta R.T. -0.02 min
 Lab File: BF088146.D
 Acq: 18 Jun 2016 21:01




Instrument :
 BNA_F
 ClientSampleId :
 08-B5(0-8)C


Tot Ion: 82 Resp: 395714
 Ion Ratio Lower Upper
 82 100
 128 48.7 35.9 53.9
 54 44.8 40.9 61.3

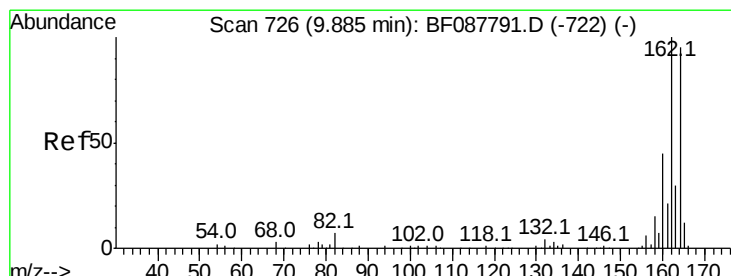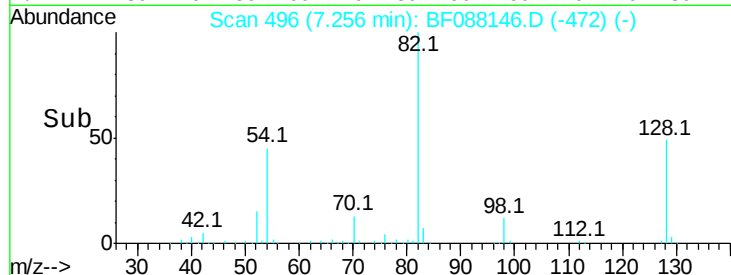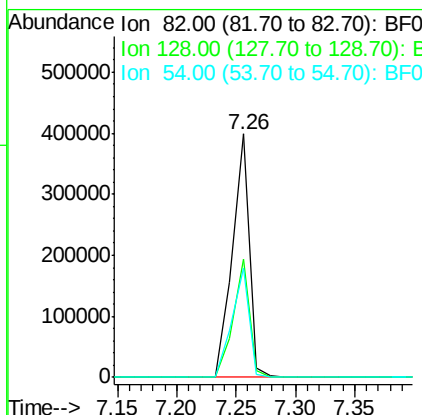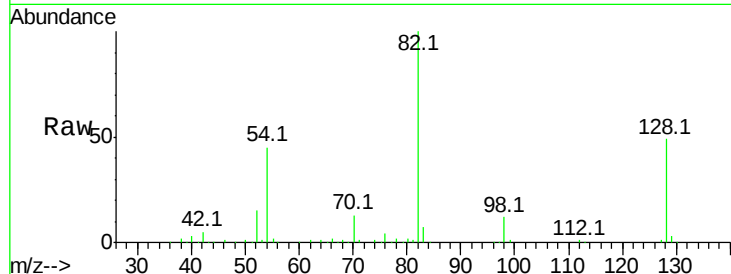

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.72 min Scan# 712
 Delta R.T. -0.01 min
 Lab File: BF088146.D
 Acq: 18 Jun 2016 21:01

Tgt Ion:164 Resp: 135306
 Ion Ratio Lower Upper
 164 100
 162 104.6 85.4 128.2
 160 47.2 39.5 59.3

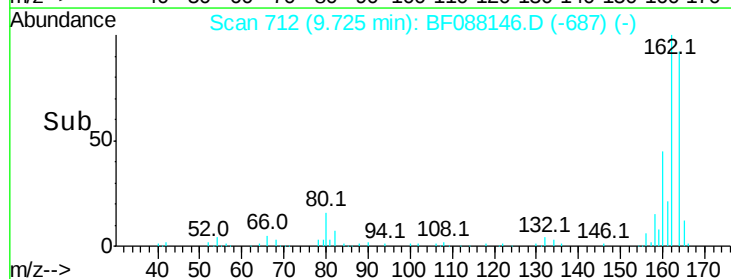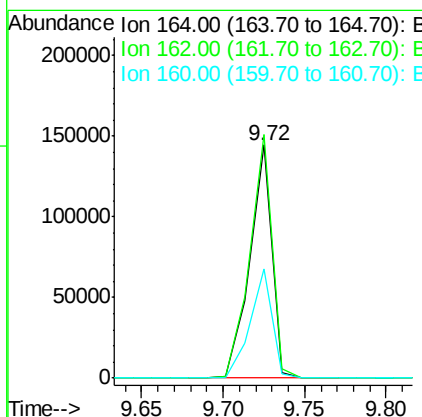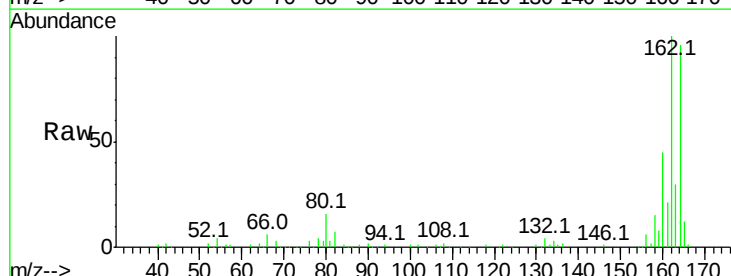


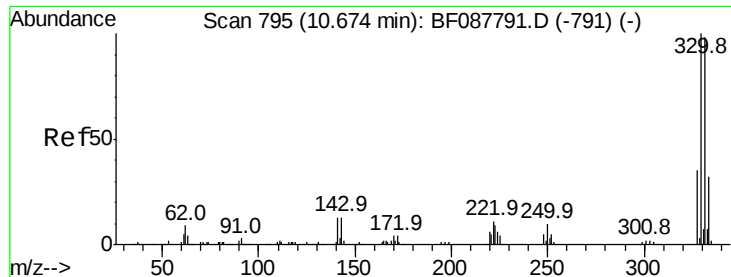




#41
 2,4,6-Tribromophenol
 Concen: 72.42 ng
 RT: 10.51 min Scan# 781
 Delta R.T. -0.01 min
 Lab File: BF088146.D
 Acq: 18 Jun 2016 21:01

Instrument :
 BNA_F
 ClientSampleId :
 08-B5(0-8)C

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	0.0	0.0#
141	37.5	0.0	0.0#

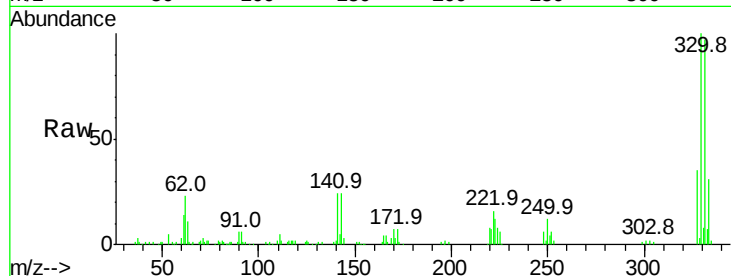


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

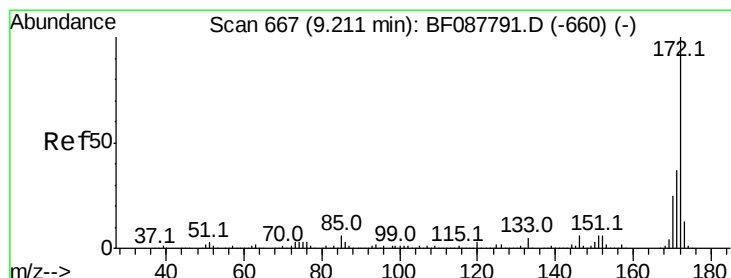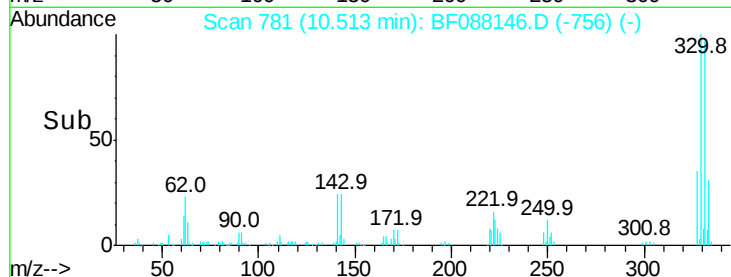
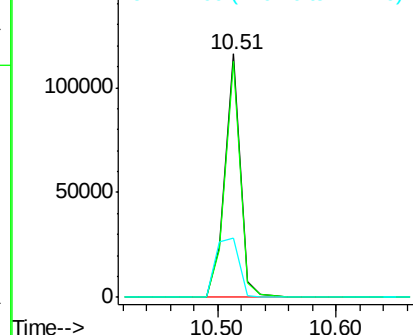



#44
 2-Fluorobiphenyl
 Concen: 72.81 ng
 RT: 9.05 min Scan# 653
 Delta R.T. -0.02 min
 Lab File: BF088146.D
 Acq: 18 Jun 2016 21:01

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	28.6	43.0
170	24.2	19.2	28.8

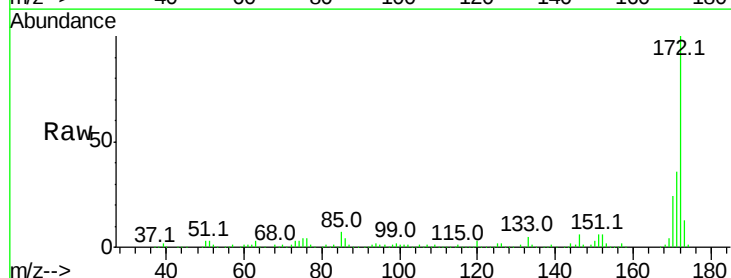

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

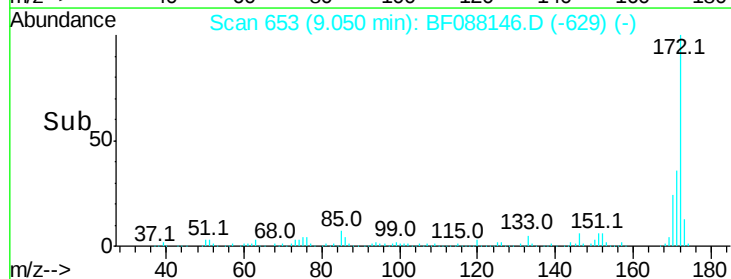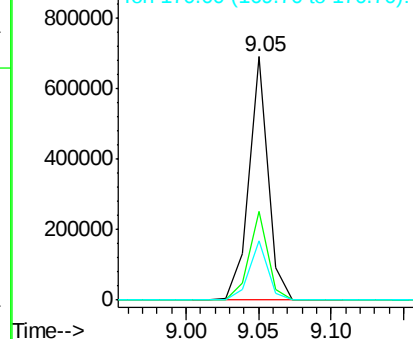

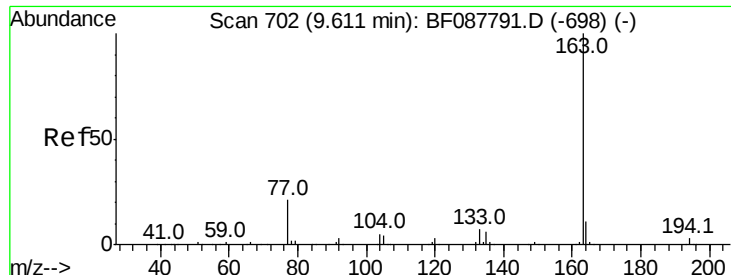

#49

Dimethylphthalate

Concen: 26.15 ng

RT: 9.45 min Scan# 688

Delta R.T. -0.02 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01

Instrument :

BNA_F

ClientSampleId :

08-B5(0-8)C


Tot Ion:163 Resp: 256338

Ion Ratio Lower Upper

163 100

194 3.3 2.8 4.2




164 10.0 8.3 12.5

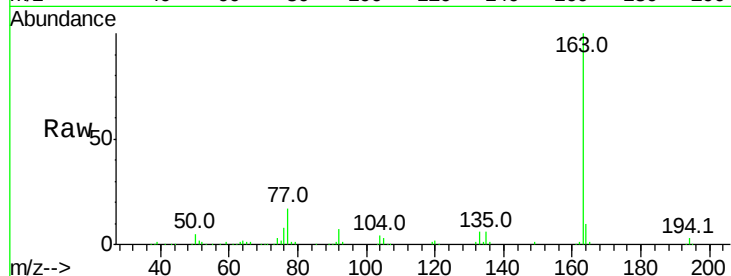

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

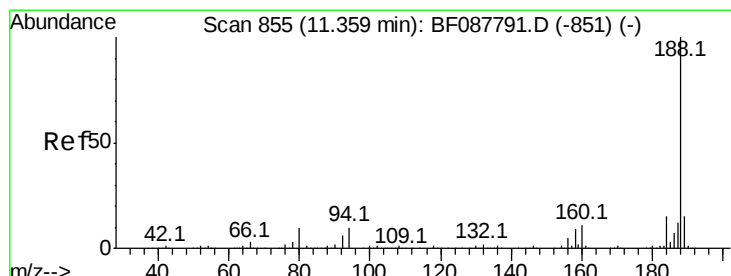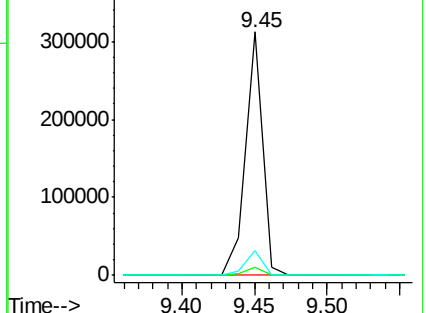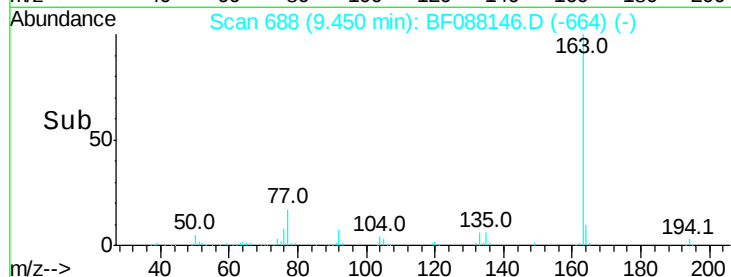

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.20 min Scan# 841

Delta R.T. -0.01 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01


Tgt Ion:188 Resp: 213867

Ion Ratio Lower Upper

188 100

94 10.5 9.0 13.6



80 11.0 10.0 15.0

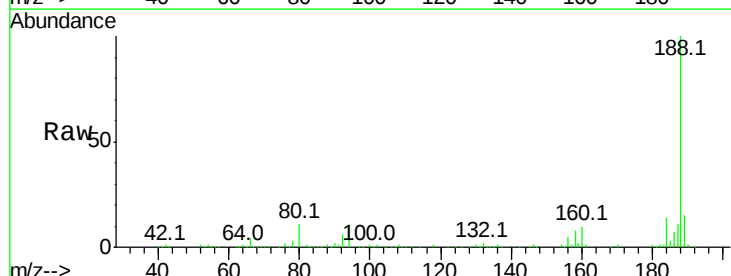


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

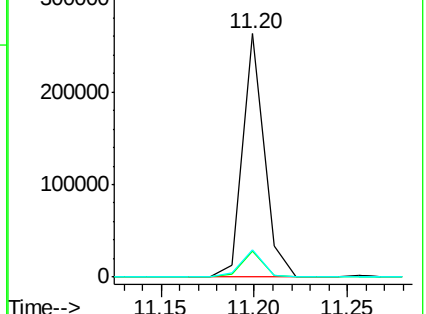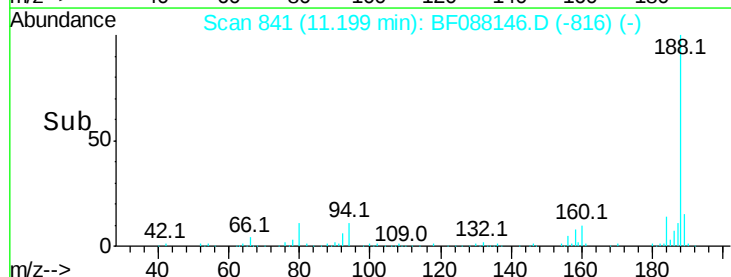

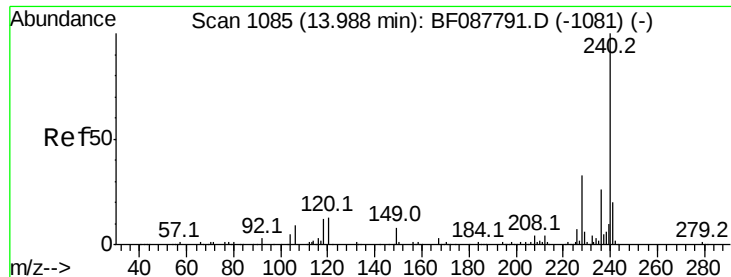

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.83 min Scan# 1071

Delta R.T. -0.02 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01

Instrument :

BNA_F

ClientSampleId :

08-B5(0-8)C


Tot Ion:240 Resp: 177871

Ion Ratio Lower Upper

240 100

120 13.9 6.8 10.2#




236 25.4 20.2 30.2

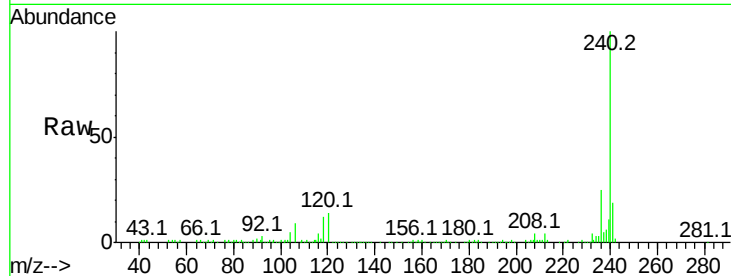

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

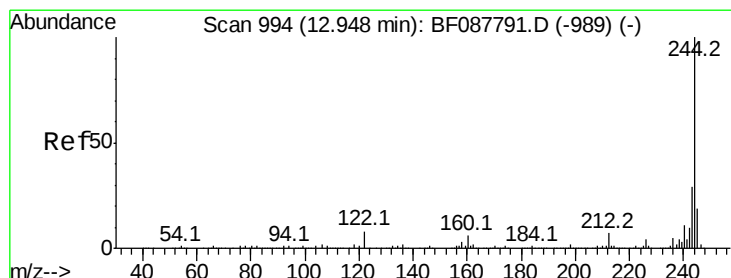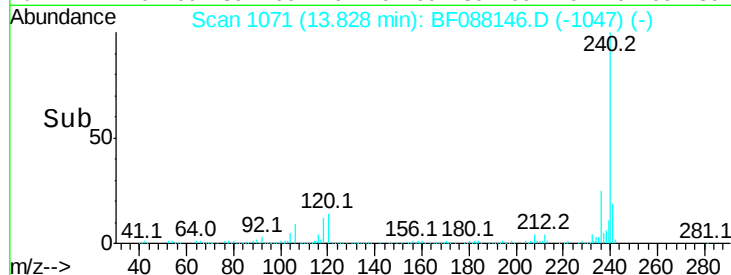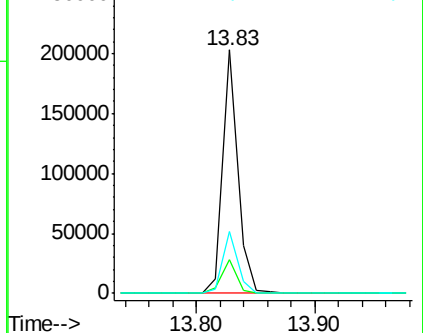

#78

Terphenyl-d14

Concen: 61.31 ng

RT: 12.79 min Scan# 980

Delta R.T. -0.01 min

Lab File: BF088146.D

Acq: 18 Jun 2016 21:01


Tgt Ion:244 Resp: 479246

Ion Ratio Lower Upper

244 100

212 6.4 6.0 9.0



122 8.3 11.2 16.8#

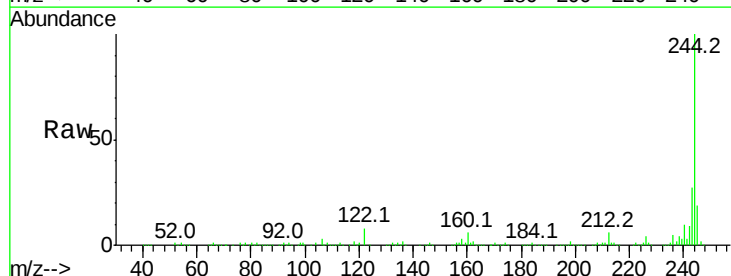


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

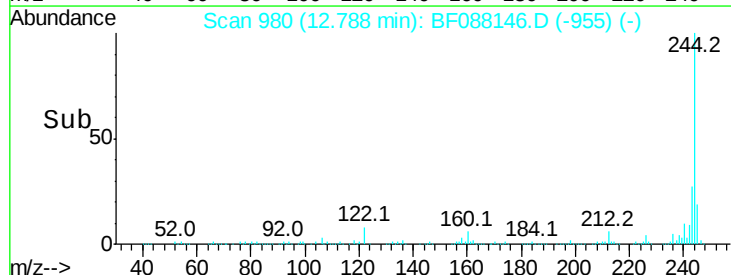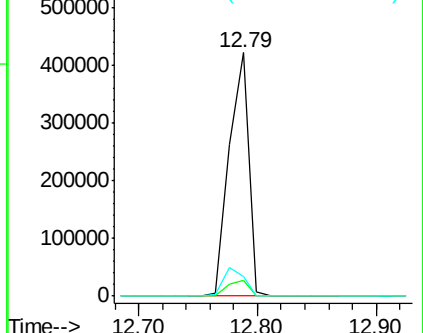


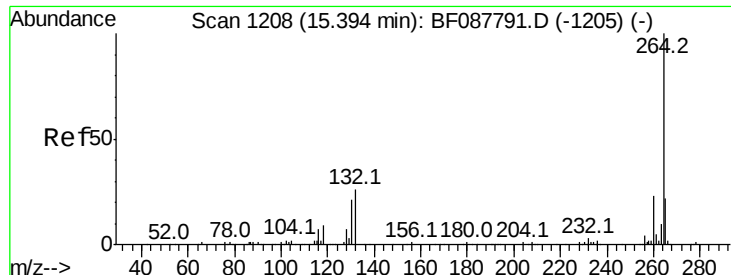

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.21 min Scan# 1192
Delta R.T. -0.01 min
Lab File: BF088146.D
Acq: 18 Jun 2016 21:01

Instrument :
BNA_F
ClientSampleId :
08-B5(0-8)C

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.2	28.8
265	21.2	16.9	25.3

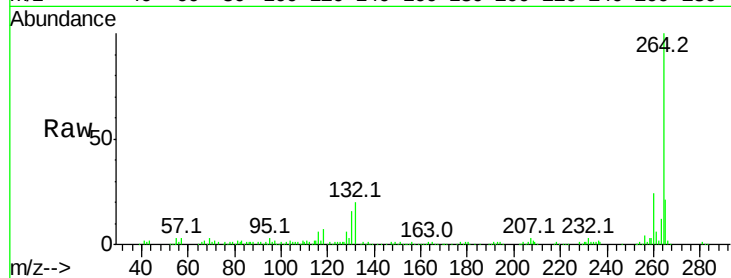

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

