


Data Path : Z:\HPCHEM1\BNA F\Data\BF061816\
 Data File : BF088126.D
 Acq On : 18 Jun 2016 10:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 17 16:09:13 2016

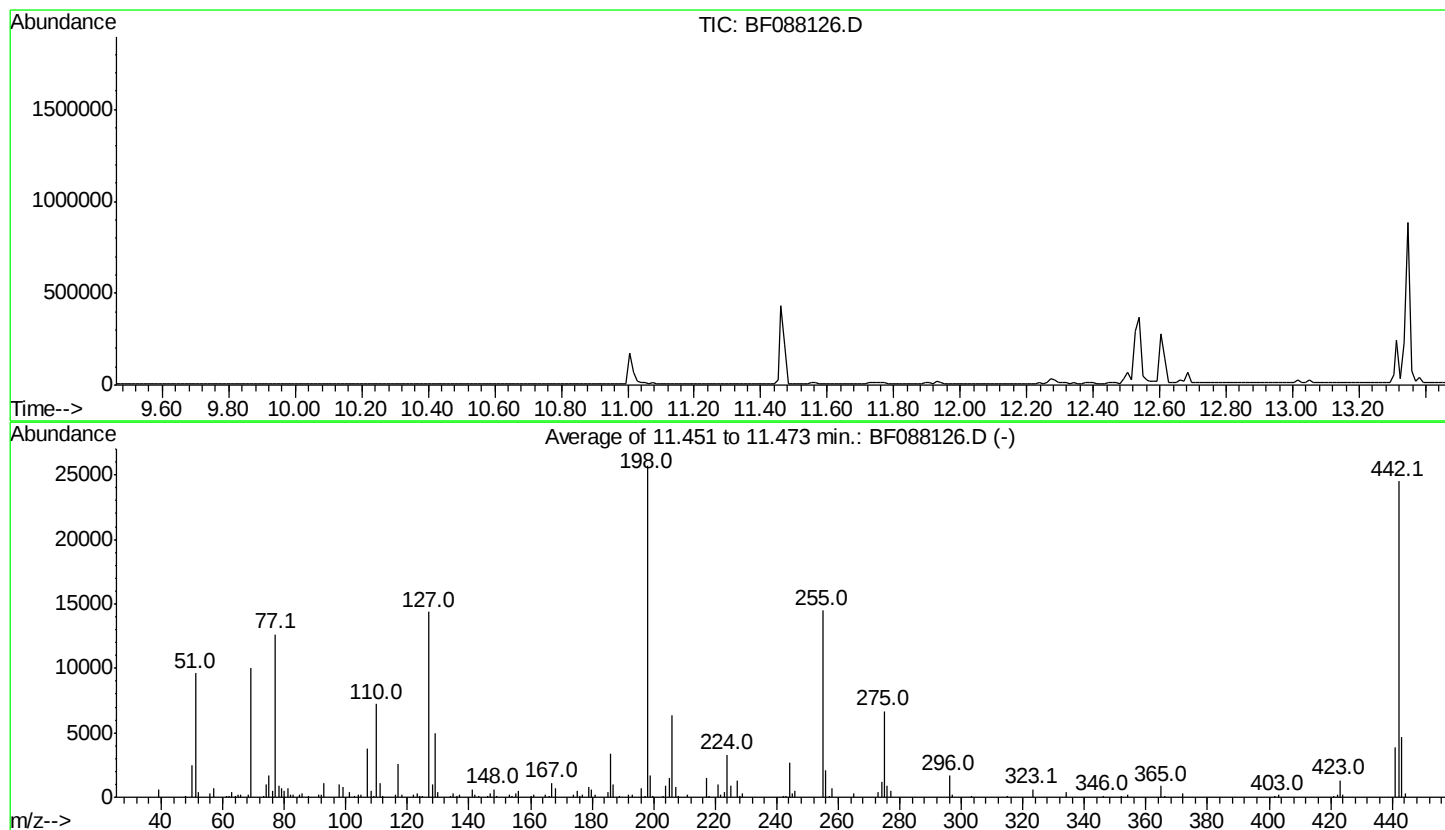

AutoFind: Scans 863, 864, 865; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	9604	PASS
68	69	0.00	2	1.5	154	PASS
69	198	0.00	100	39.2	10074	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.9	14369	PASS
197	198	0.00	2	0.5	119	PASS
198	198	100	100	100.0	25724	PASS
199	198	5	9	6.7	1713	PASS
275	198	10	60	26.0	6678	PASS
365	198	1	100	3.3	849	PASS
441	442	0.01	24	15.8	3861	PASS
442	198	50	100	95.3	24510	PASS
443	442	15	24	19.0	4654	PASS