


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061816\
 Data File : BF088149.D
 Acq On : 18 Jun 2016 22:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 17 16:09:13 2016

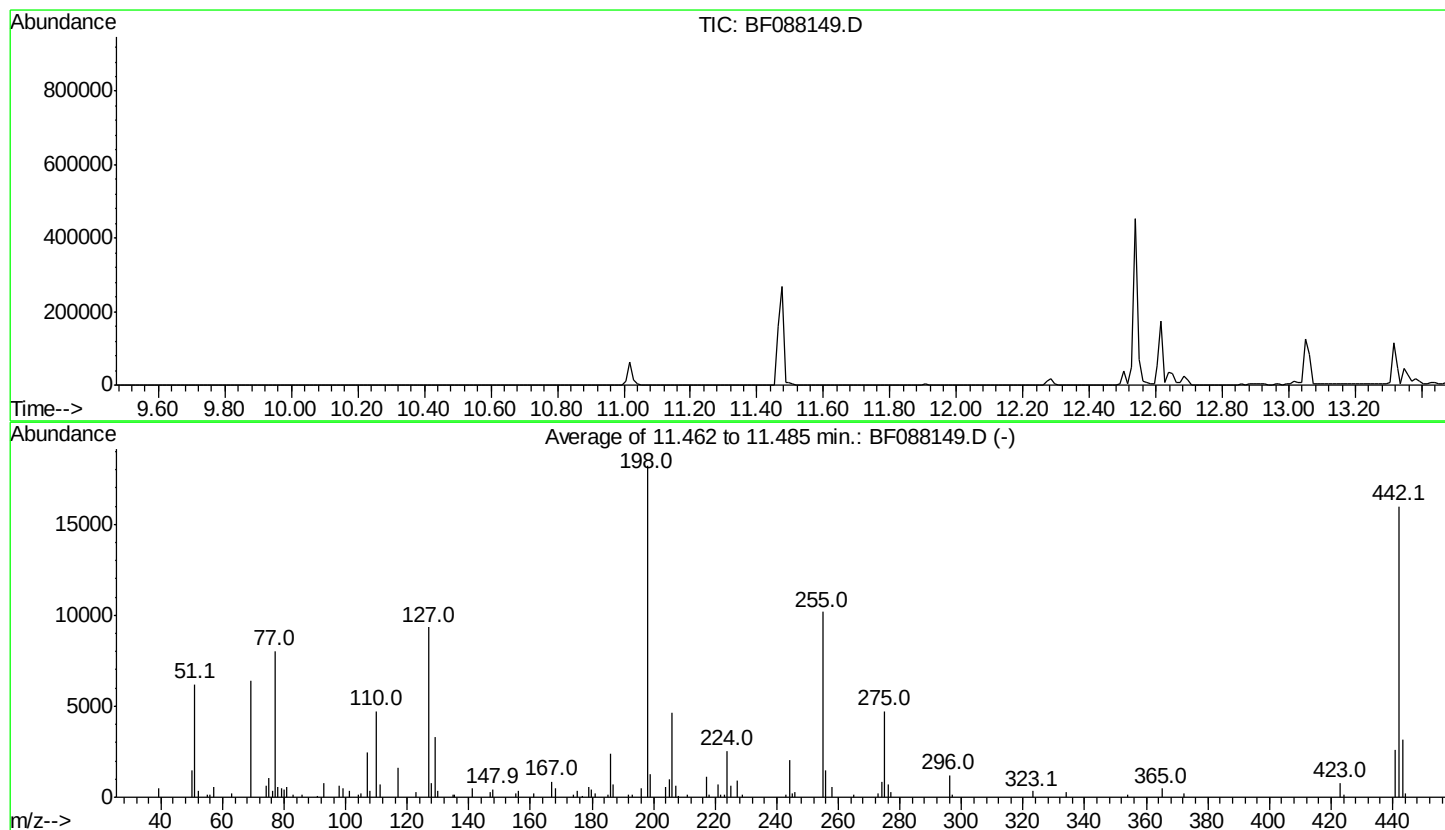

AutoFind: Scans 864, 865, 866; Background Corrected with Scan 861

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	6204	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.0	6370	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	9348	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18218	PASS
199	198	5	9	6.9	1263	PASS
275	198	10	60	25.9	4712	PASS
365	198	1	100	2.6	474	PASS
441	442	0.01	24	16.2	2585	PASS
442	198	50	100	87.8	16001	PASS
443	442	15	24	19.8	3174	PASS