

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061818\
 Data File : BF106548.D
 Acq On : 18 Jun 2018 19:36
 Operator : JU/SJ
 Sample : J3566-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-6-D

Quant Time: Jun 19 04:45:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 15 11:11:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	107494	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	390254	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	158857	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	249523	20.00	ng	0.00
75) Chrysene-d12	14.15	240	276438	20.00	ng	0.00
86) Perylene-d12	15.69	264	264536	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	734746	115.69	ng	0.00
7) Phenol-d6	6.61	99	875225	109.07	ng	0.00
23) Nitrobenzene-d5	7.53	82	593457	89.46	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	181265	118.59	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	943316	119.13	ng	0.00
78) Terphenyl-d14	13.08	244	814529	73.19	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.71	163	126250	11.124	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061818\
Data File : BF106548.D
Acq On : 18 Jun 2018 19:36
Operator : JU/SJ
Sample : J3566-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-6-D

Quant Time: Jun 19 04:45:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 15 11:11:47 2018
Response via : Initial Calibration

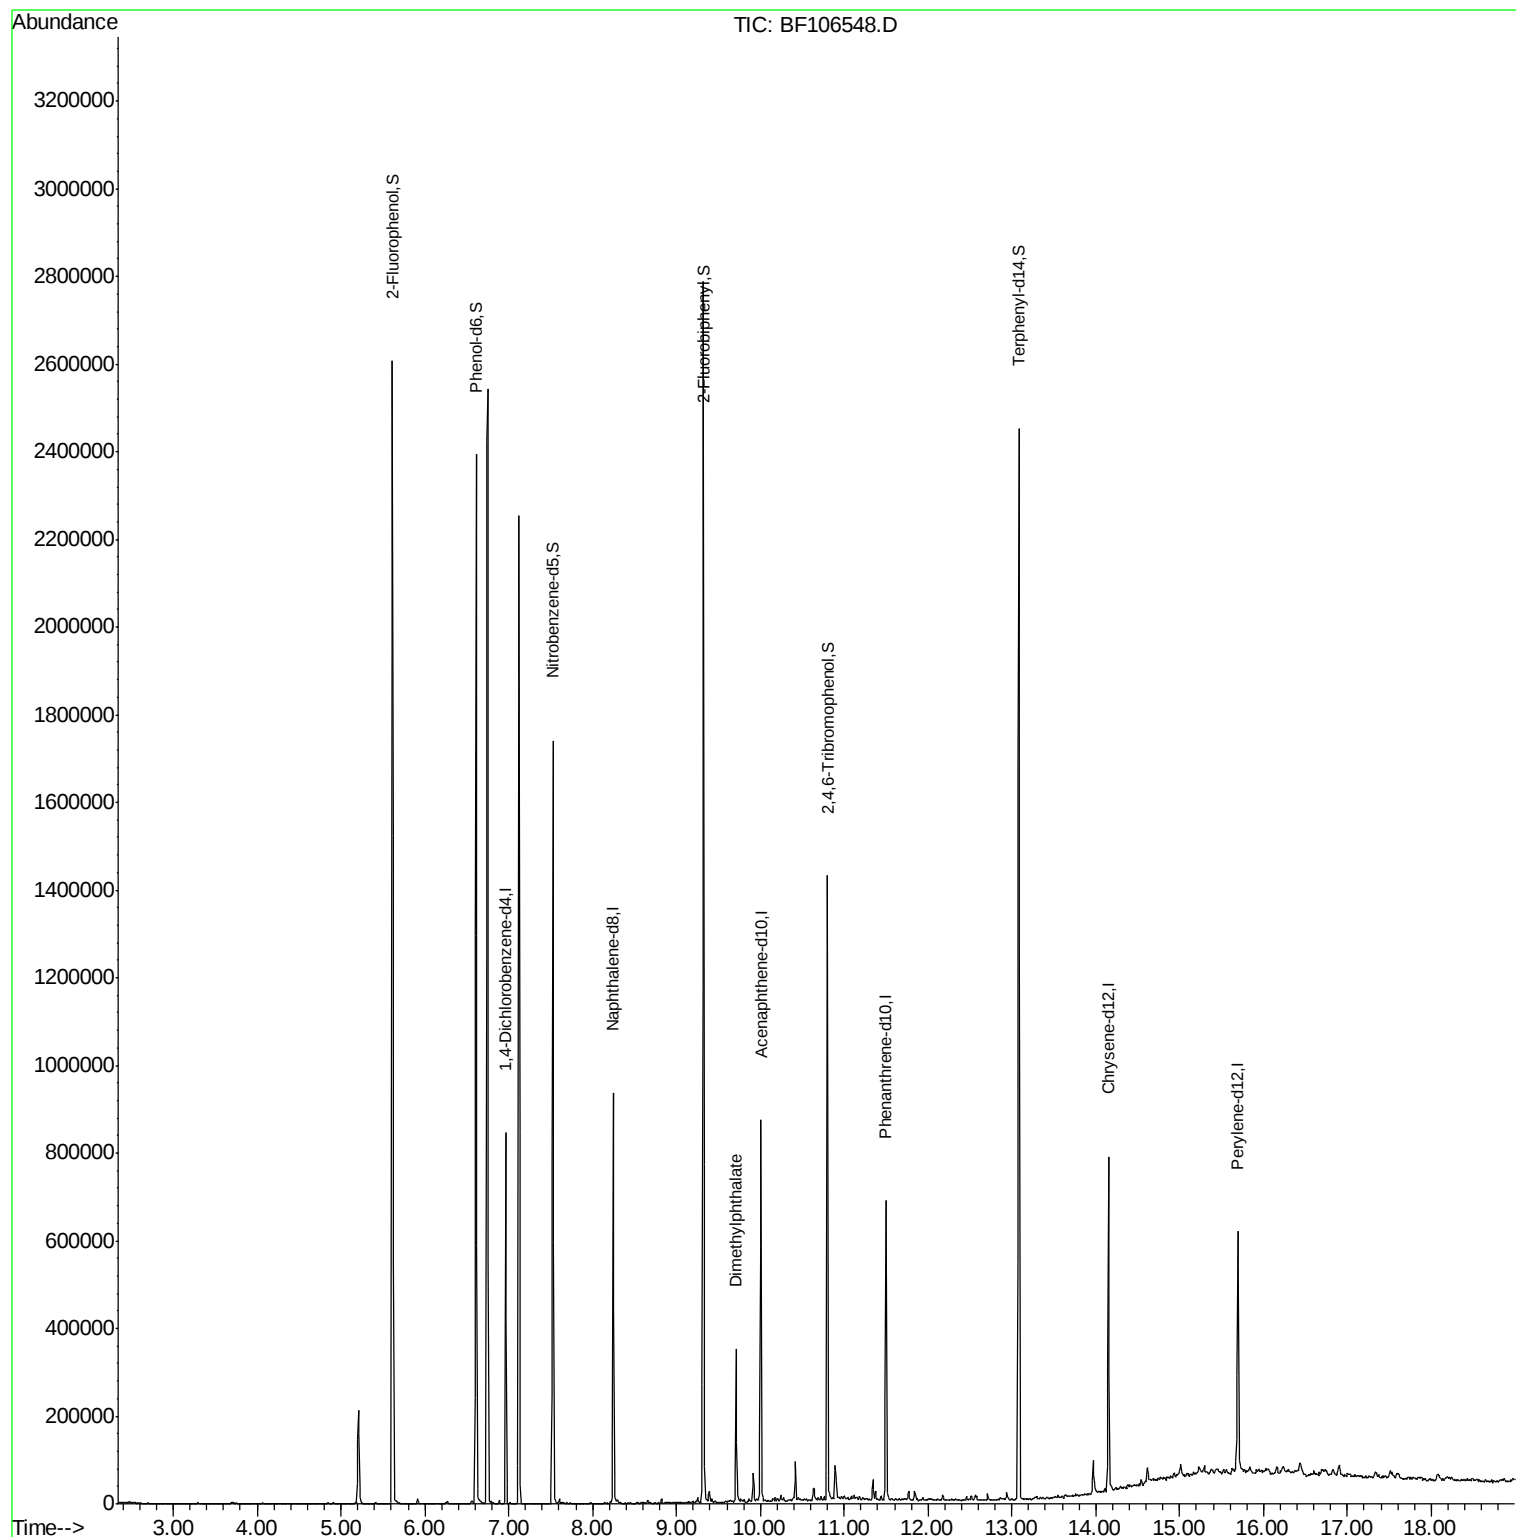




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. 0.00 min
Lab File: BF106548.D
Acq: 18 Jun 2018 19:36

Instrument :
BNA_F
ClientSampleId :
TP-6-D

Tot Ion:152 Resp: 107494
Ion Ratio Lower Upper
152 100
150 158.4 124.6 186.8
115 62.0 50.1 75.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

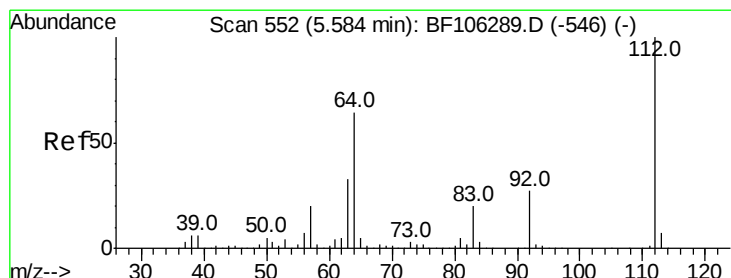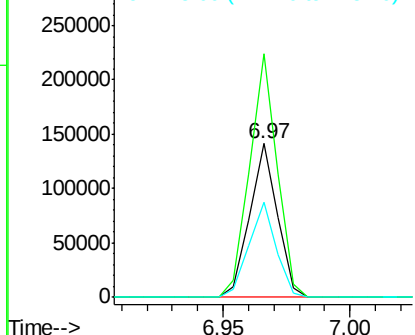



#5

2-Fluorophenol
Concen: 115.686 ng
RT: 5.61 min Scan# 557
Delta R.T. 0.00 min
Lab File: BF106548.D
Acq: 18 Jun 2018 19:36

Tgt Ion:112 Resp: 734746
Ion Ratio Lower Upper
112 100
64 59.1 47.9 71.9
63 29.6 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

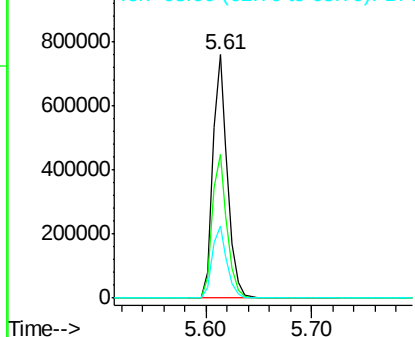



#7

Phenol-d6

Concen: 109.074 ng

RT: 6.61 min Scan# 727

Delta R.T. 0.00 min

Lab File: BF106548.D

Acq: 18 Jun 2018 19:36

Instrument :

BNA_F

ClientSampleId :

TP-6-D


Tot Ion: 99 Resp: 875225

Ion Ratio Lower Upper




99 100

42 16.5 14.5 21.7

71 33.8 25.4 38.0

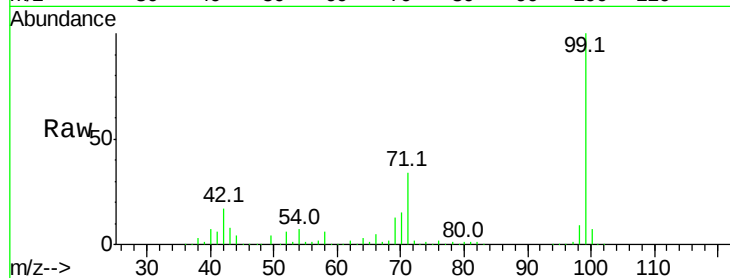

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

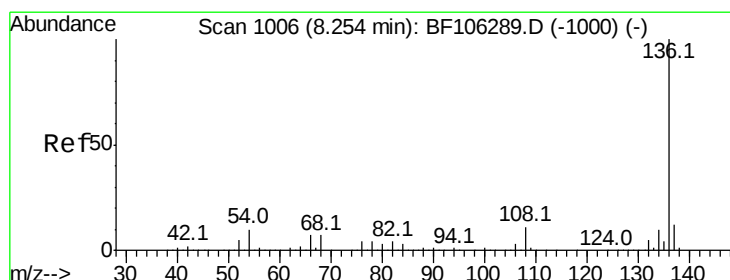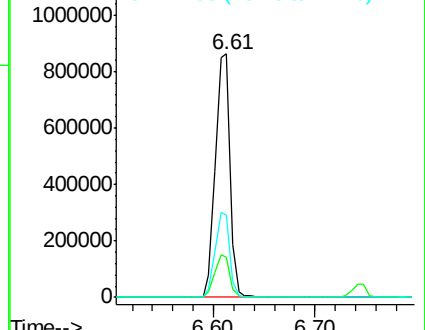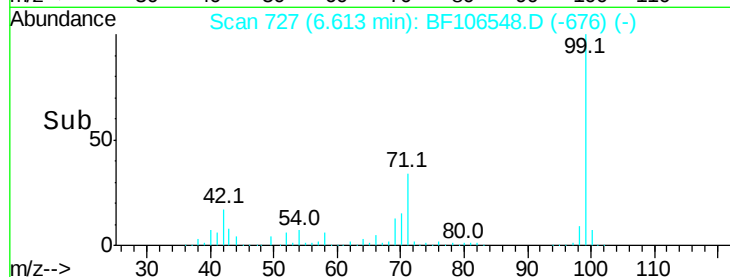

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. 0.00 min

Lab File: BF106548.D

Acq: 18 Jun 2018 19:36

Tgt Ion: 136 Resp: 390254


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 8.8 6.6 9.8

68 6.6 5.0 7.4

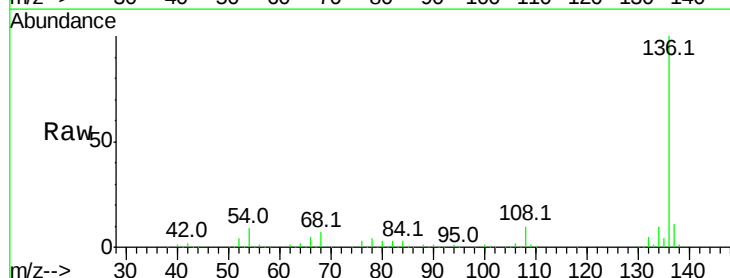

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

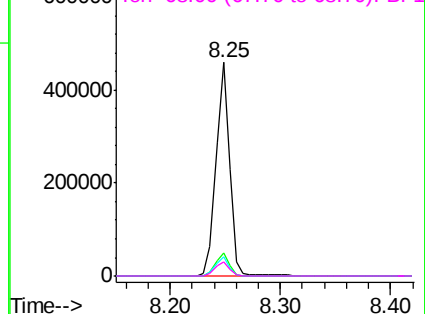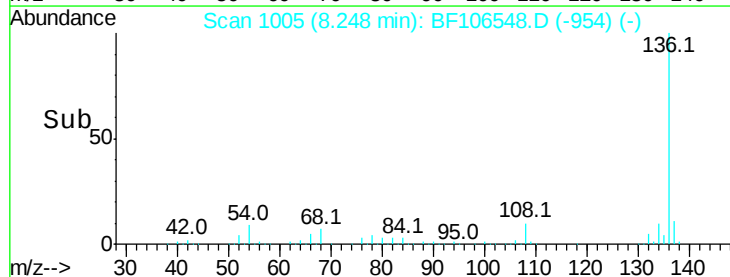


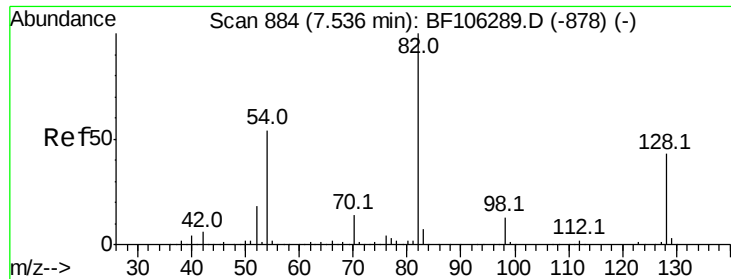




#23
 Nitrobenzene-d5
 Concen: 89.460 ng
 RT: 7.53 min Scan# 883
 Delta R.T. 0.00 min
 Lab File: BF106548.D
 Acq: 18 Jun 2018 19:36

Instrument :
 BNA_F
 ClientSampleId :
 TP-6-D

Tot Ion	Ratio	Lower	Upper
82	100		
128	44.0	36.1	54.1
54	50.8	41.4	62.2

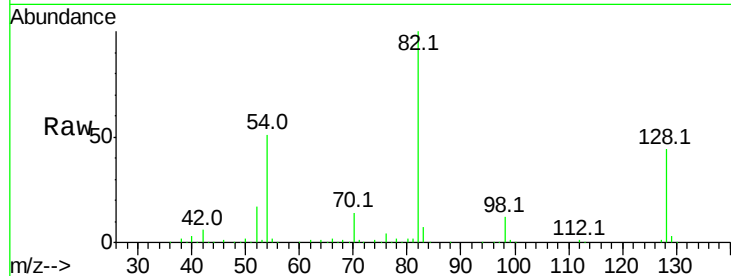


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1


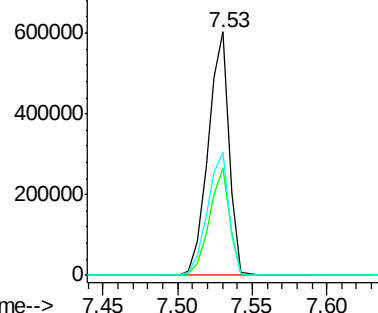


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.01 min Scan# 1304
 Delta R.T. 0.00 min
 Lab File: BF106548.D
 Acq: 18 Jun 2018 19:36

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.2	86.1	129.1
160	49.2	38.3	57.5



Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

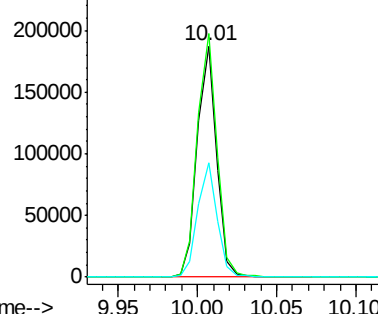







#41
 2,4,6-Tribromophenol
 Concen: 118.592 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. 0.00 min
 Lab File: BF106548.D
 Acq: 18 Jun 2018 19:36

Instrument :
 BNA_F
 ClientSampleId :
 TP-6-D

Tot Ion:330 Resp: 181265
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.0 115.6
 141 29.3 29.9 44.9#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

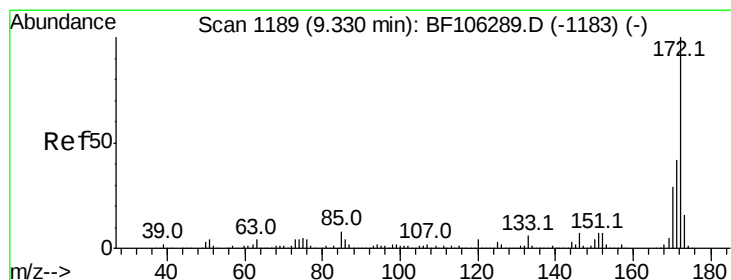
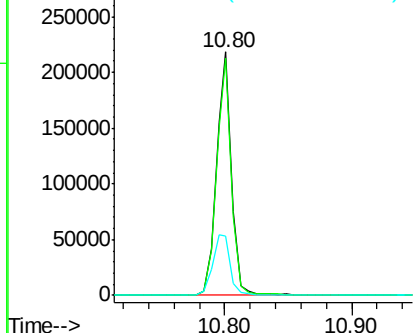



#44
 2-Fluorobiphenyl
 Concen: 119.135 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. 0.00 min
 Lab File: BF106548.D
 Acq: 18 Jun 2018 19:36

Tgt Ion:172 Resp: 943316
 Ion Ratio Lower Upper
 172 100
 171 37.2 29.7 44.5
 170 25.0 19.6 29.4

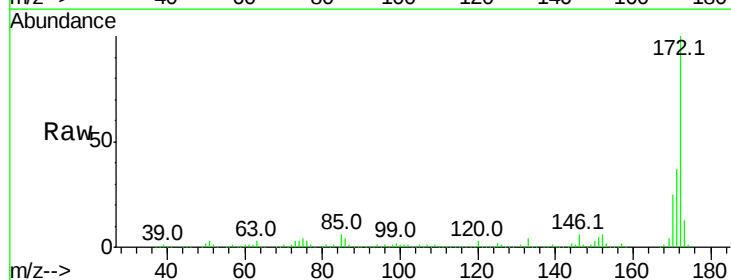

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

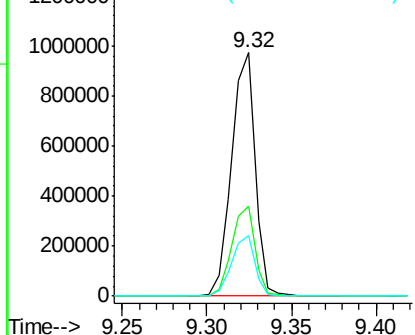

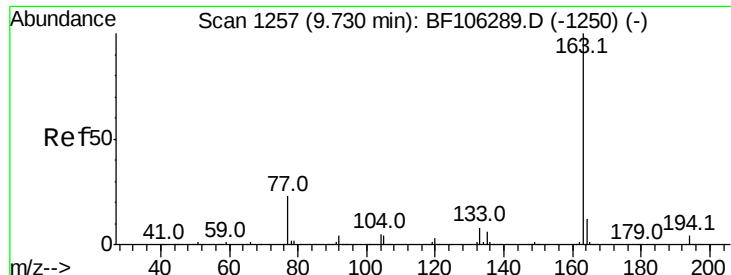

#49

Dimethylphthalate

Concen: 11.124 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.01 min

Lab File: BF106548.D

Acq: 18 Jun 2018 19:36

Instrument :

BNA_F

ClientSampleId :

TP-6-D


Tot Ion:163 Resp: 126250

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 9.7 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

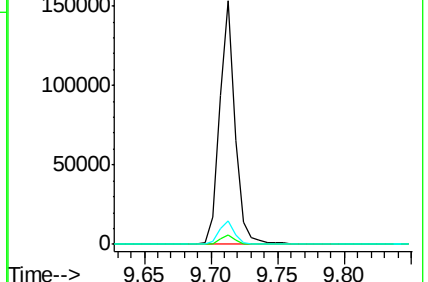

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.49 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106548.D

Acq: 18 Jun 2018 19:36


Tgt Ion:188 Resp: 249523

Ion Ratio Lower Upper

188 100

94 10.2 8.5 12.7



80 11.3 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

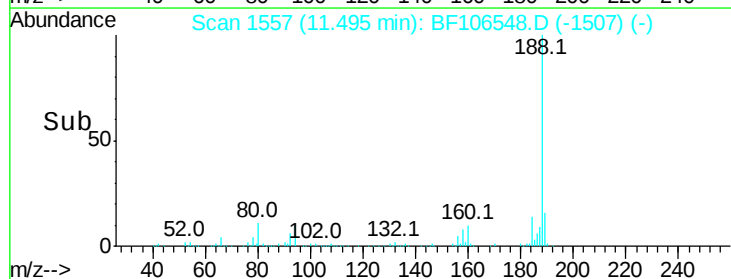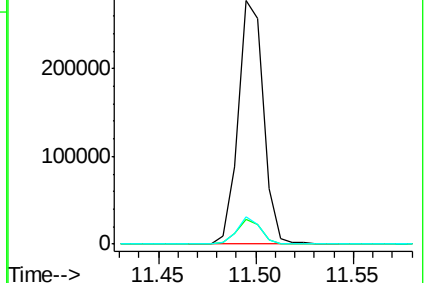



#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2009

Delta R.T. 0.00 min

Lab File: BF106548.D

Acq: 18 Jun 2018 19:36

Instrument :

BNA_F

ClientSampleId :

TP-6-D


Tot Ion:240 Resp: 276438

Ion Ratio Lower Upper

240 100

120 9.4 9.5 14.3#


236 26.1 20.7 31.1





Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

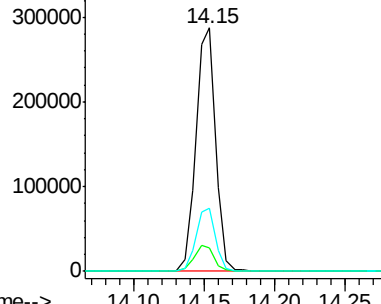

Time-->



#78

Terphenyl-d14

Concen: 73.185 ng

RT: 13.08 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BF106548.D

Acq: 18 Jun 2018 19:36


Tgt Ion:244 Resp: 814529

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0


122 10.3 11.0 16.4#




Abundance Ion 244.00 (243.70 to 244.70): E




Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

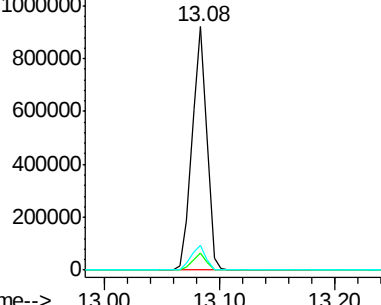

Time-->



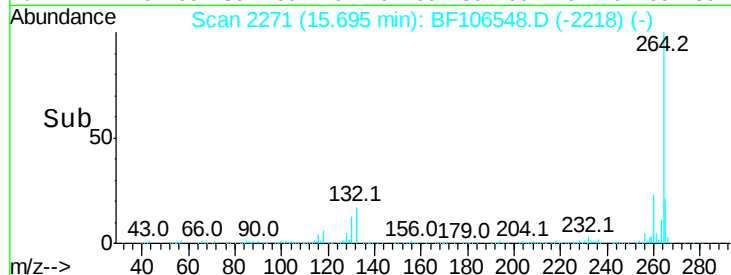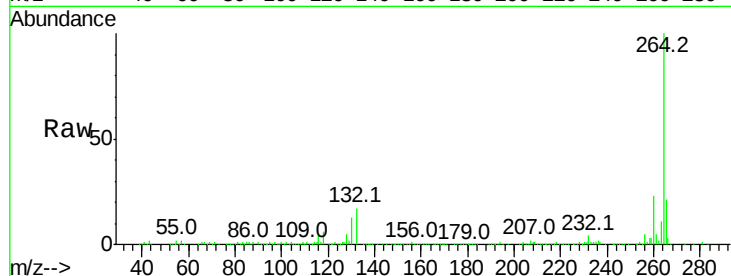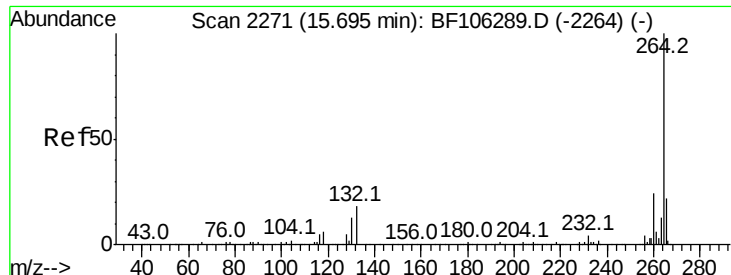

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.69 min Scan# 2271
 Delta R.T. 0.01 min
 Lab File: BF106548.D
 Acq: 18 Jun 2018 19:36

Instrument :
 BNA_F
 ClientSampleId :
 TP-6-D

Tot Ion:	264	Resp:	264536
Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	21.1	17.5	26.3

