


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061818\
 Data File : BF106551.D
 Acq On : 18 Jun 2018 21:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 15 11:11:47 2018

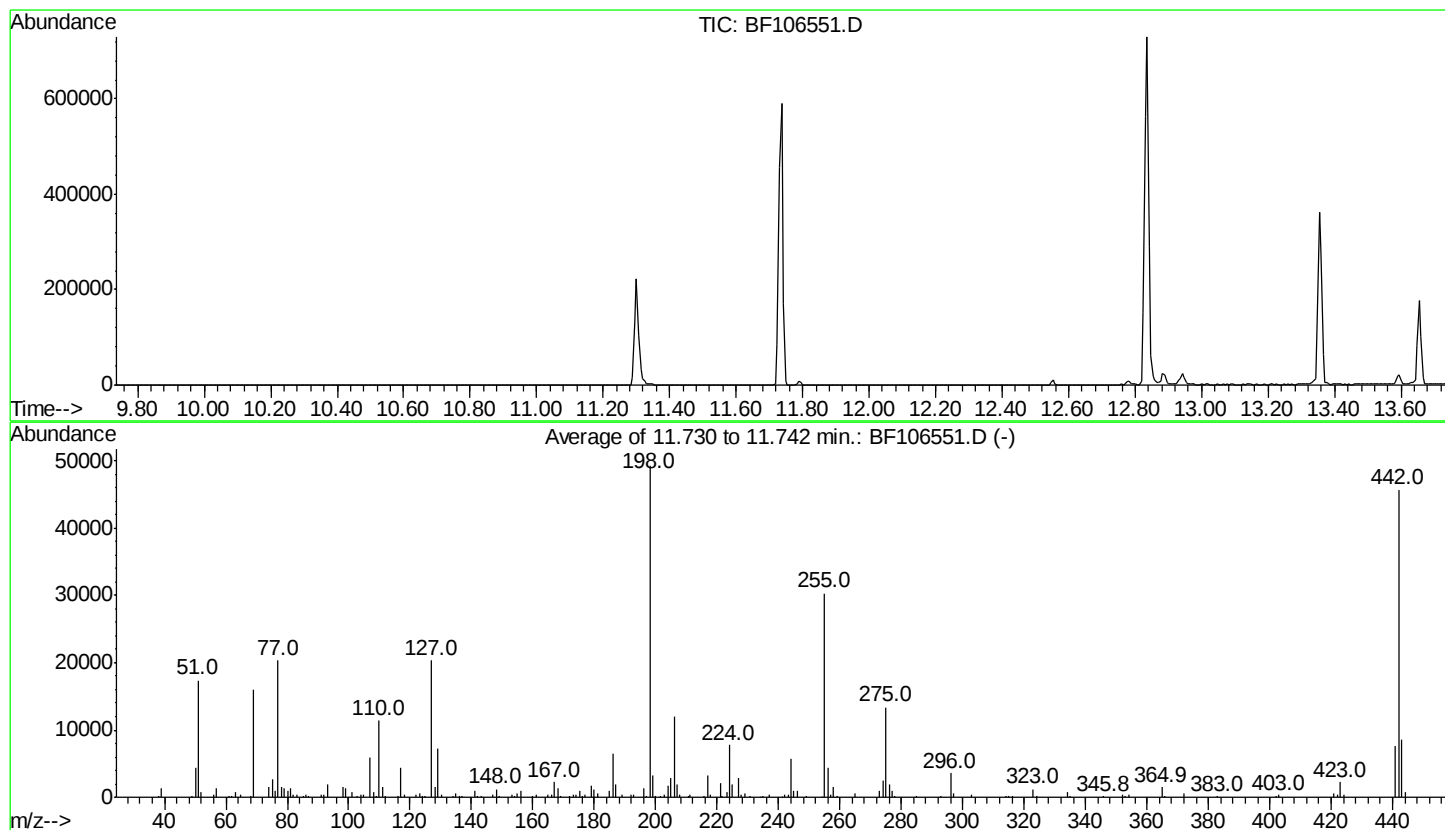

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	17374	PASS
68	69	0.00	2	1.8	284	PASS
69	198	0.00	100	32.6	16075	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.3	20357	PASS
197	198	0.00	2	0.2	121	PASS
198	198	100	100	100.0	49320	PASS
199	198	5	9	6.4	3178	PASS
275	198	10	60	27.1	13364	PASS
365	198	1	100	2.9	1442	PASS
441	443	0.01	100	88.3	7600	PASS
442	198	50	100	92.8	45781	PASS
443	442	15	24	18.8	8610	PASS