


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061820\
 Data File : BF120641.D
 Acq On : 18 Jun 2020 14:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 11:28:22 2020

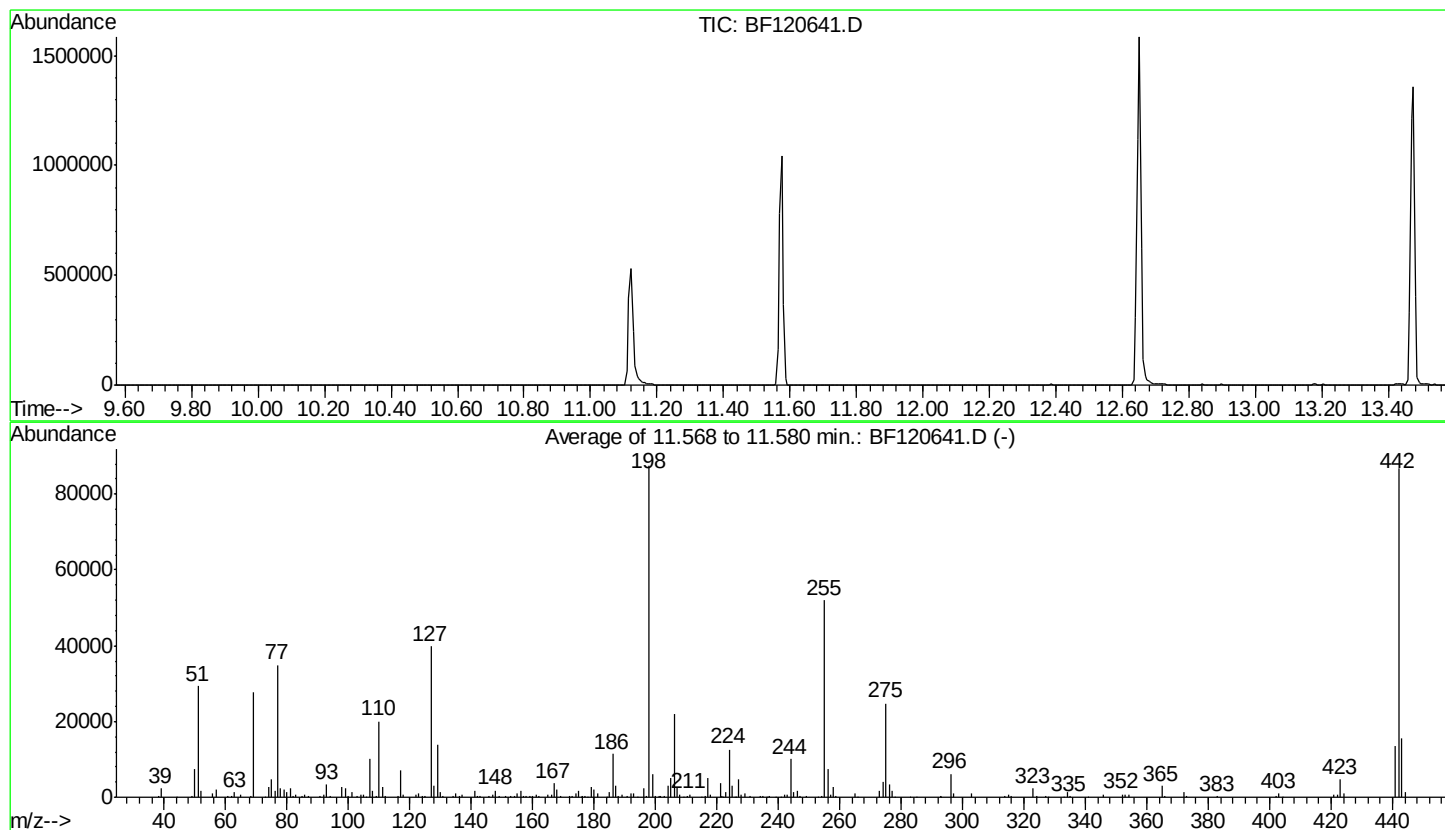

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	29260	PASS
68	69	0.00	2	1.7	476	PASS
69	198	0.00	100	31.6	27635	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	39778	PASS
197	198	0.00	2	0.5	455	PASS
198	198	100	100	100.0	87546	PASS
199	198	5	9	7.1	6181	PASS
275	198	10	60	28.2	24708	PASS
365	198	1	100	3.4	2957	PASS
441	198	0.01	100	15.4	13496	PASS
442	198	50	100	99.3	86904	PASS
443	442	15	24	17.9	15570	PASS