
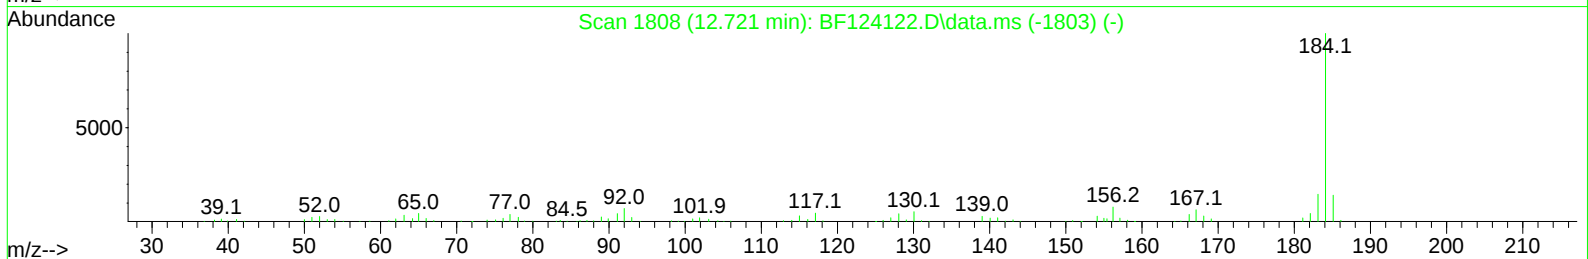
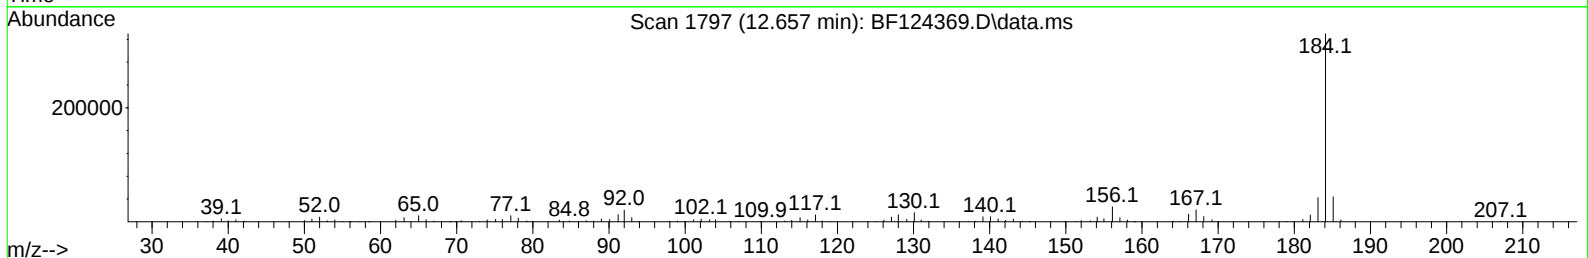


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
 Data File : BF124369.D
 Acq On : 18 Jun 2021 11:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 12:18:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:09:26 2021
 Response via : Initial Calibration

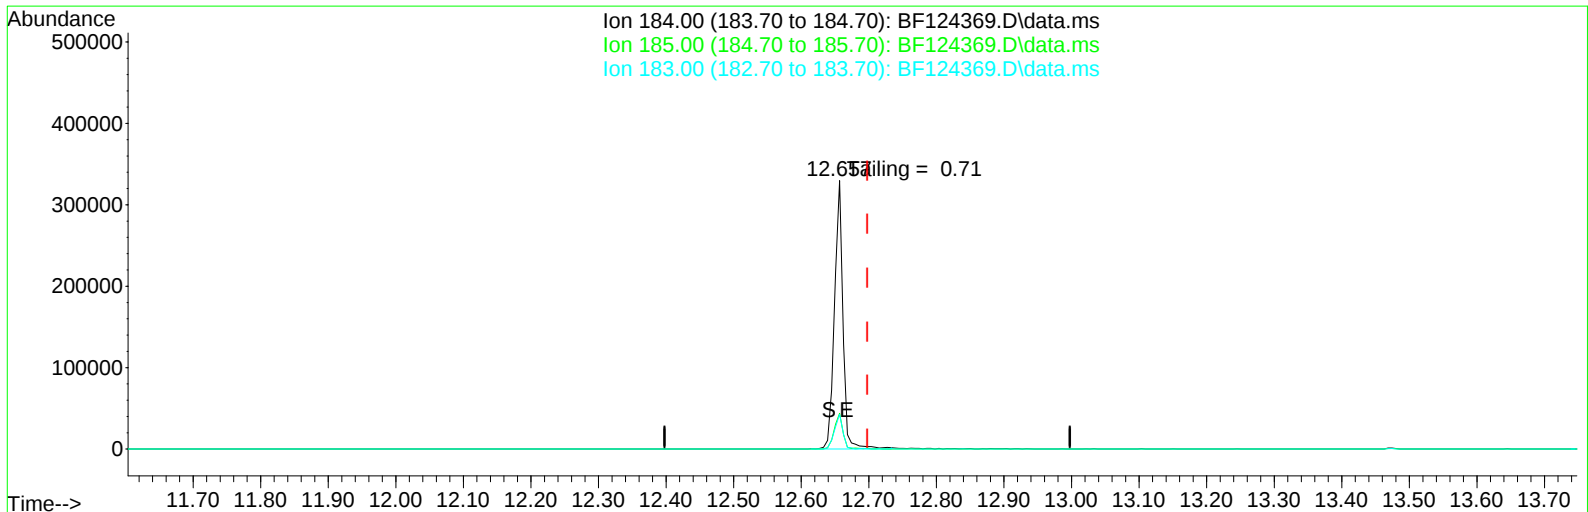

TIC: BF124369.D\data.ms

(77) Benzidine




12.657min (-0.041) 0.00 ng

response 285947

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.33
183.00	9.80	12.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
Data File : BF124369.D
Acq On : 18 Jun 2021 11:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 12:18:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

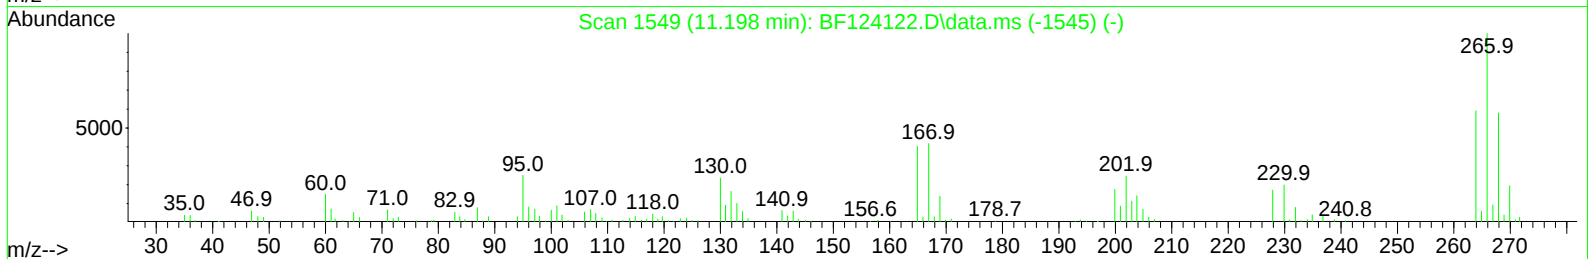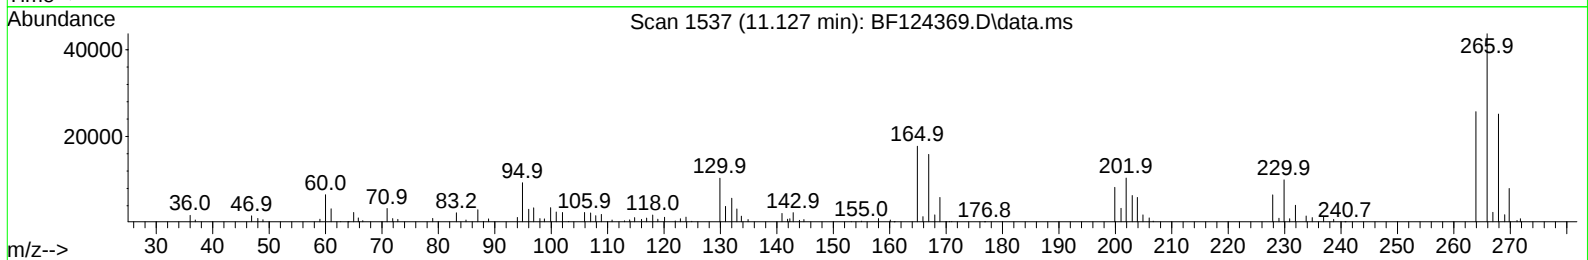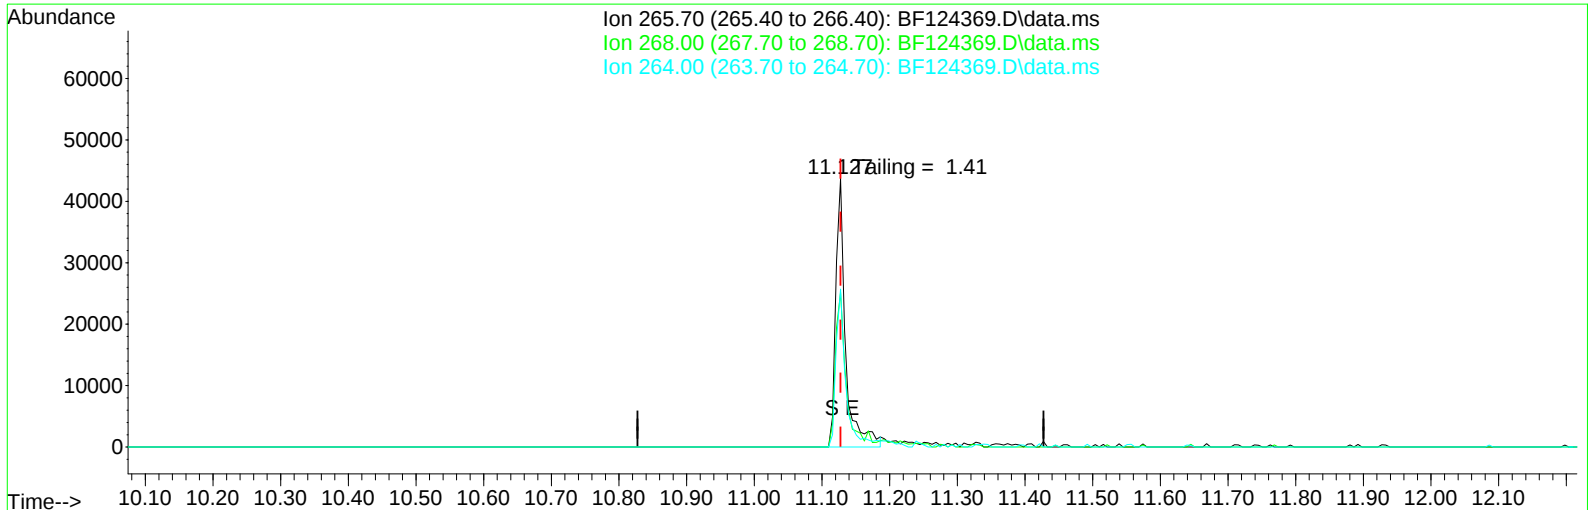

TIC: BF124369.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 14243.95 ng

response 46082

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	57.62
264.00	65.70	58.84
0.00	0.00	0.00