

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
 Data File : BF124374.D
 Acq On : 18 Jun 2021 15:11
 Operator : JU/CG
 Sample : PB137196BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137196BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	497	500	510	rBB2	16593	23091	1.25%	0.229%
2	5.422	563	567	576	rBV	1485952	1351107	73.25%	13.426%
3	6.434	735	739	742	rBV	1219014	1292493	70.07%	12.844%
4	6.781	795	798	802	rBV	298406	257634	13.97%	2.560%
5	7.351	890	895	898	rBV	854116	904656	49.05%	8.990%
6	8.069	1013	1017	1020	rBV	411154	332560	18.03%	3.305%
7	9.145	1195	1200	1203	rBV	2034636	1844508	100.00%	18.329%
8	9.822	1312	1315	1319	rBV	502312	406257	22.03%	4.037%
9	10.616	1446	1450	1461	rBV	1225508	1114844	60.44%	11.078%
10	11.310	1565	1568	1574	rBV	482418	404894	21.95%	4.023%
11	12.904	1834	1839	1842	rBV	1841262	1653983	89.67%	16.436%
12	13.957	2014	2018	2022	rBV	303465	258784	14.03%	2.572%
13	15.415	2261	2266	2274	rBV	166061	218427	11.84%	2.171%




Sum of corrected areas: 10063238

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
Data File : BF124374.D
Acq On : 18 Jun 2021 15:11
Operator : JU/CG
Sample : PB137196BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137196BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

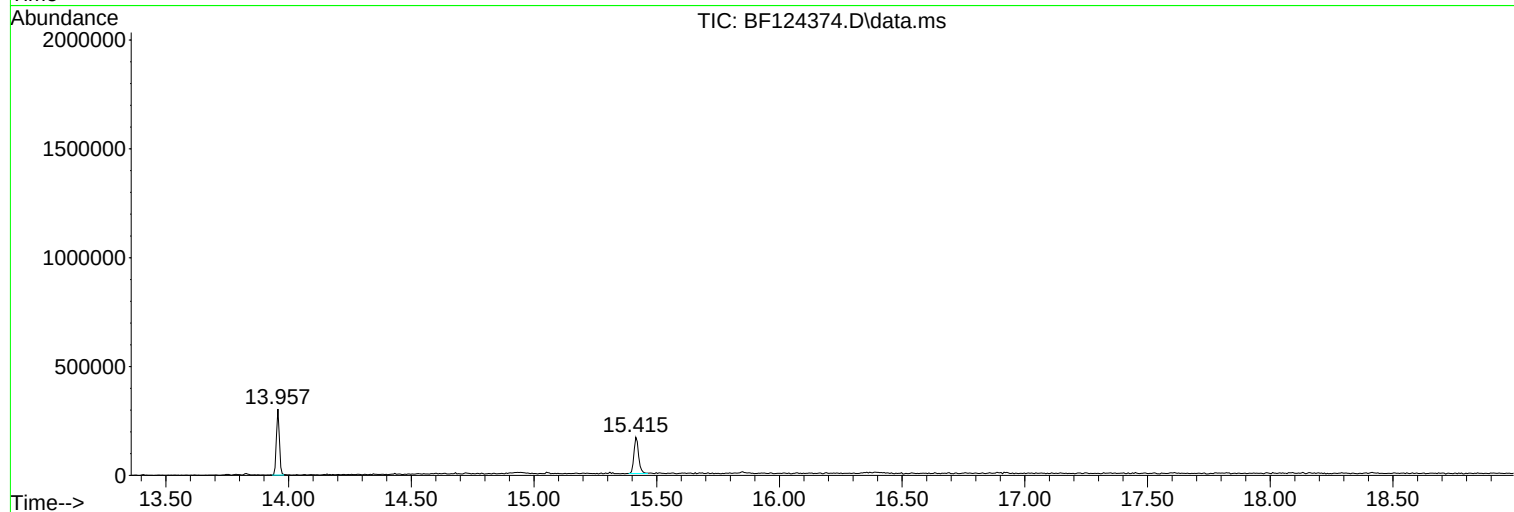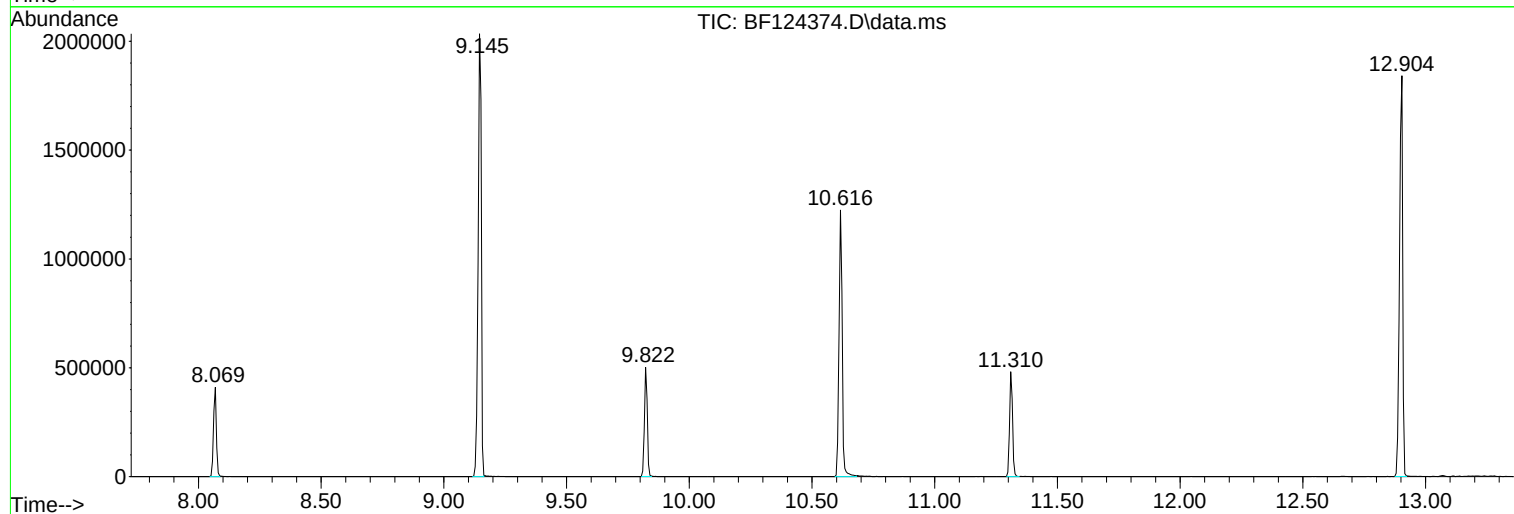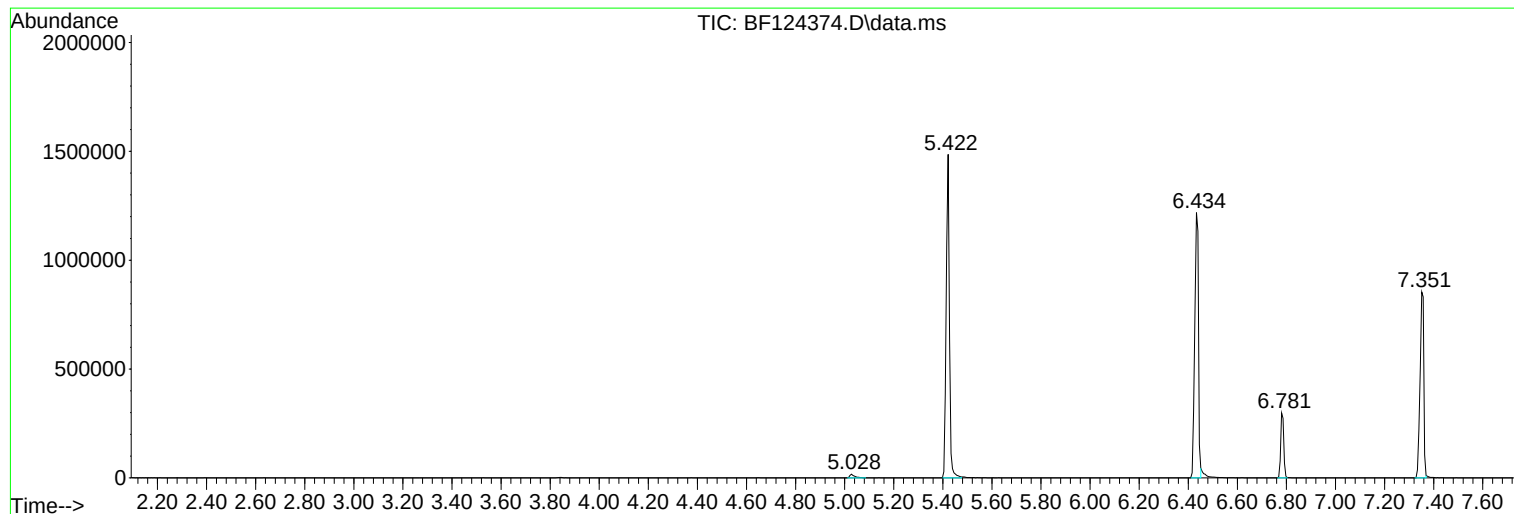

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
Data File : BF124374.D
Acq On : 18 Jun 2021 15:11
Operator : JU/CG
Sample : PB137196BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137196BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
Data File : BF124374.D
Acq On : 18 Jun 2021 15:11
Operator : JU/CG
Sample : PB137196BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137196BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------