


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
 Data File : BF124369.D
 Acq On : 18 Jun 2021 11:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 15 20:09:26 2021

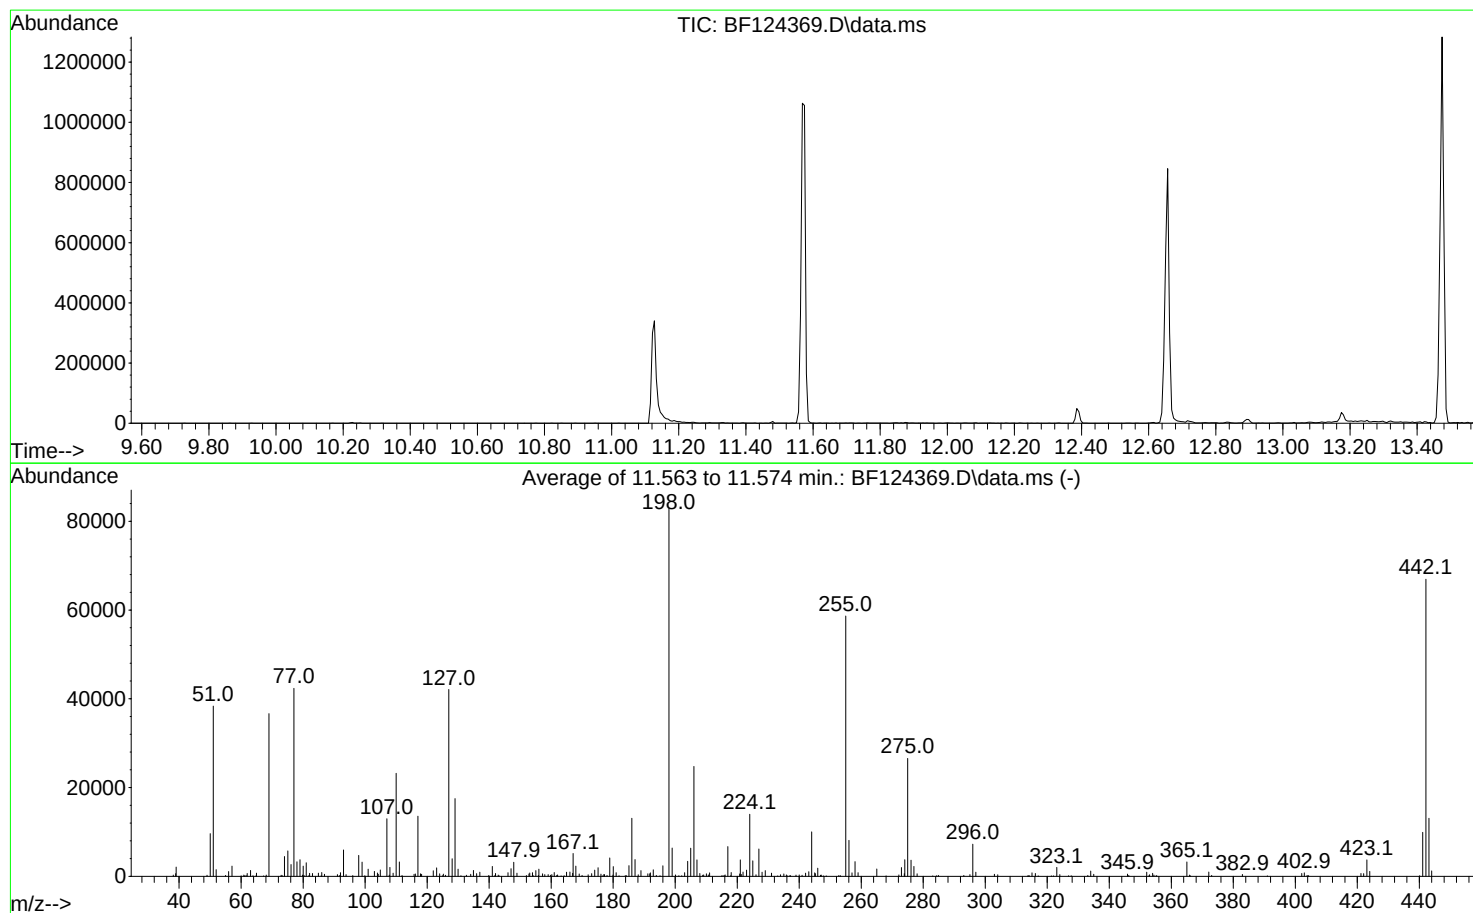

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	38349	PASS
68	69	0.00	2	0.8	284	PASS
69	198	0.00	100	44.2	36659	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	42120	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82872	PASS
199	198	5	9	7.7	6378	PASS
275	198	10	60	32.1	26571	PASS
365	198	1	100	3.9	3248	PASS
441	198	0.01	100	12.0	9930	PASS
442	442	50	100	100.0	66930	PASS
443	442	15	24	19.5	13081	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/18/2021	BNA_F	<u>BF124369.D</u>
Compound Name	Response	Retention Time
DDT	177483	13.47
DDD	5524	13.17
DDE	755	12.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6279	183762	3.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
Data File : BF124369.D
Acq On : 18 Jun 2021 11:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 12:18:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

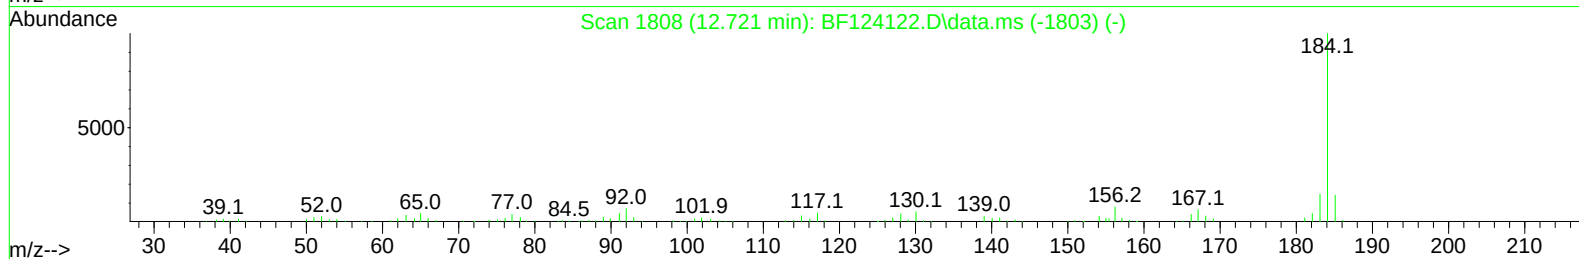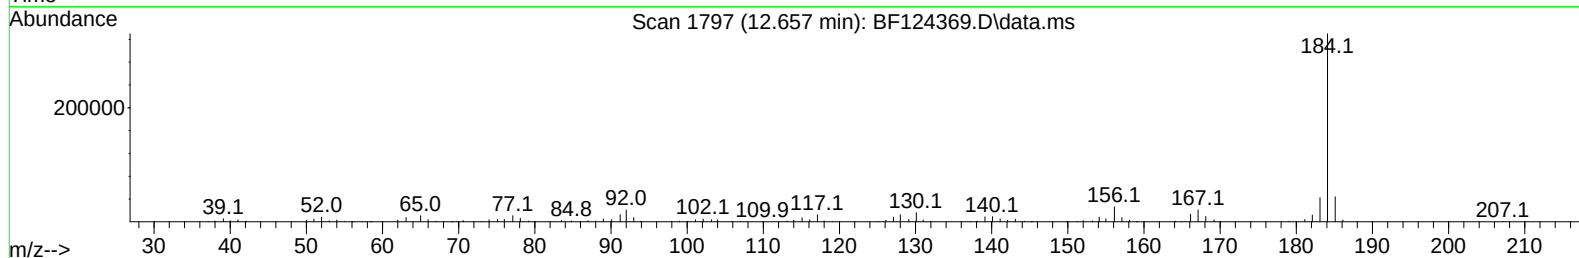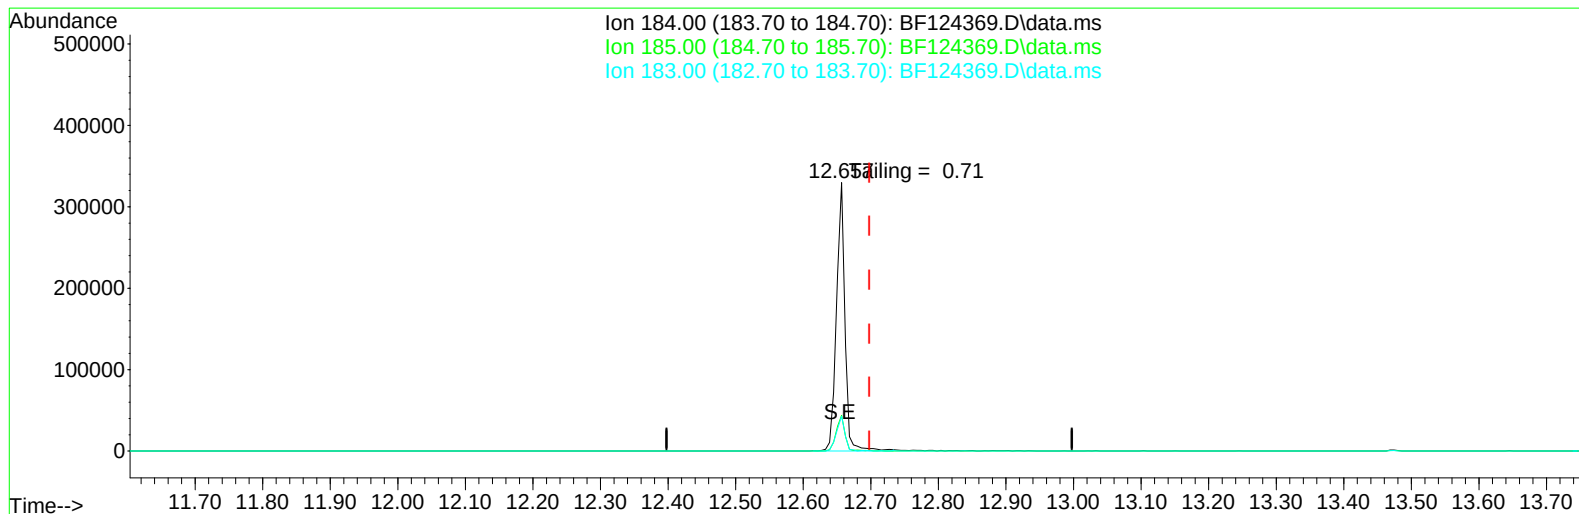

TIC: BF124369.D\data.ms

(77) Benzidine

12.657min (-0.041) 0.00 ng




response 285947

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.33
183.00	9.80	12.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061821\
Data File : BF124369.D
Acq On : 18 Jun 2021 11:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 12:18:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

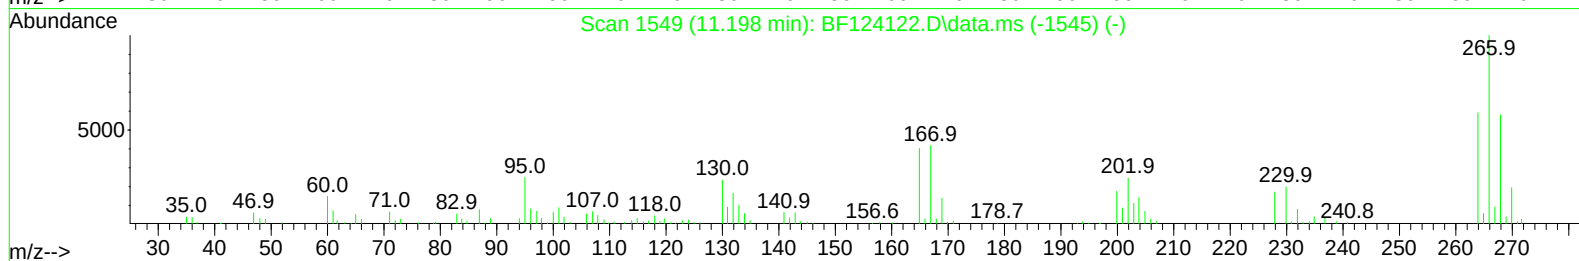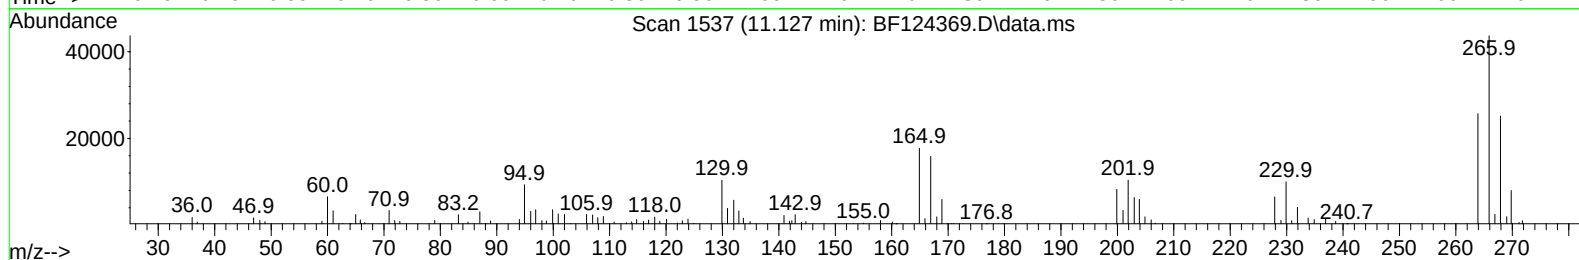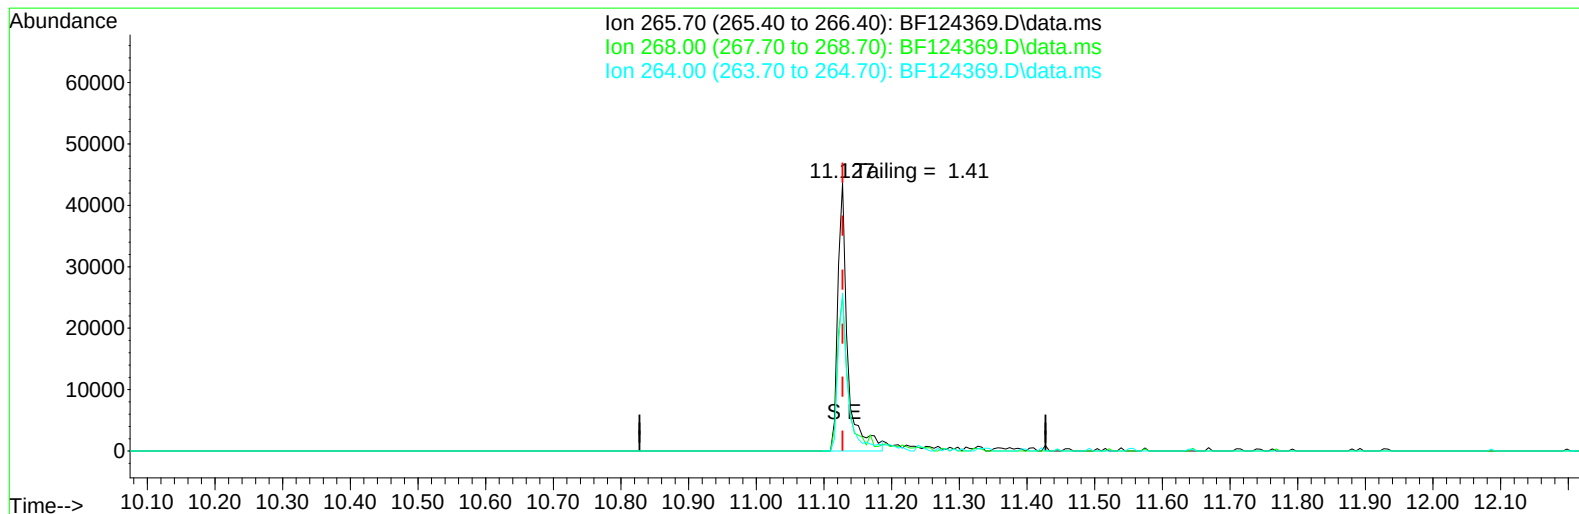

TIC: BF124369.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 14243.95 ng

response 46082

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	57.62
264.00	65.70	58.84
0.00	0.00	0.00