
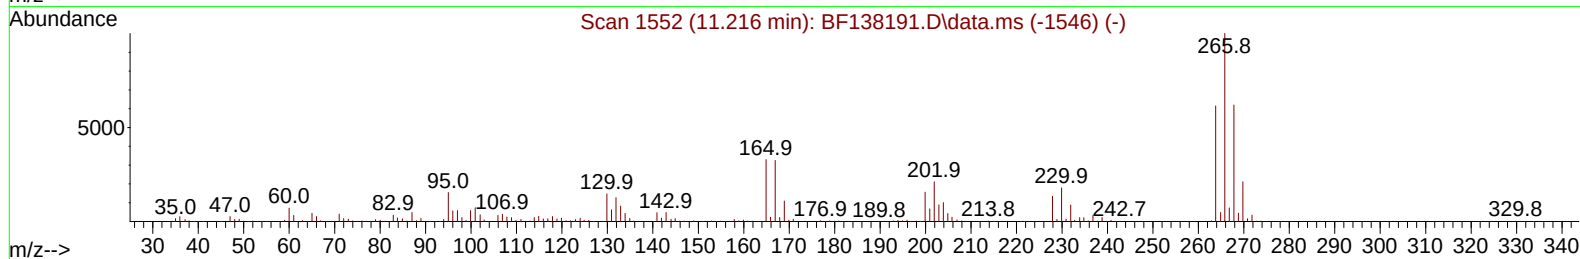
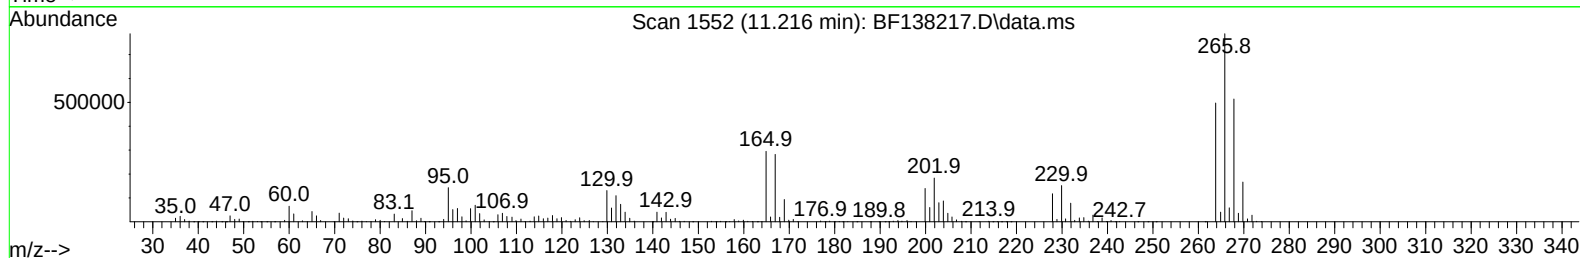


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061824\
Data File : BF138217.D
Acq On : 18 Jun 2024 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 11:23:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

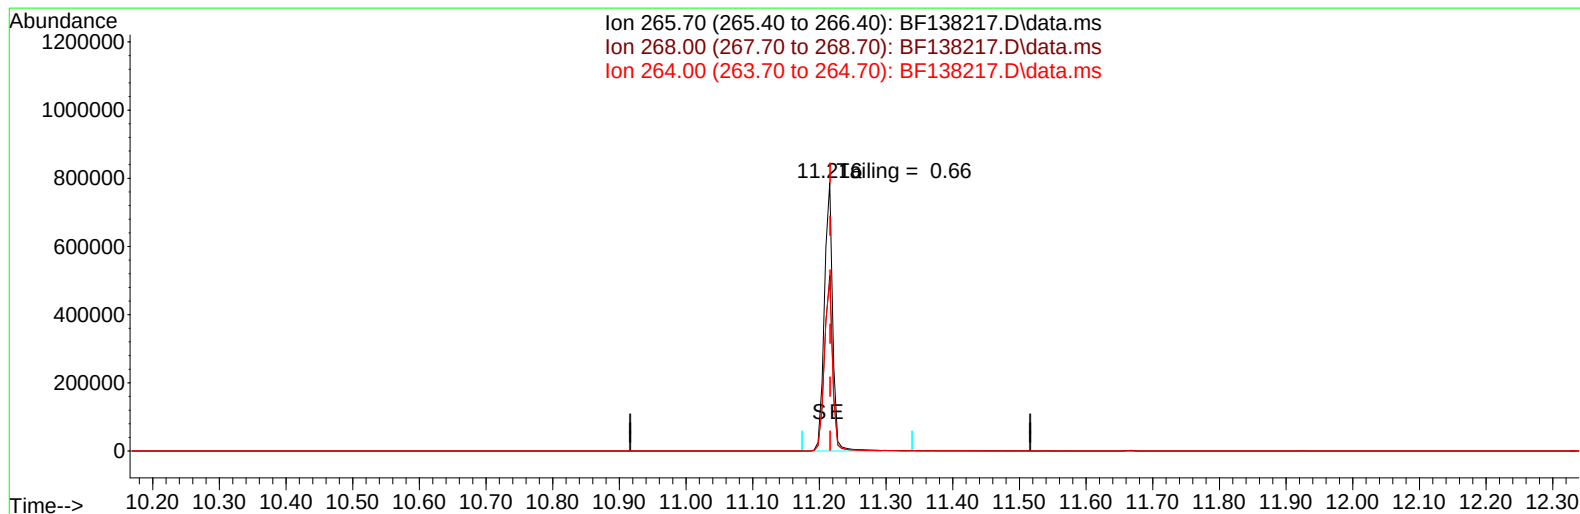

TIC: BF138217.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 782708.16 ng

response 690318

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	65.31
264.00	61.50	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061824\
Data File : BF138217.D
Acq On : 18 Jun 2024 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 11:23:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

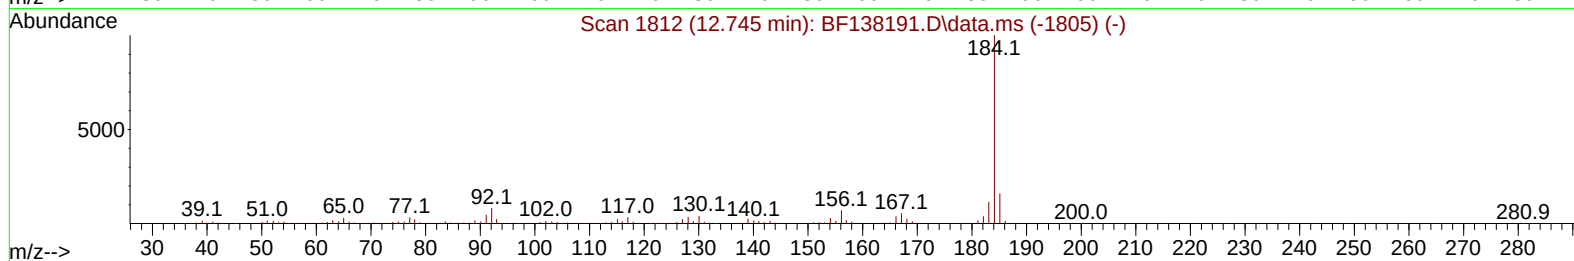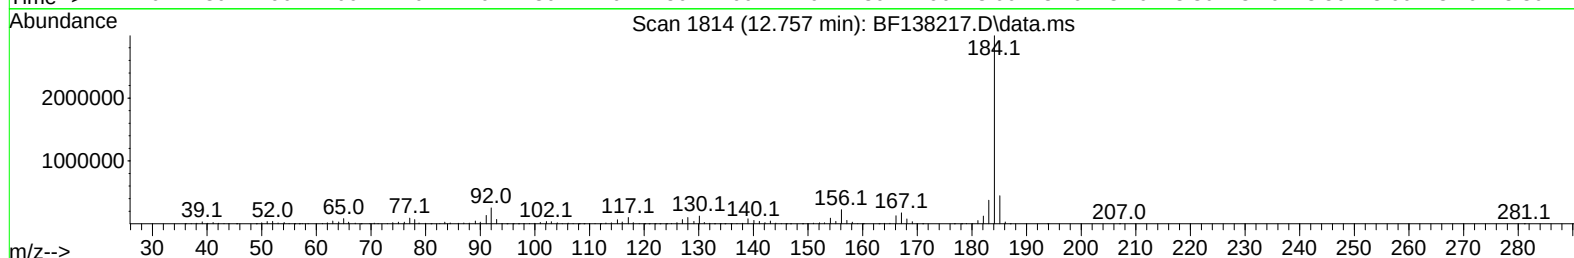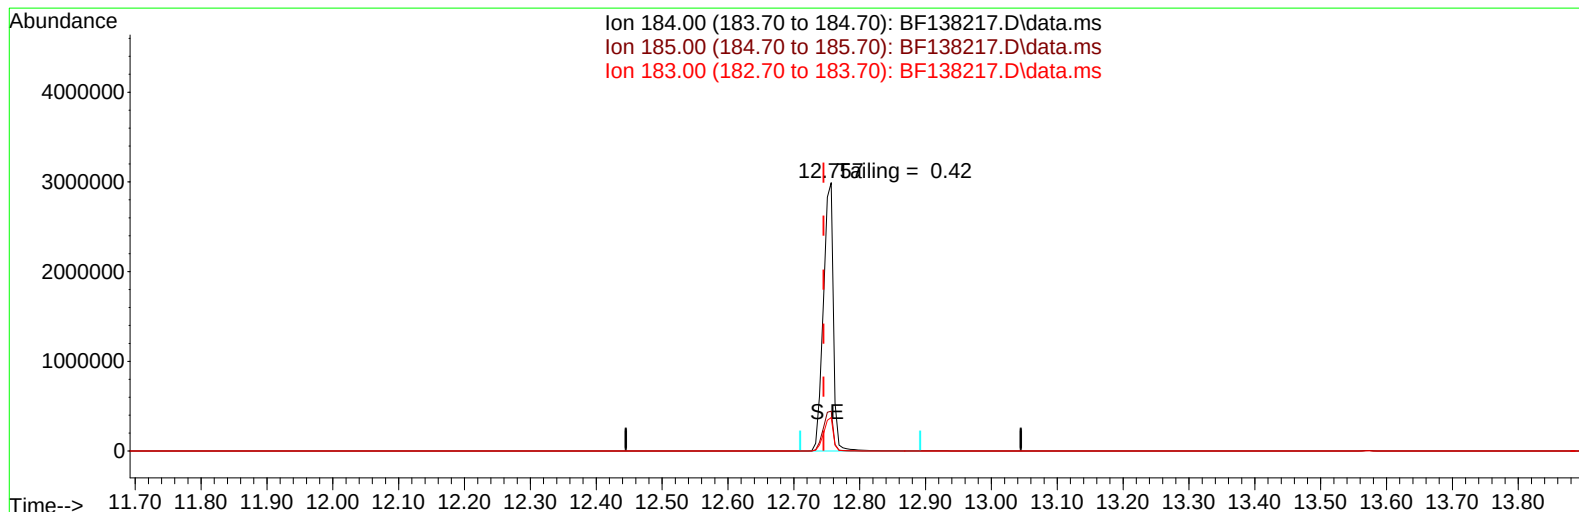

TIC: BF138217.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 1673017.61 ng

response 3173615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.87
183.00	11.30	12.49
0.00	0.00	0.00