
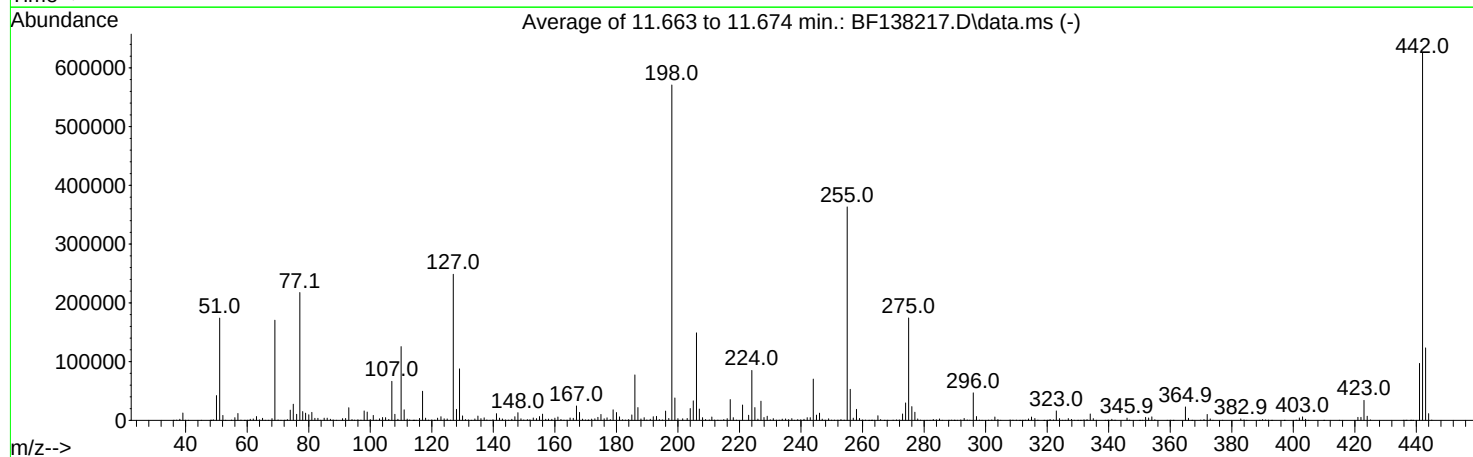


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061824\
Data File : BF138217.D
Acq On : 18 Jun 2024 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

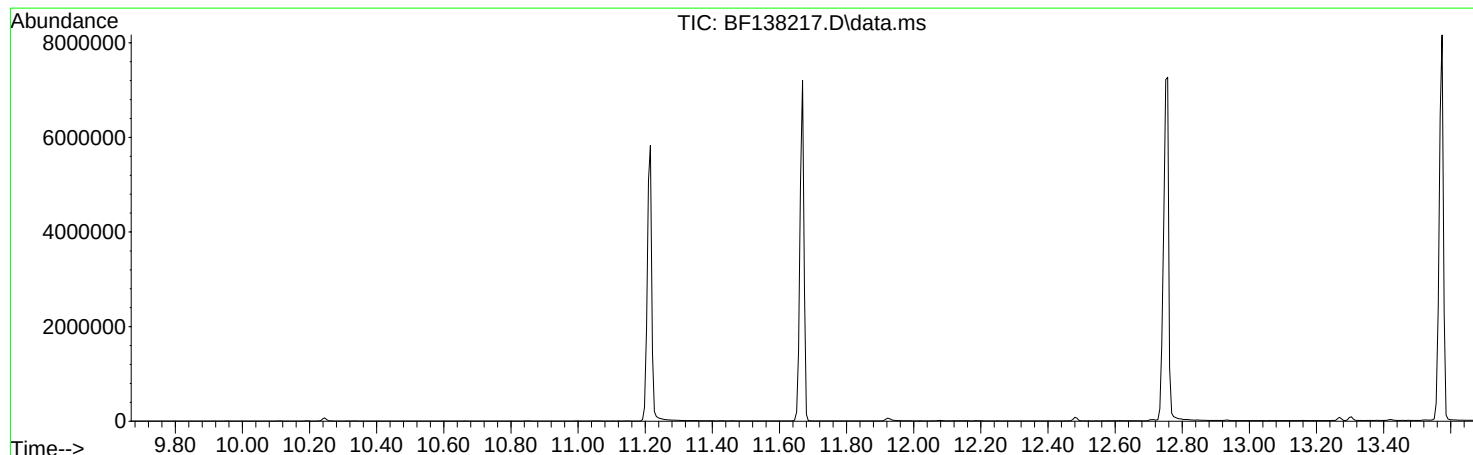

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	173973	PASS
68	69	0.00	2	1.8	3104	PASS
69	198	0.00	100	29.9	170576	PASS
70	69	0.00	2	0.5	891	PASS
127	198	10	80	43.6	248749	PASS
197	198	0.00	2	0.6	3422	PASS
198	198	100	100	100.0	570901	PASS
199	198	5	9	6.7	38045	PASS
275	198	10	60	30.5	174235	PASS
365	198	1	100	4.0	22920	PASS
441	198	0.01	100	17.0	97107	PASS
442	442	50	100	100.0	626133	PASS
443	442	15	24	19.7	123504	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/18/2024	BNA_F	<u>BF138217.D</u>
Compound Name	Response	Retention Time
DDT	1381124	13.574
DDD	21814	13.304
DDE	1549	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23363	1404487	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061824\
Data File : BF138217.D
Acq On : 18 Jun 2024 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 11:23:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

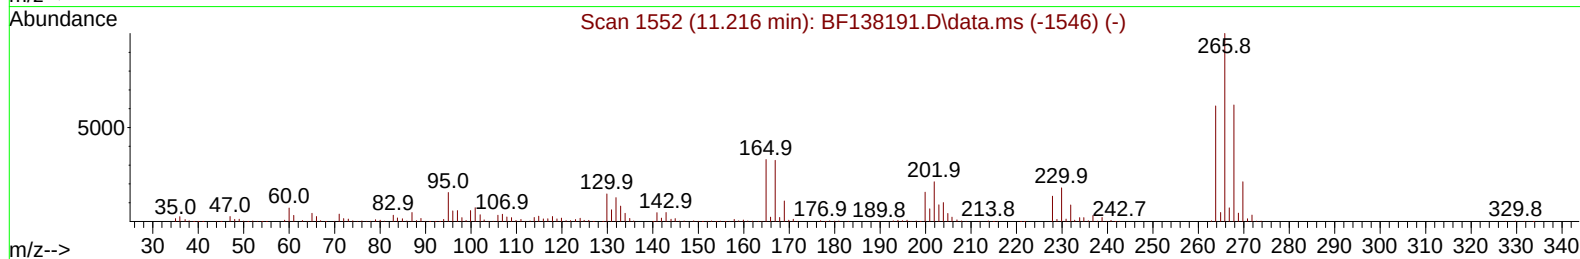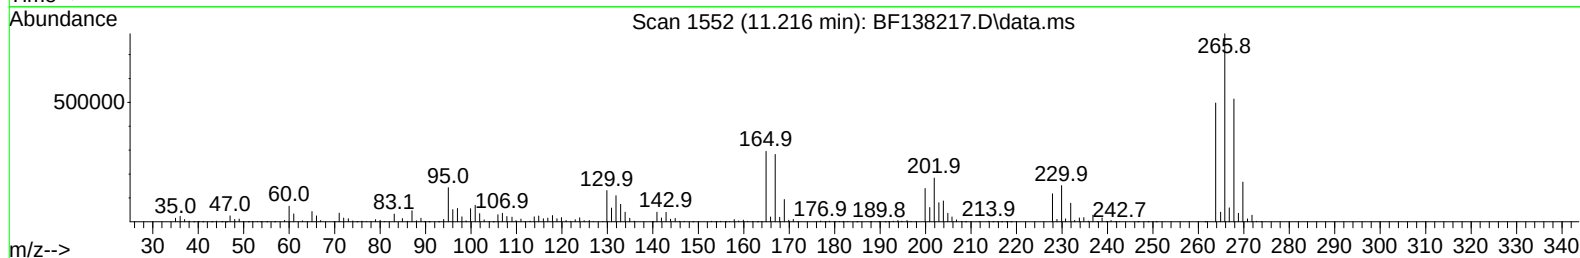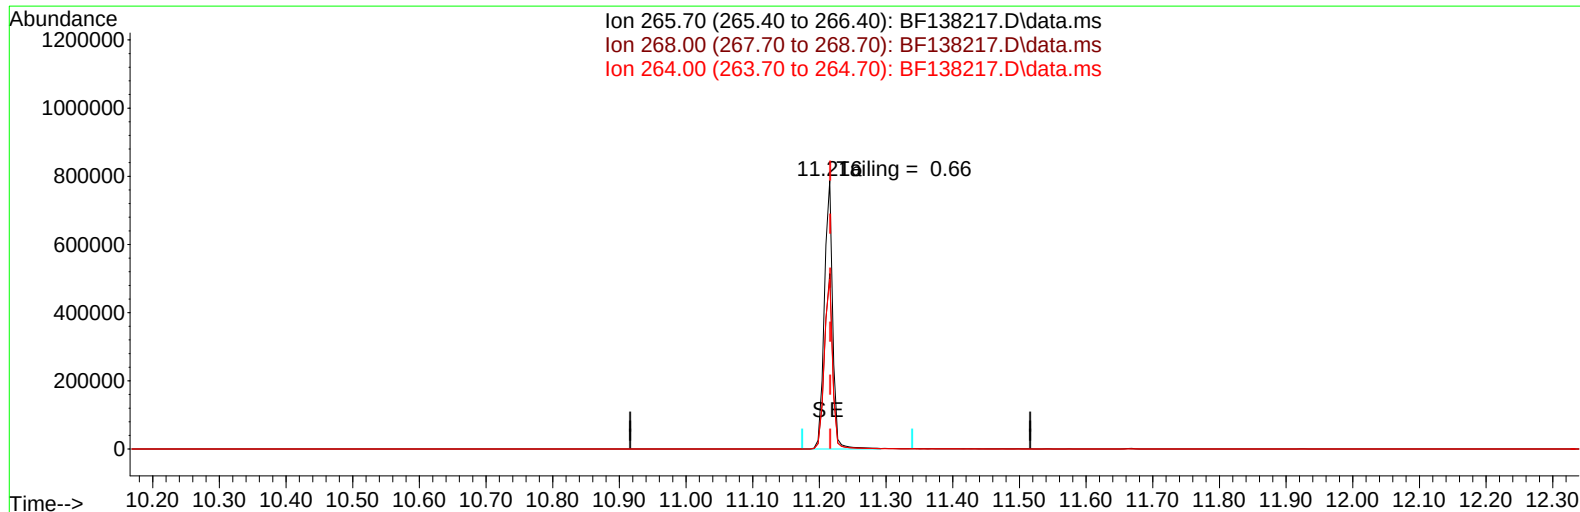

TIC: BF138217.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 782708.16 ng




response 690318

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	65.31
264.00	61.50	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061824\
Data File : BF138217.D
Acq On : 18 Jun 2024 10:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 11:23:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

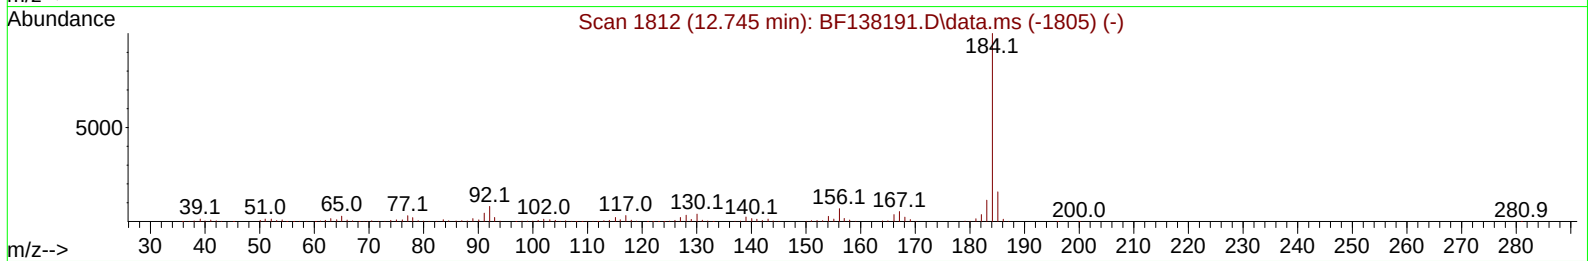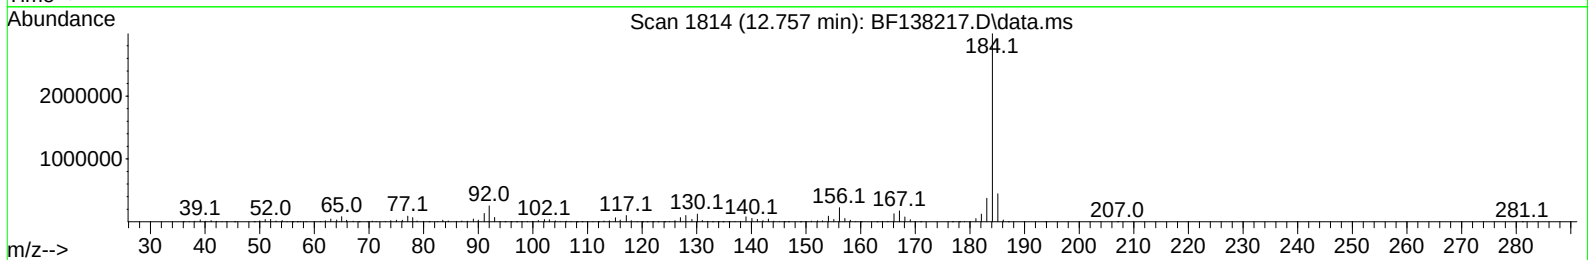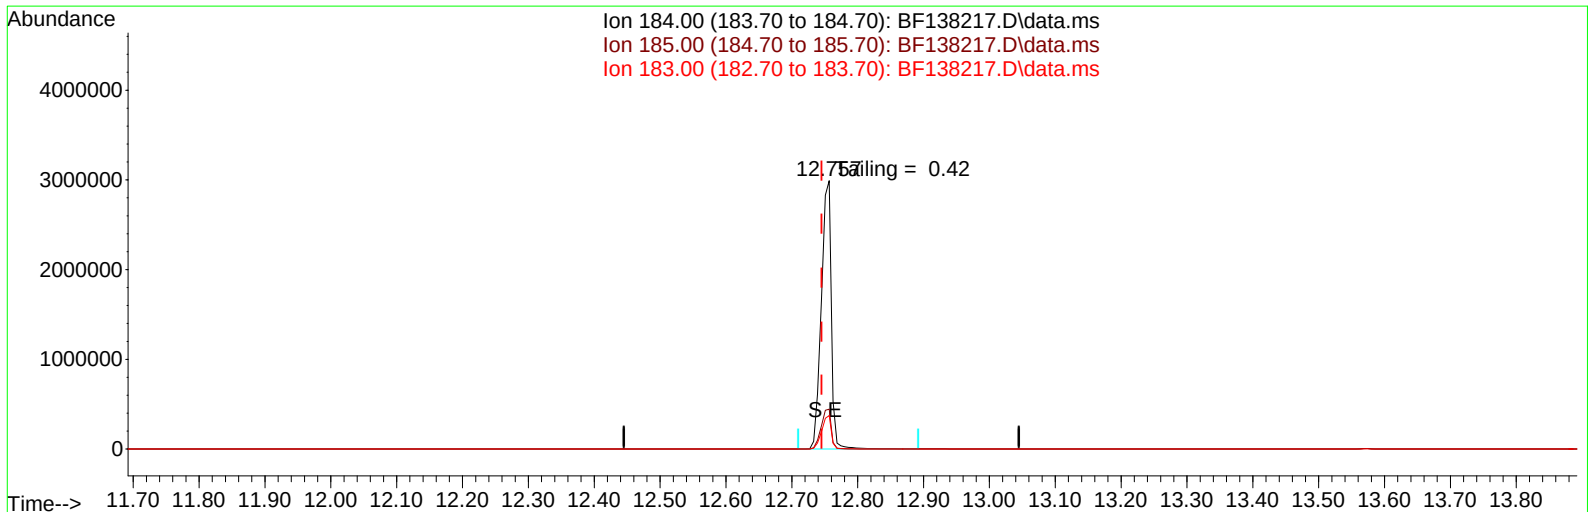

TIC: BF138217.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 1673017.61 ng

response 3173615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.87
183.00	11.30	12.49
0.00	0.00	0.00