
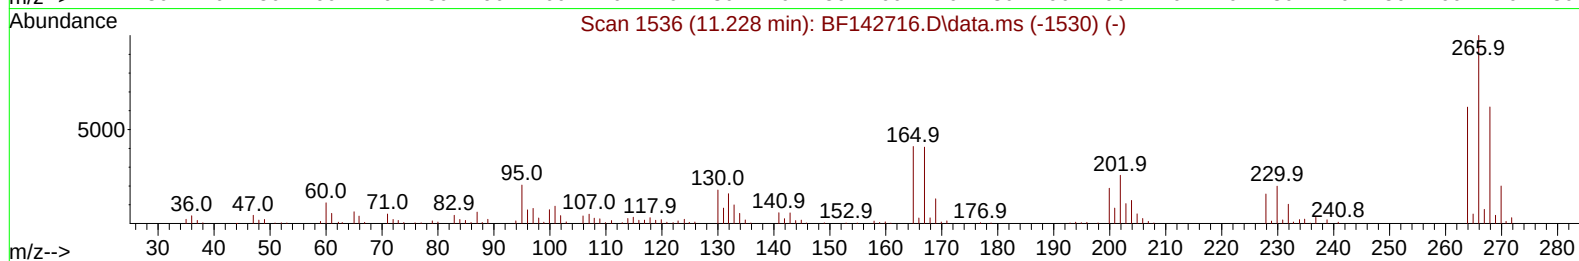
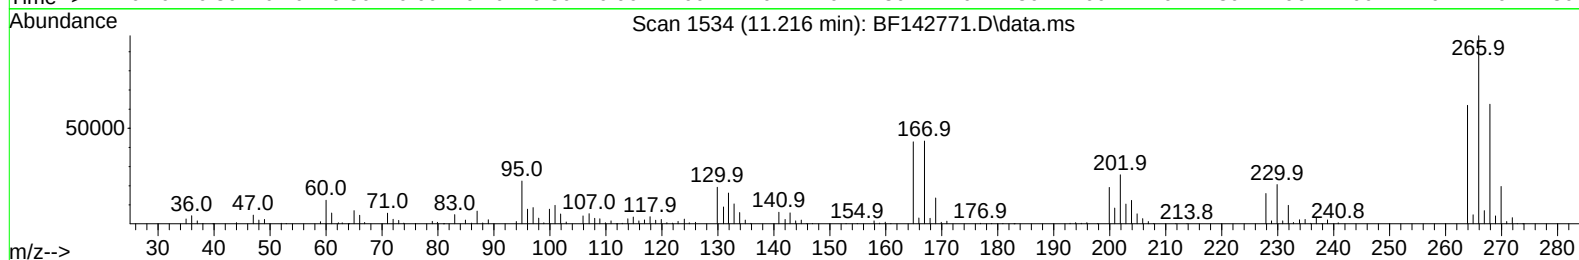


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061825\
Data File : BF142771.D
Acq On : 18 Jun 2025 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 13:05:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

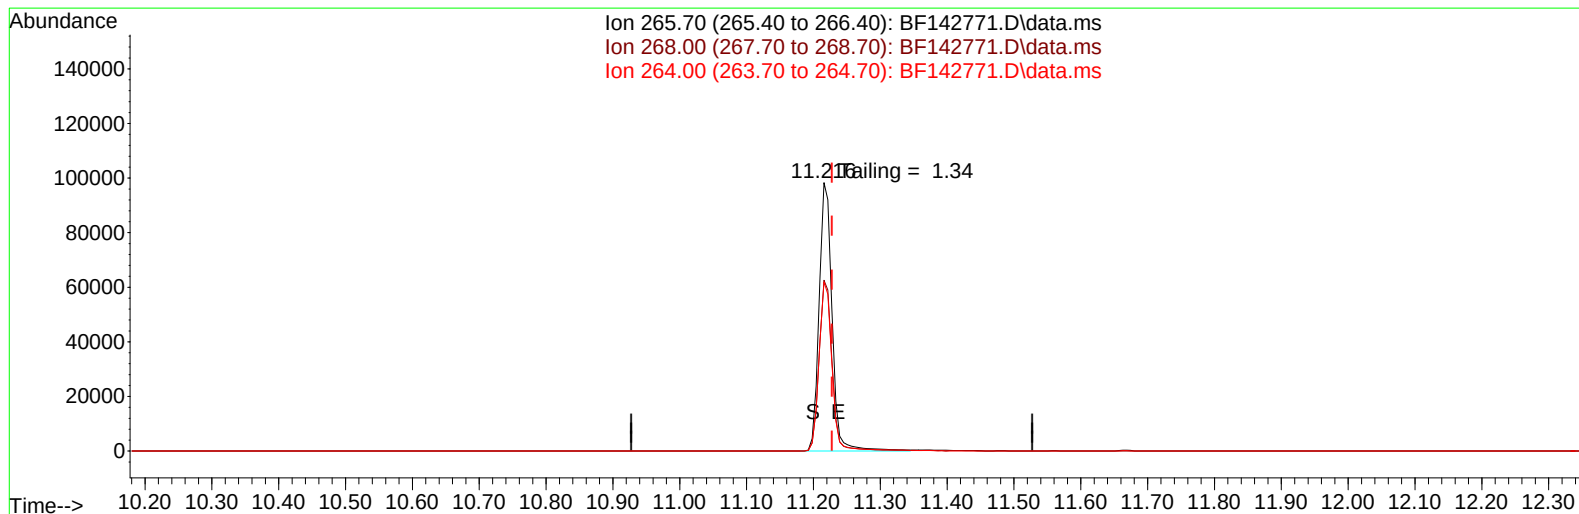

TIC: BF142771.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.012) 34494.01 ng

response 132909

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	63.62
264.00	61.90	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061825\
Data File : BF142771.D
Acq On : 18 Jun 2025 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 13:05:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

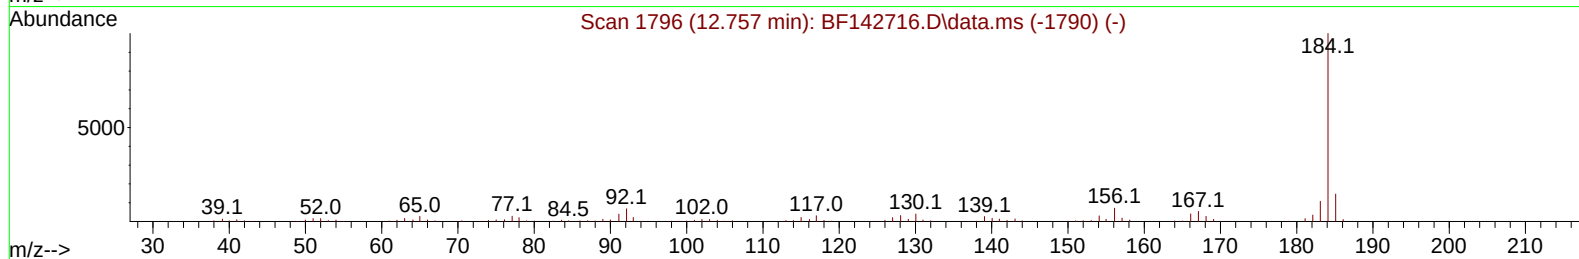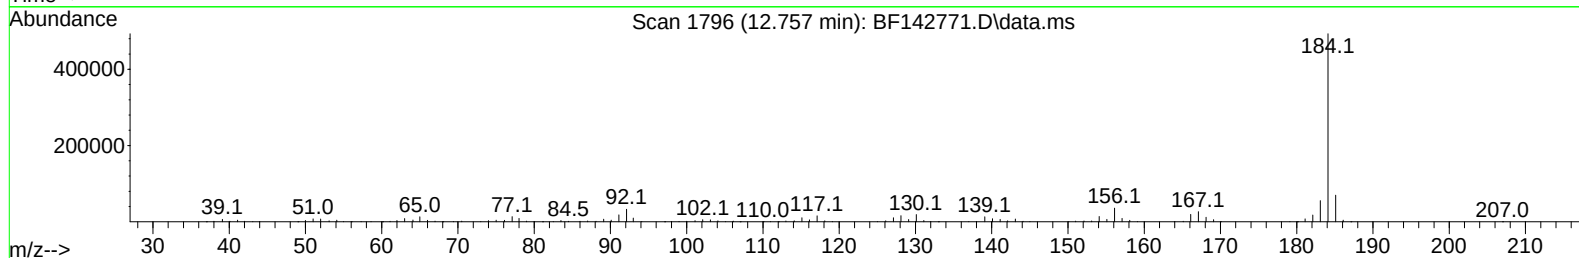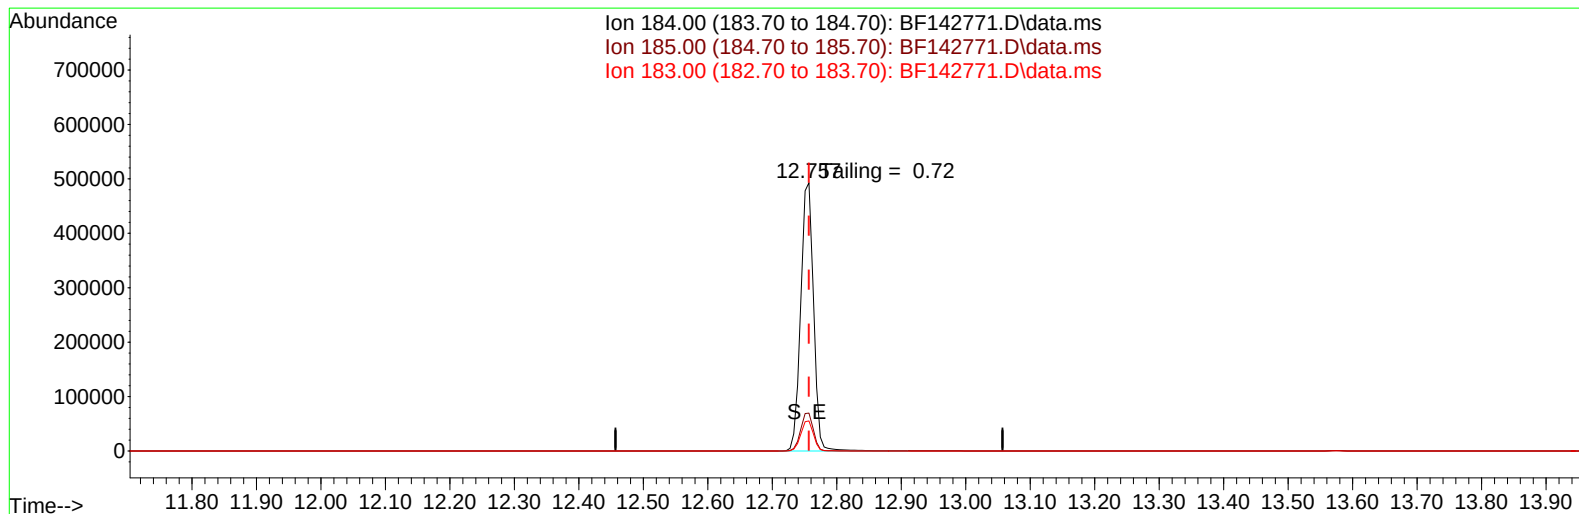

TIC: BF142771.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 680187

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.15
183.00	10.70	11.24
0.00	0.00	0.00