


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061825\
Data File : BF142771.D
Acq On : 18 Jun 2025 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 11 05:56:09 2025

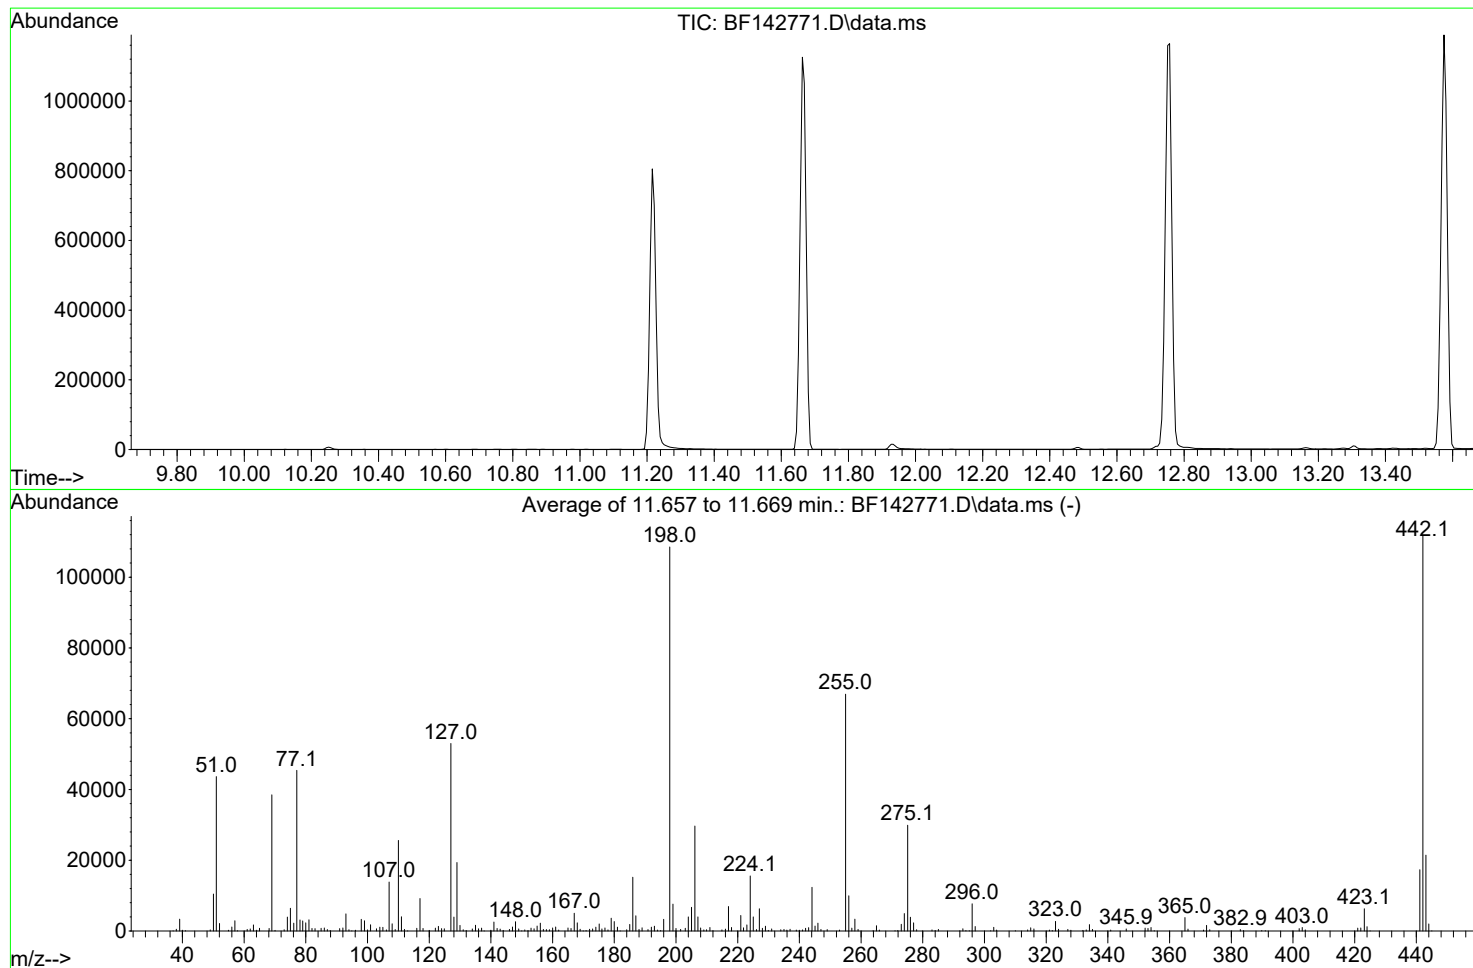

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	706	PASS
69	69	100	100	100.0	38480	PASS
70	69	0.00	2	0.5	203	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108533	PASS
199	198	5	9	7.0	7586	PASS
365	198	1	100	3.5	3821	PASS
441	443	0.01	150	80.8	17318	PASS
442	442	100	100	100.0	111592	PASS
443	442	15	24	19.2	21432	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/18/2025	BNA_F	<u>BF142771.D</u>
Compound Name	Response	Retention Time
DDT	303010	13.574
DDD	4347	13.304
DDE	430	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4777	307787	1.55

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061825\
Data File : BF142771.D
Acq On : 18 Jun 2025 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 13:05:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

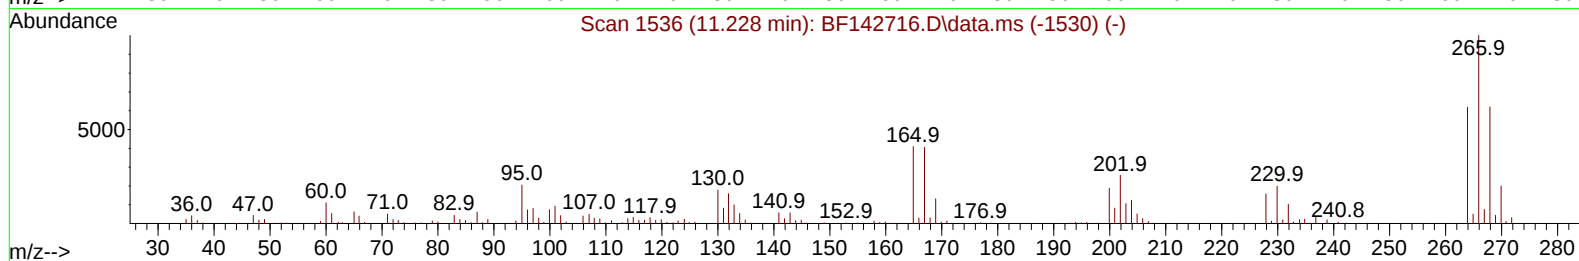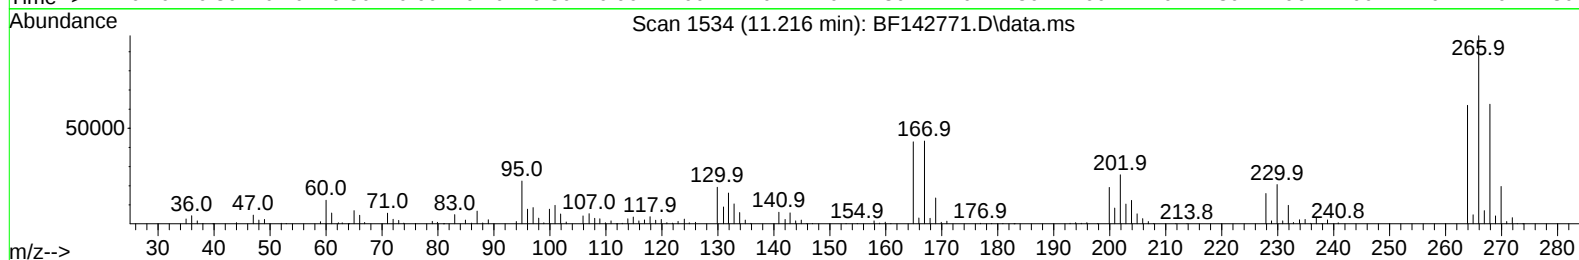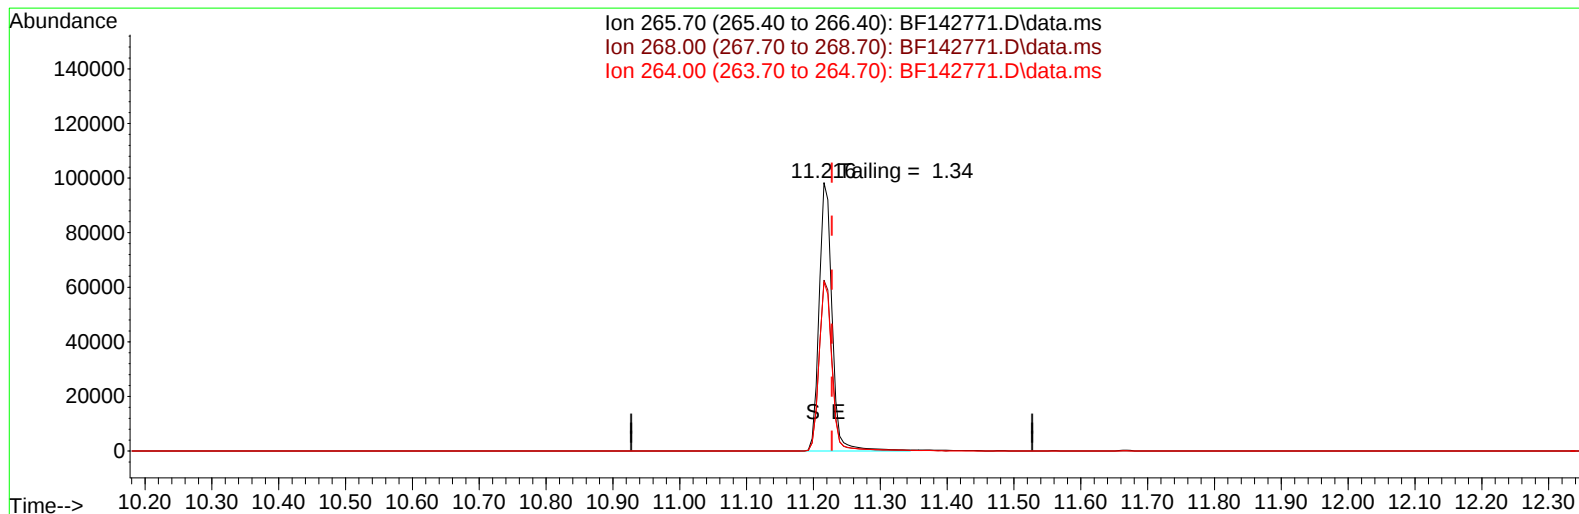

TIC: BF142771.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.012) 34494.01 ng




response 132909

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	63.62
264.00	61.90	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061825\
Data File : BF142771.D
Acq On : 18 Jun 2025 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 13:05:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

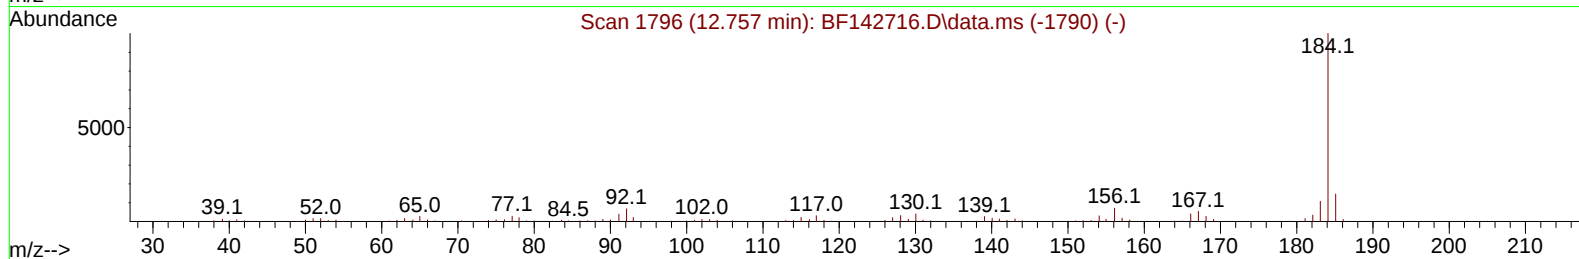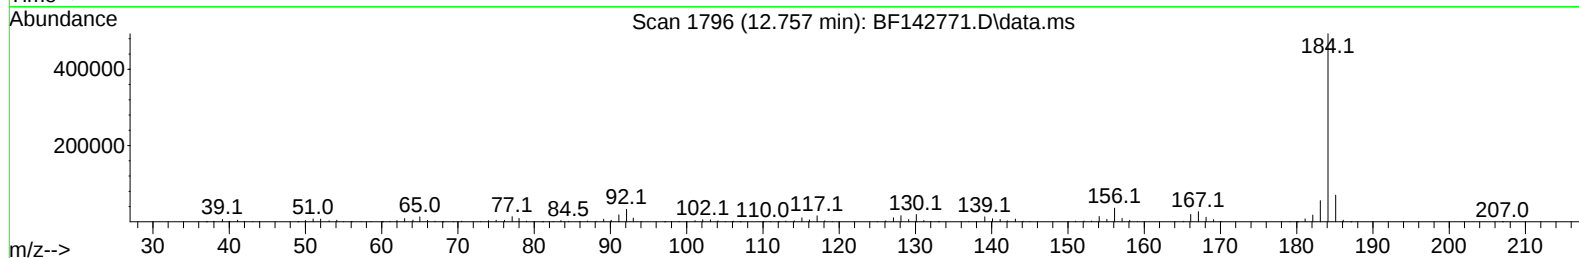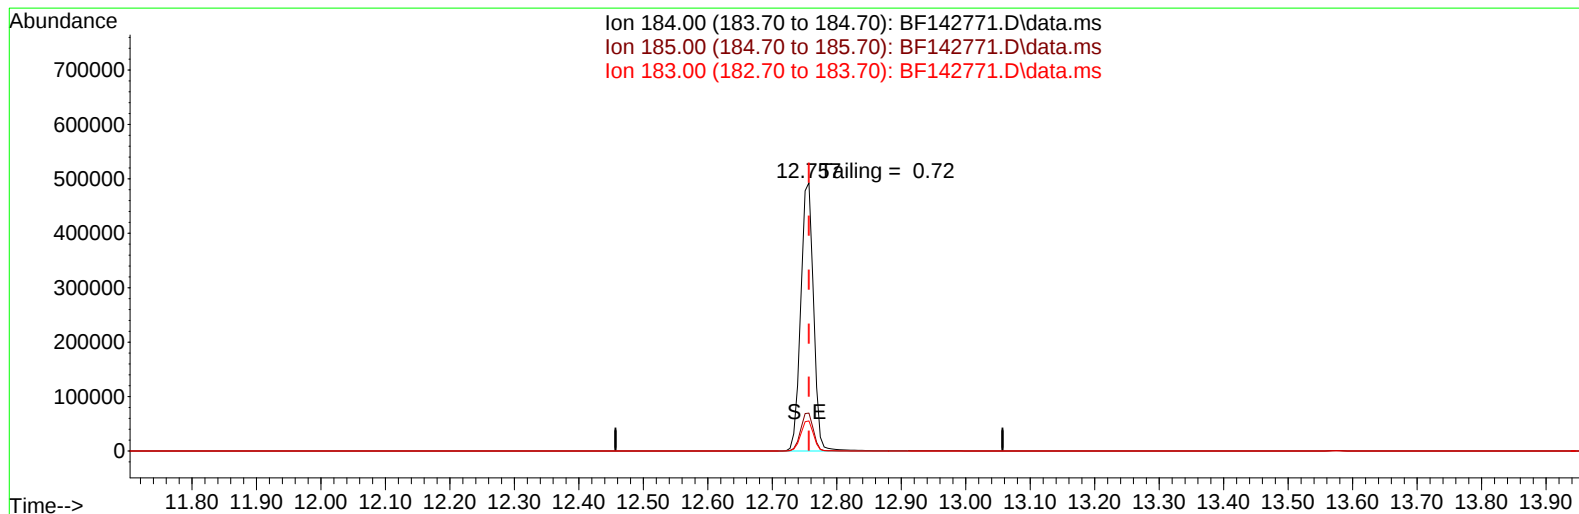

TIC: BF142771.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 680187

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.15
183.00	10.70	11.24
0.00	0.00	0.00