
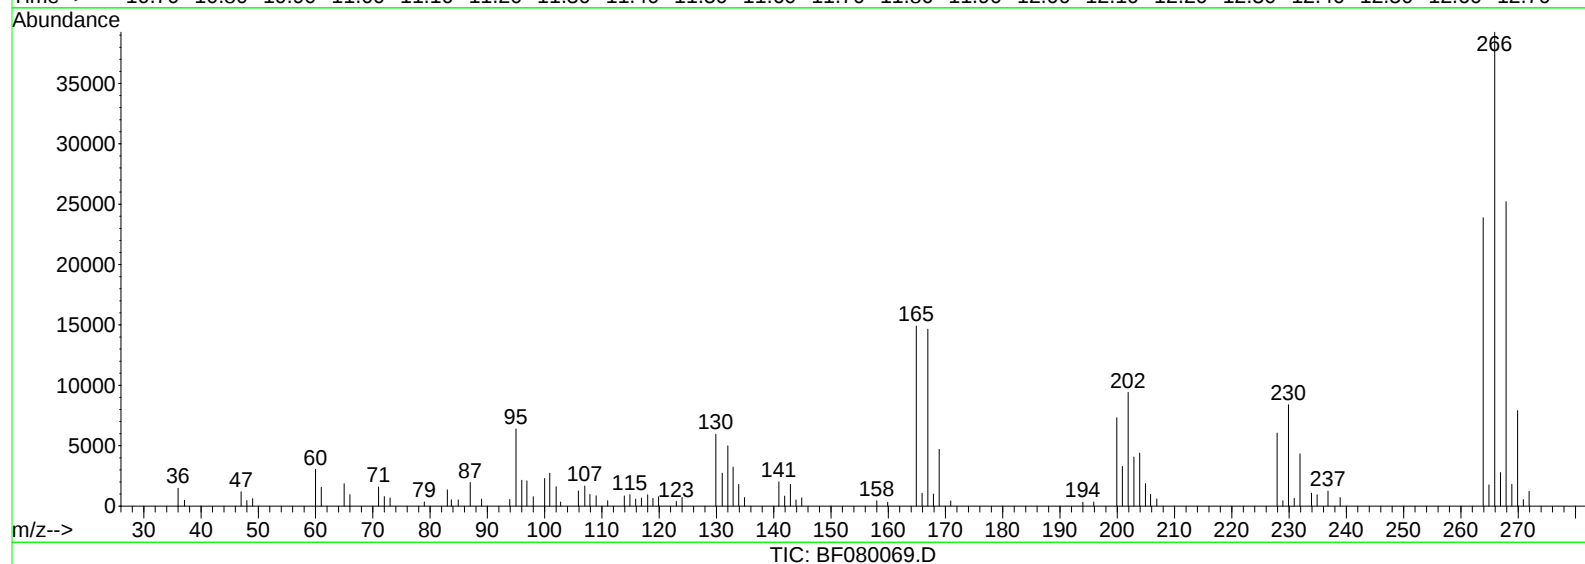


Data Path : Z:\HPCHEM1\BNA F\Data\BF061915\
Data File : BF080069.D
Acq On : 19 Jun 2015 22:48
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 01:52:38 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 17 16:41:53 2015
Response via : Initial Calibration

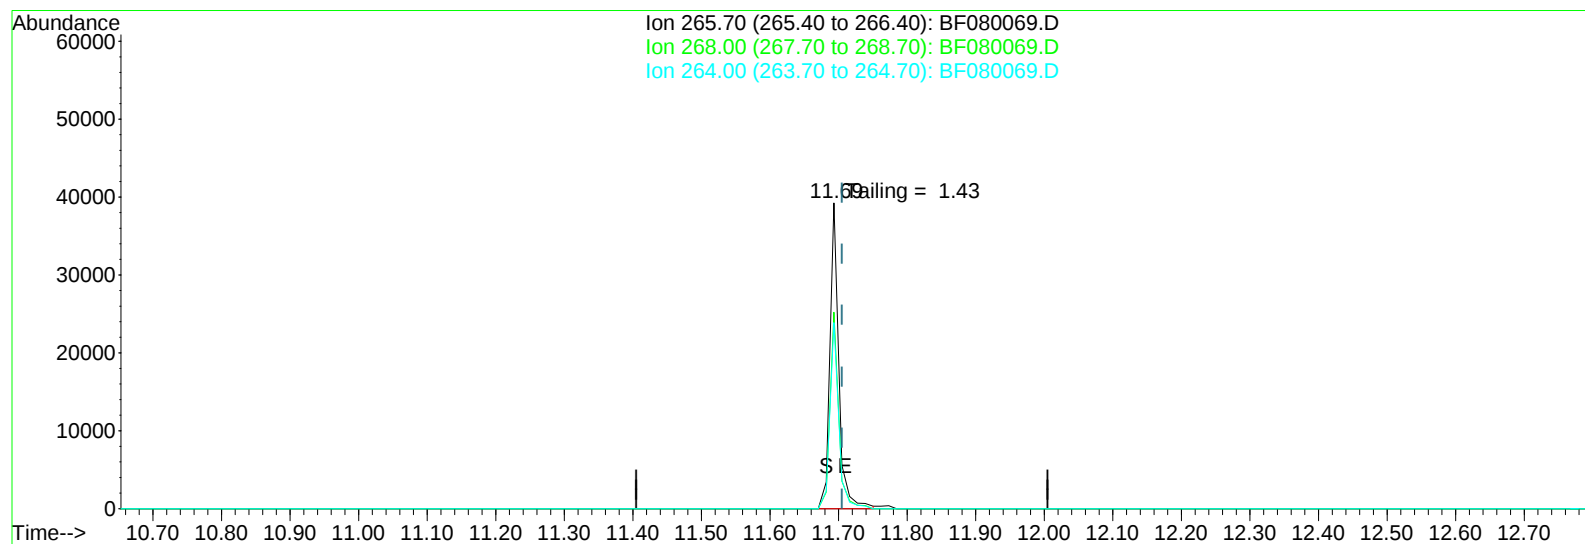

(69) Pentachlorophenol (C)



11.693min (-0.011) 0.00ng

response 35793

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.23
264.00	62.70	60.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF061915\
Data File : BF080069.D
Acq On : 19 Jun 2015 22:48
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 01:52:38 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 17 16:41:53 2015
Response via : Initial Calibration

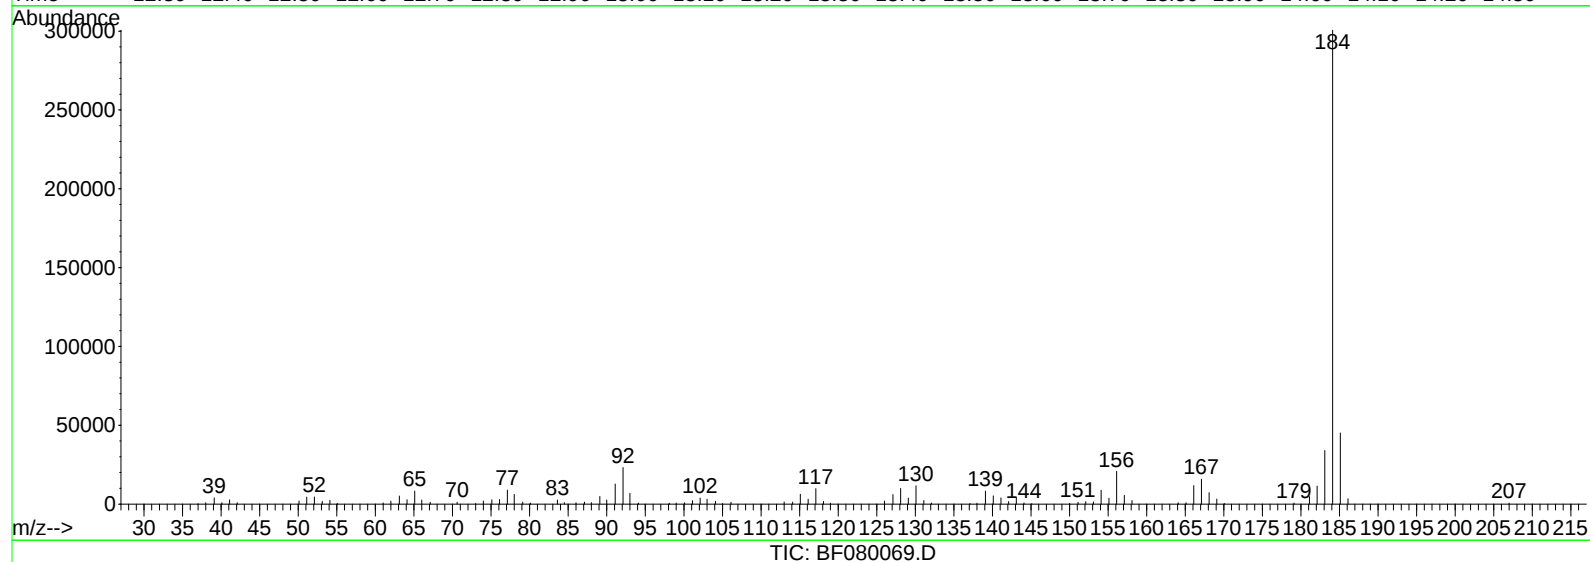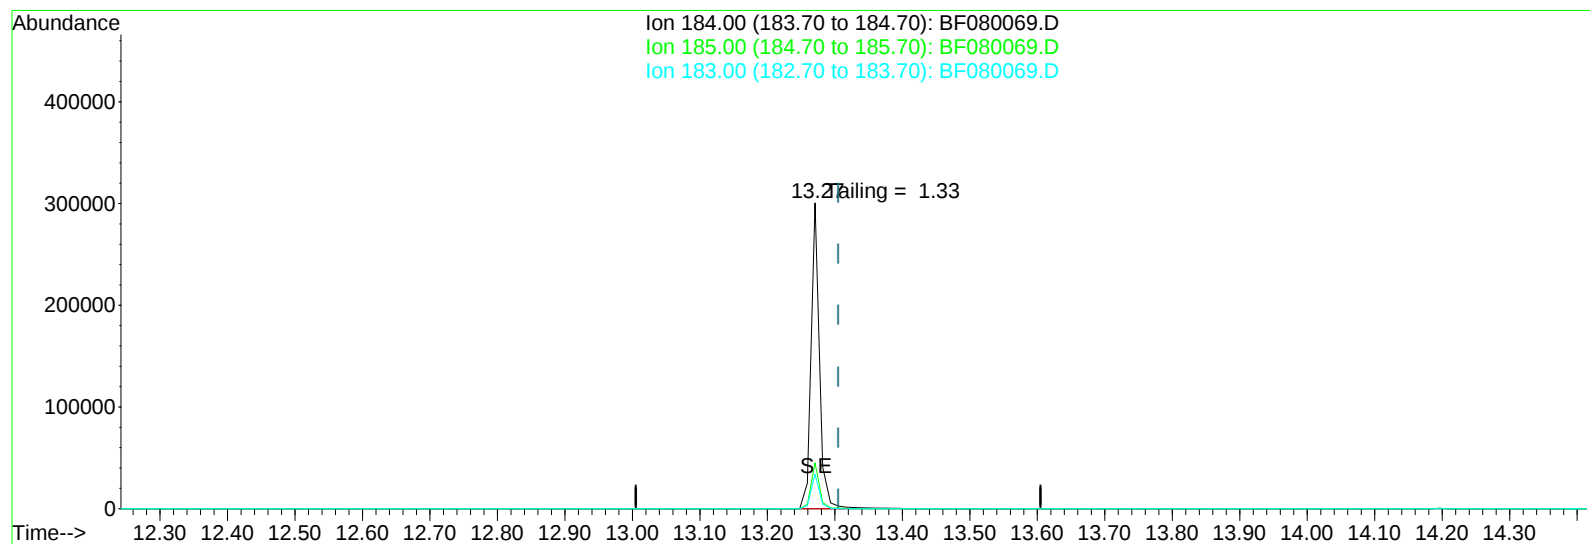

(76) Benzidine

13.271min (-0.034) 18525.11ng

response 261498

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.02
183.00	9.50	11.30
0.00	0.00	0.00