

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061917\
 Data File : BF095998.D
 Acq On : 19 Jun 2017 10:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 19 16:37:44 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 17:12:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-7.32
21) Naphthalene-d8	0.00	136	0	0.00	ng	-9.36
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-12.18
63) Phenanthrene-d10	0.00	188	0	0.00	ng	-14.57
75) Chrysene-d12	0.00	240	0	0.00	ng	-18.30
86) Perylene-d12	0.00	264	0	0.00	ng	-19.96
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
78) Terphenyl-d14	0.00	244	0	0.00	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061917\
Data File : BF095998.D
Acq On : 19 Jun 2017 10:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jun 19 16:37:44 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

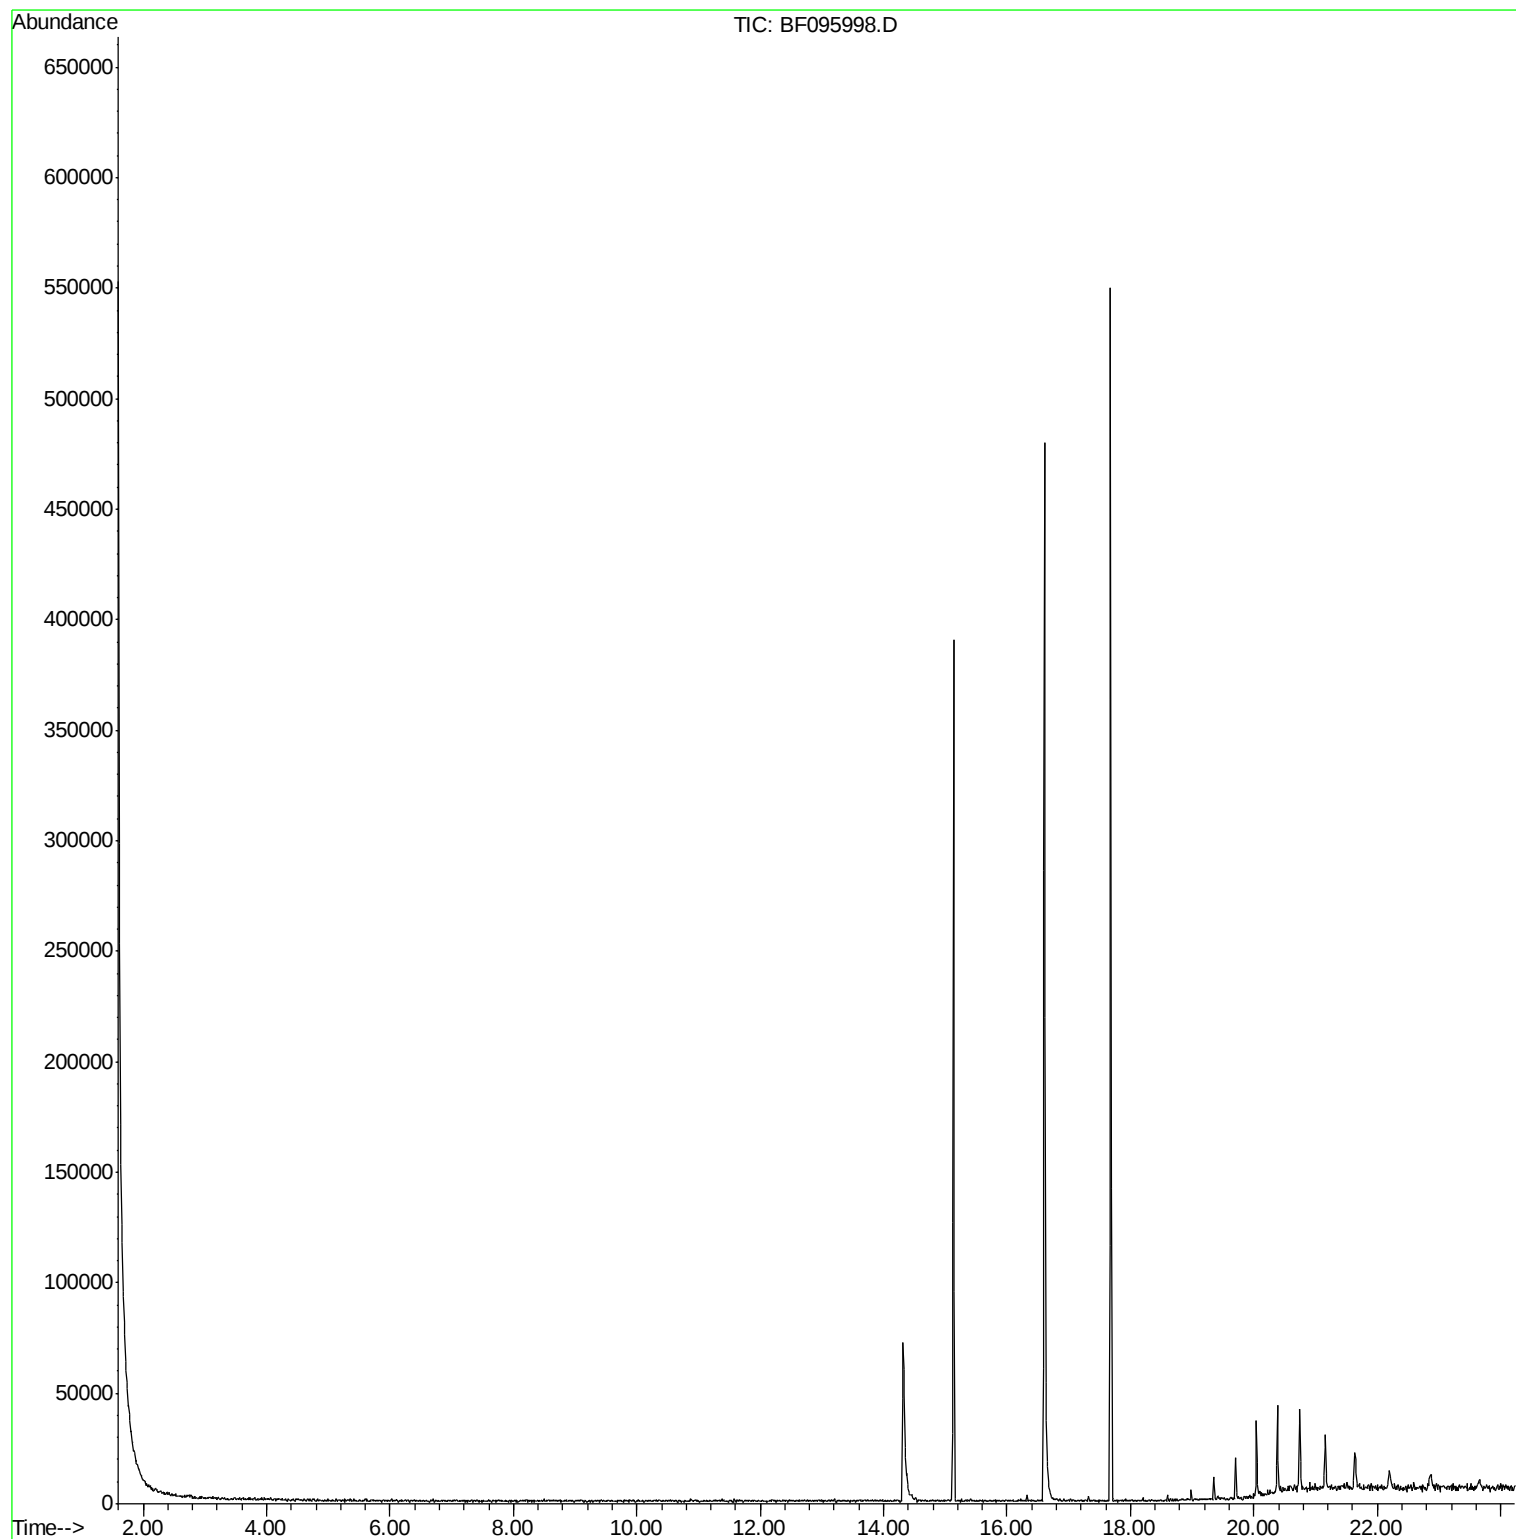


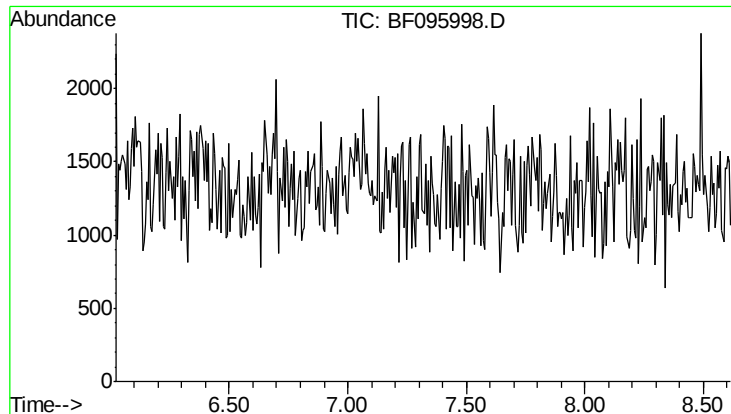


#1
1,4-Dichlorobenzene-d4
Concen: 0.00 ng
Expected RT: 7.32 min

Lab File: BF095998.D
Acq: 19 Jun 2017 10:41

Instrument :
BNA_F
ClientSampleId :


Tot Ion:	152
Sig	Exp Ratio
152	100
150	157.7
115	65.2

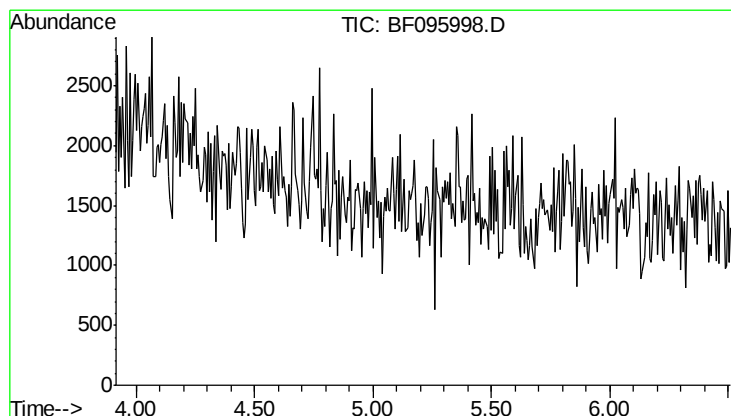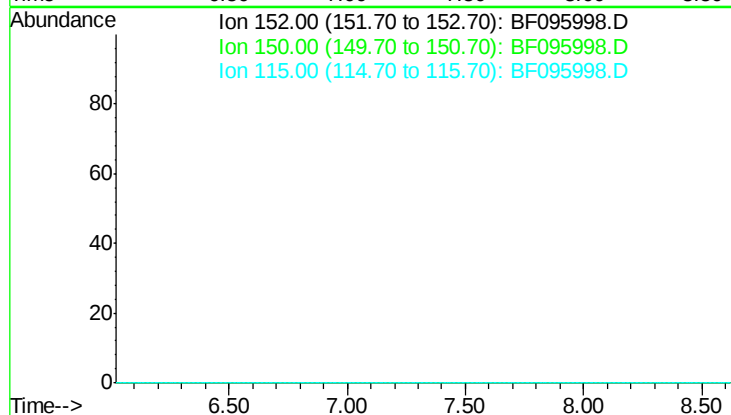


#5
2-Fluorophenol
Concen: 0.00 ng
Expected RT: 5.22 min

Lab File: BF095998.D
Acq: 19 Jun 2017 10:41

Tgt Ion:	112
Sig	Exp Ratio
112	100
64	57.5
63	29.2

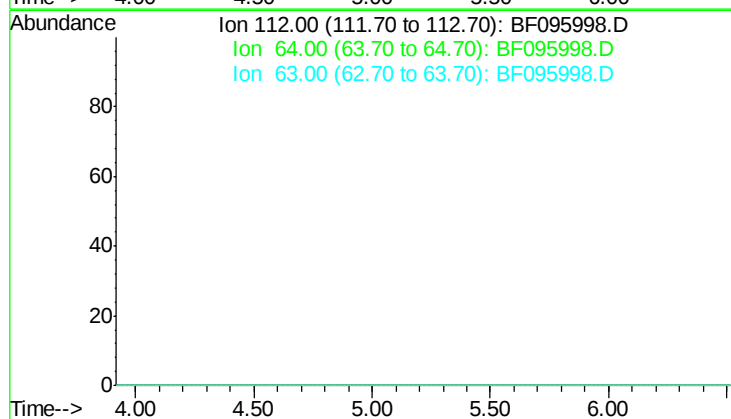

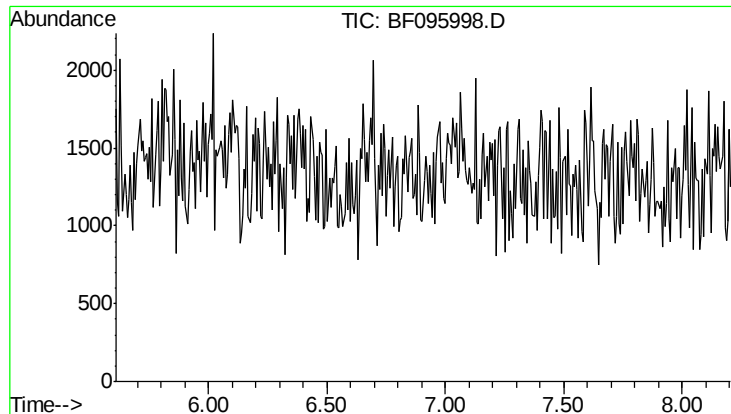

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 6.91 min

Lab File: BF095998.D

Acq: 19 Jun 2017 10:41

Instrument :

BNA_F

ClientSampleId :



Tot Ion: 99

Sig Exp Ratio

99 100

42 16.9

71 30.6

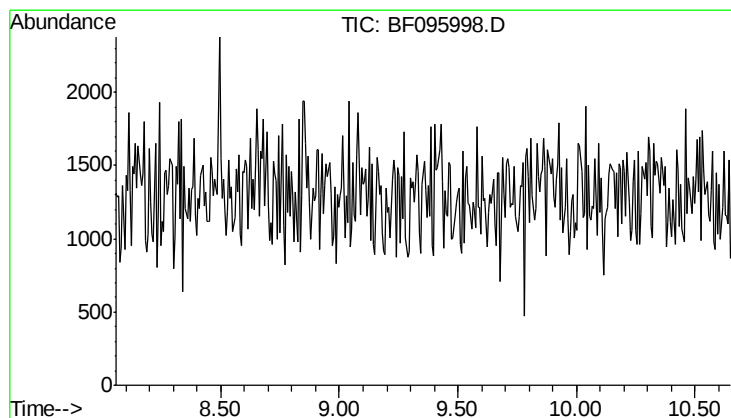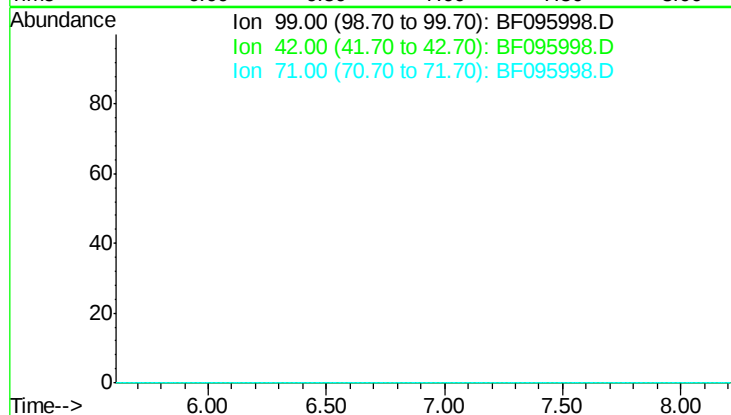

#21

Naphthalene-d8

Concen: 0.00 ng

Expected RT: 9.36 min

Lab File: BF095998.D

Acq: 19 Jun 2017 10:41

Tgt Ion: 136


Sig Exp Ratio


136 100

137 10.6

54 6.1

68 5.1


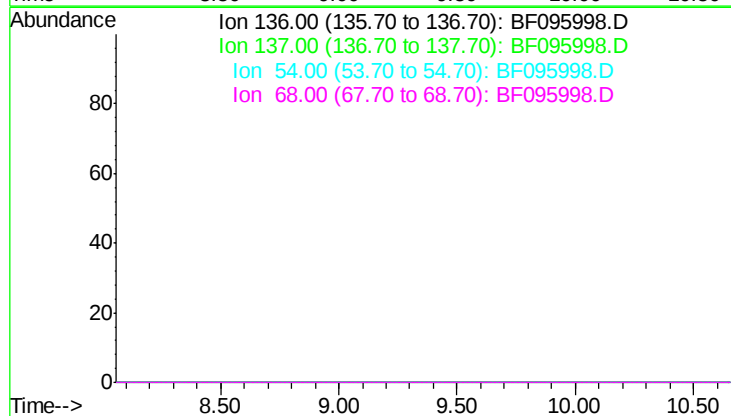


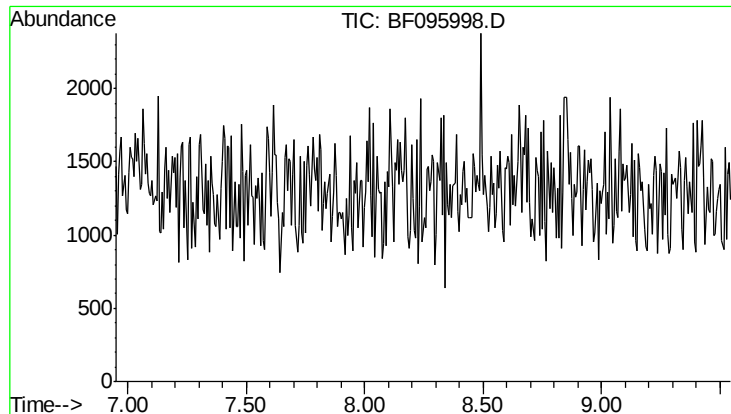

#23
 Nitrobenzene-d5
 Concen: 0.00 ng
 Expected RT: 8.25 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41


Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	82
Sig	Exp Ratio
82	100
128	42.5
54	52.7

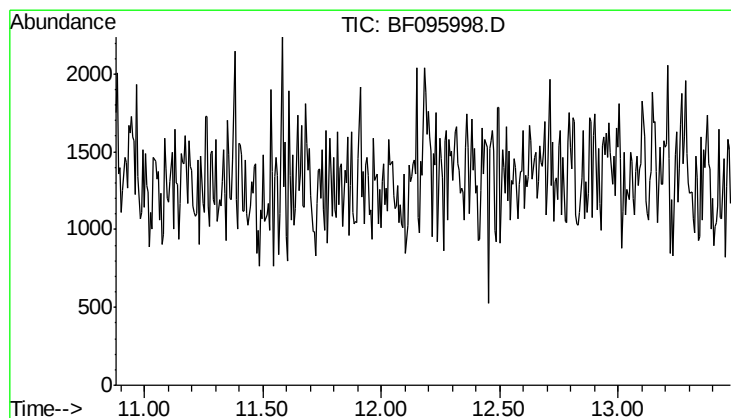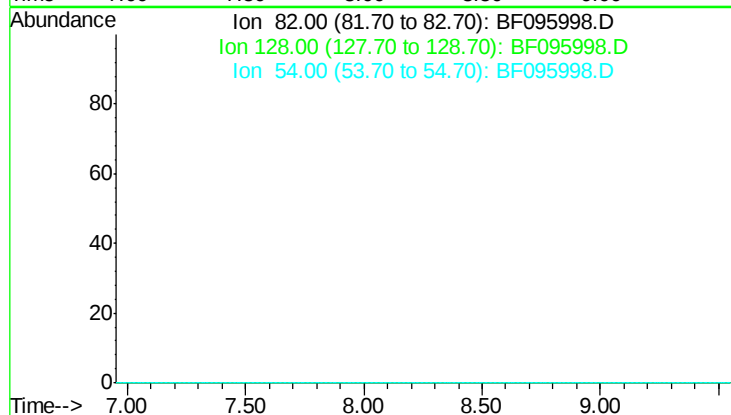

#38
 Acenaphthene-d10
 Concen: 0.00 ng
 Expected RT: 12.18 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41

Tgt Ion	164
Sig	Exp Ratio
164	100
162	103.2
160	45.2


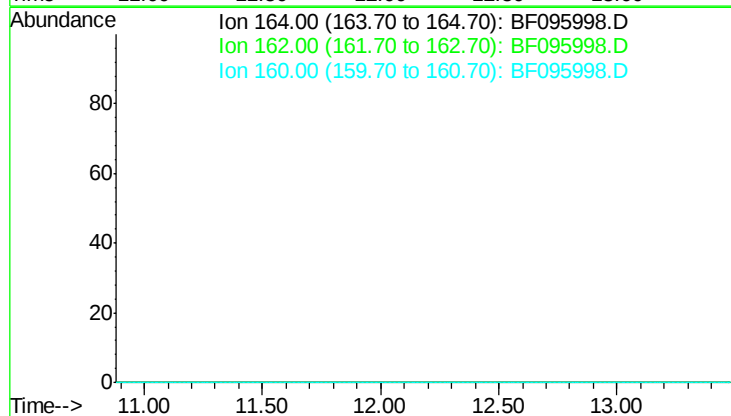


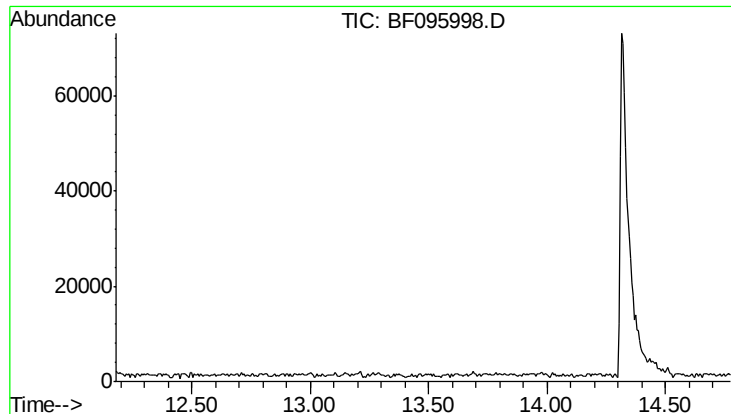

#41
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 13.48 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41


Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	330	332	141
Sig	100	95.8	39.3
Exp Ratio			

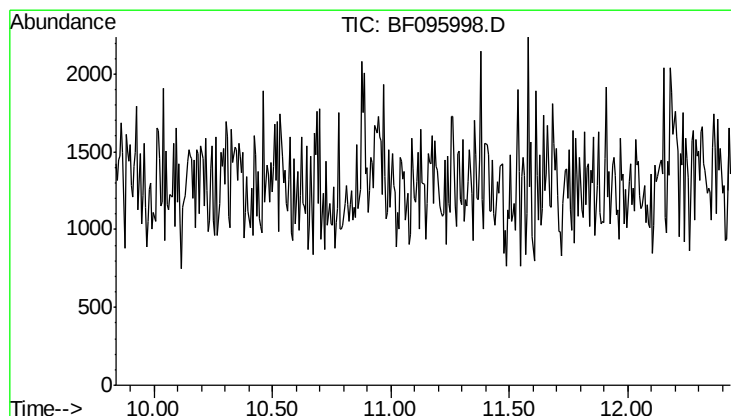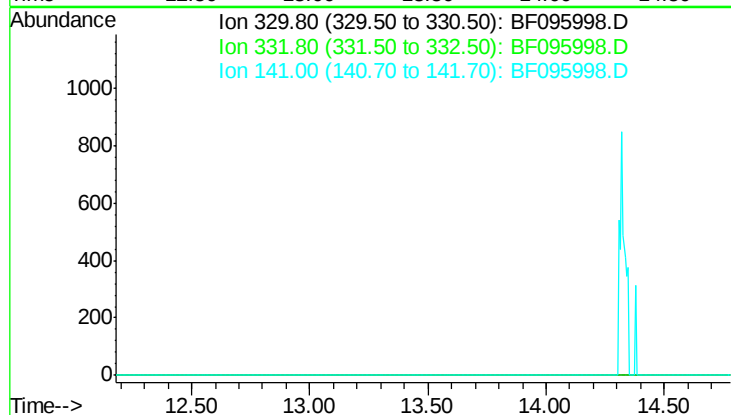

#44
 2-Fluorobiphenyl
 Concen: 0.00 ng
 Expected RT: 11.14 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41

Tgt Ion	172	171	170
Sig	100	37.0	24.8
Exp Ratio			


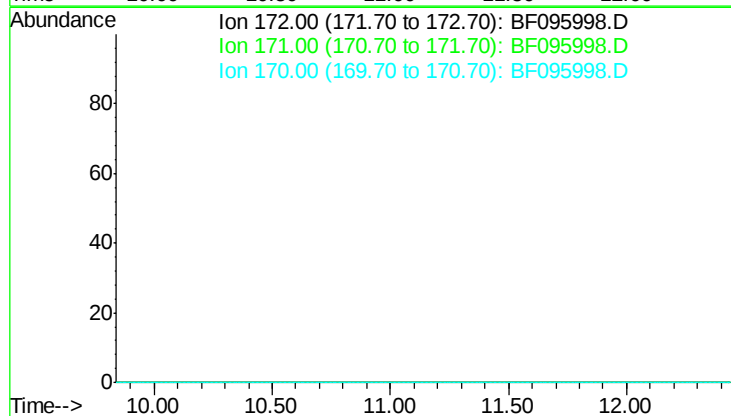


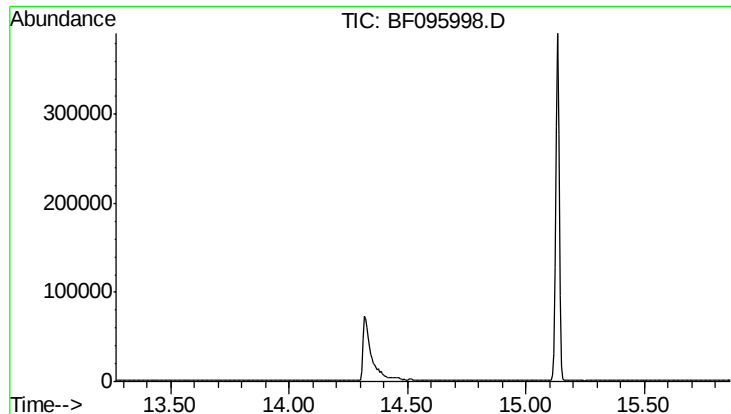

#63
 Phenanthrene-d10
 Concen: 0.00 ng
 Expected RT: 14.57 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41


Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	188
Sig	Exp Ratio
188	100
94	11.8
80	12.7

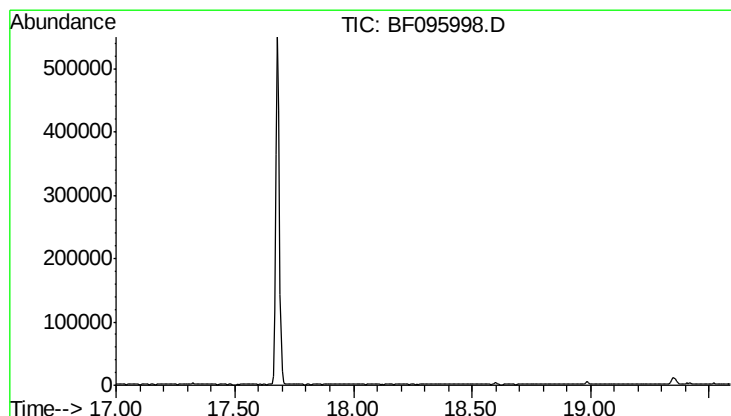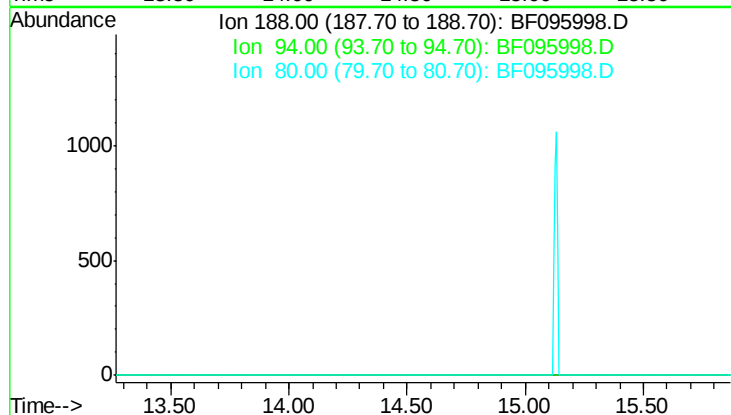

#75
 Chrysene-d12
 Concen: 0.00 ng
 Expected RT: 18.30 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41

Tgt Ion	240
Sig	Exp Ratio
240	100
120	7.3
236	25.6


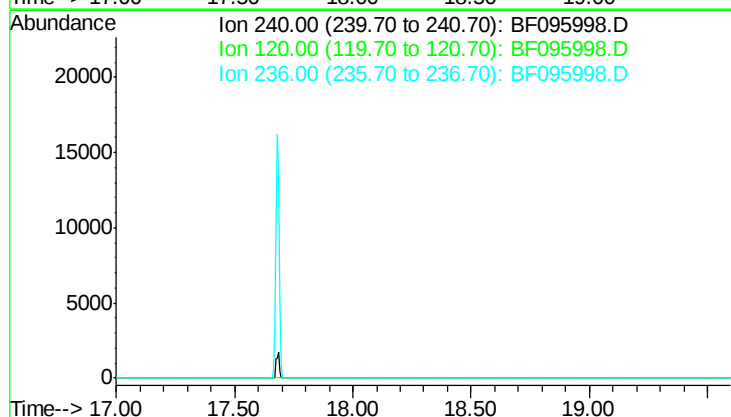


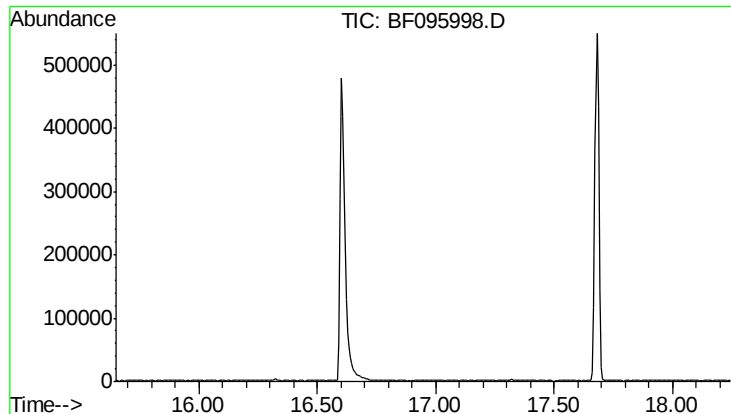

#78
 Terphenyl-d14
 Concen: 0.00 ng
 Expected RT: 16.95 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion: 244
 Sig Exp Ratio
 244 100
 212 7.5
 122 12.9

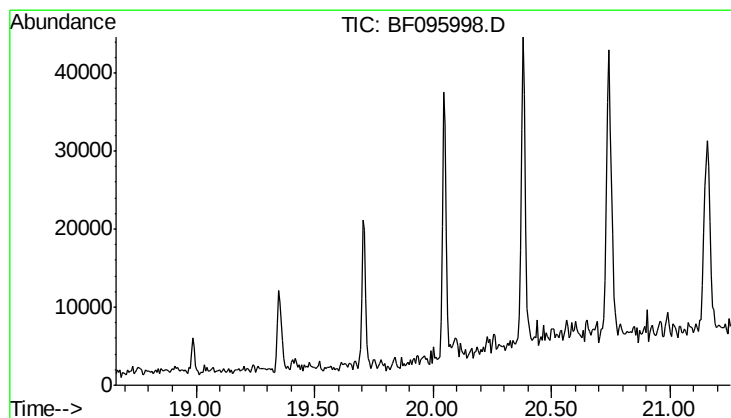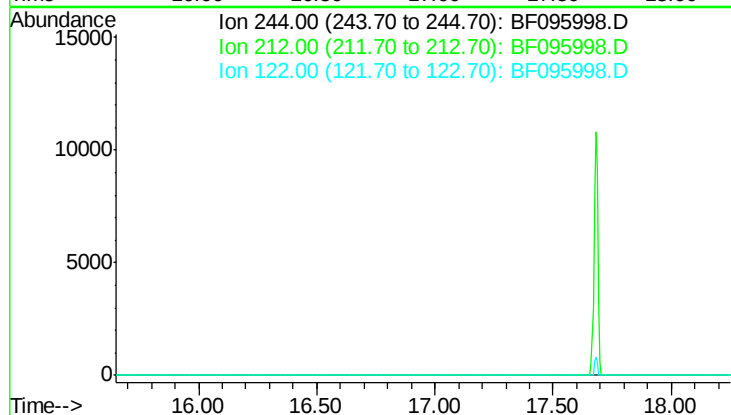

#86
 Perylene-d12
 Concen: 0.00 ng
 Expected RT: 19.96 min
 Lab File: BF095998.D
 Acq: 19 Jun 2017 10:41

Tgt Ion: 264
 Sig Exp Ratio
 264 100
 260 24.4
 265 21.5

