

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061917\
 Data File : BF096001.D
 Acq On : 19 Jun 2017 12:25
 Operator : SJ/MA
 Sample : PB99832BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB99832BL

Quant Time: Jun 19 16:53:05 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 17:12:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.30	152	70449	20.00	ng	-0.02
21) Naphthalene-d8	9.33	136	298553	20.00	ng	-0.02
38) Acenaphthene-d10	12.15	164	138592	20.00	ng	-0.03
63) Phenanthrene-d10	14.54	188	261143	20.00	ng	-0.02
75) Chrysene-d12	18.27	240	195173	20.00	ng	-0.02
86) Perylene-d12	19.95	264	135946	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.20	112	589464	133.33	ng	-0.01
7) Phenol-d6	6.87	99	709299	134.01	ng	-0.04
23) Nitrobenzene-d5	8.22	82	410332	85.36	ng	-0.03
41) 2,4,6-Tribromophenol	13.45	330	143548	117.07	ng	-0.03
44) 2-Fluorobiphenyl	11.12	172	846840	85.03	ng	-0.02
78) Terphenyl-d14	16.93	244	707079	89.91	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061917\
Data File : BF096001.D
Acq On : 19 Jun 2017 12:25
Operator : SJ/MA
Sample : PB99832BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB99832BL

Quant Time: Jun 19 16:53:05 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

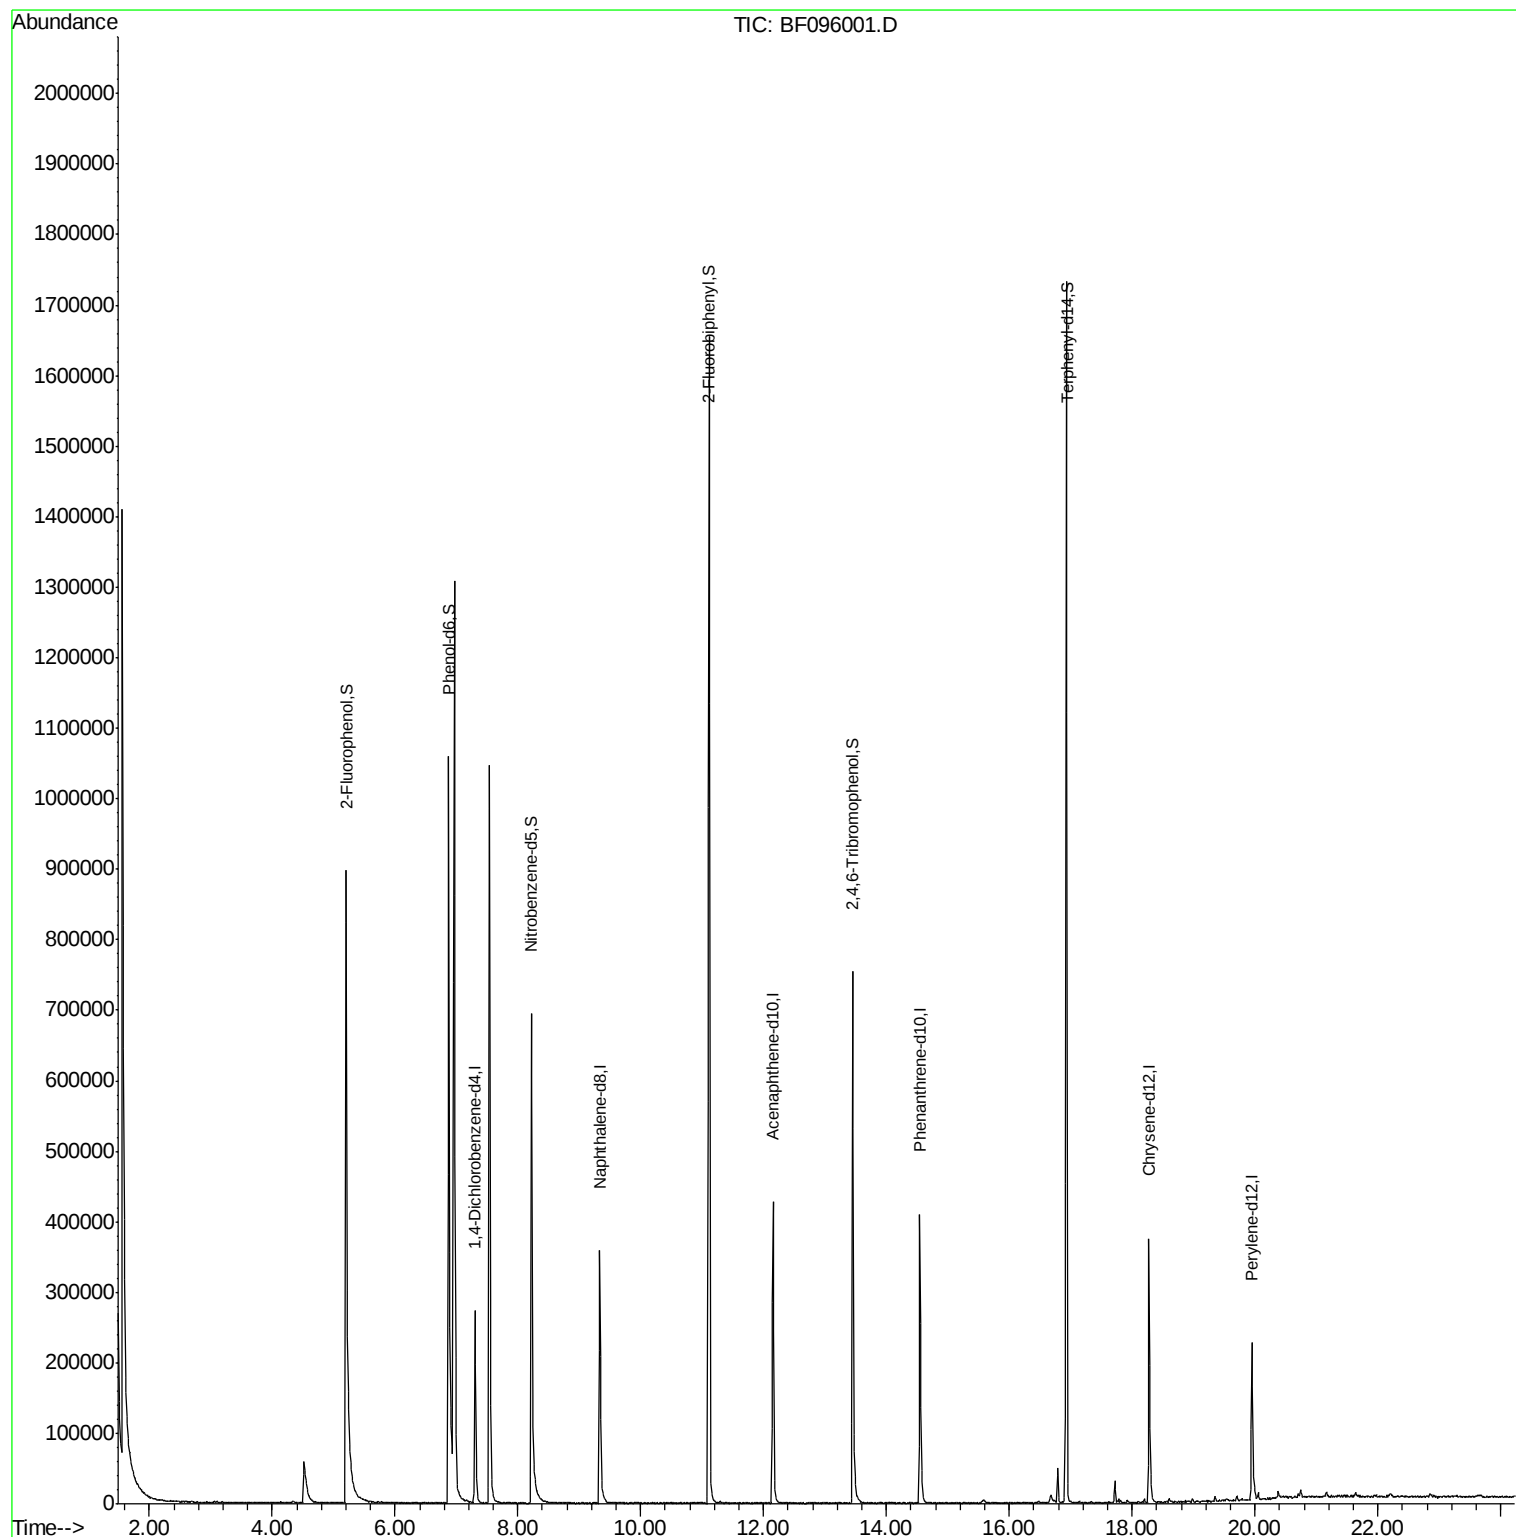




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.30 min Scan# 989
Delta R.T. -0.02 min
Lab File: BF096001.D
Acq: 19 Jun 2017 12:25

Instrument :
BNA_F
ClientSampleId :
PB99832BL

Tot Ion:152 Resp: 70449
Ion Ratio Lower Upper
152 100
150 160.8 126.2 189.2
115 59.6 52.2 78.2

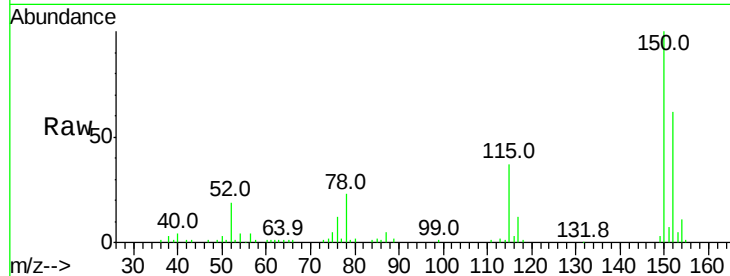


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

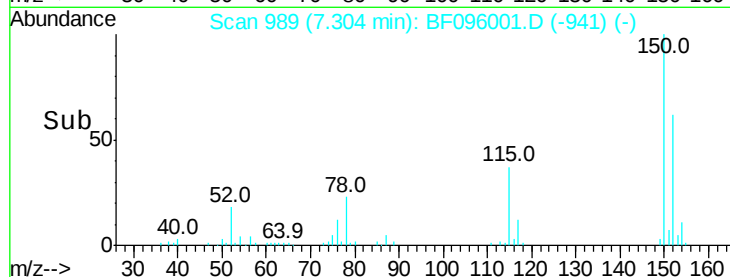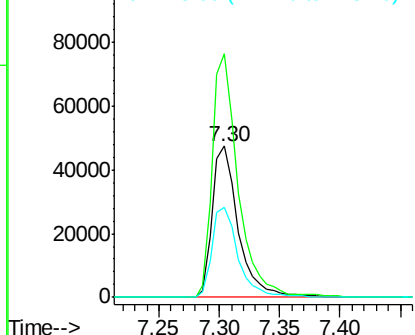



#5


2-Fluorophenol
Concen: 133.33 ng
RT: 5.20 min Scan# 632
Delta R.T. -0.01 min
Lab File: BF096001.D
Acq: 19 Jun 2017 12:25

Tgt Ion:112 Resp: 589464
Ion Ratio Lower Upper
112 100
64 53.2 46.0 69.0
63 26.1 23.4 35.0

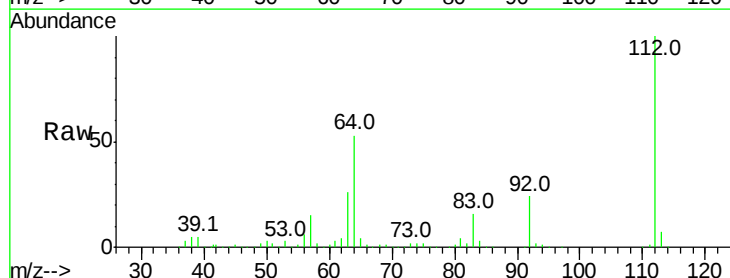

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

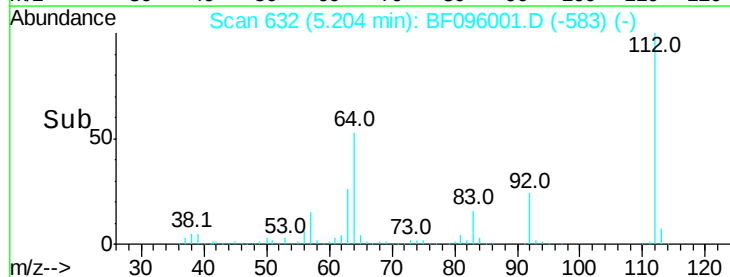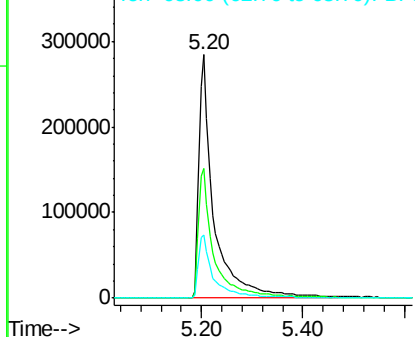

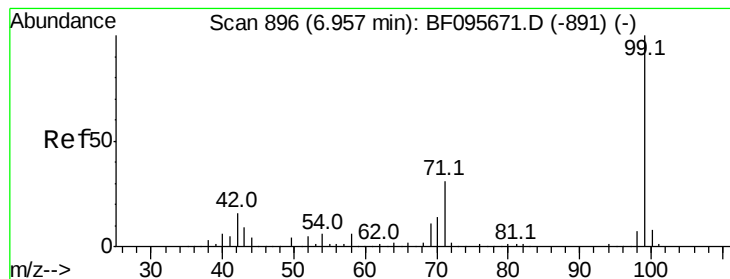

#7

Phenol-d6

Concen: 134.01 ng

RT: 6.87 min Scan# 916

Delta R.T. -0.04 min

Lab File: BF096001.D

Acq: 19 Jun 2017 12:25

Instrument :

BNA_F

ClientSampleID :

PB99832BL


Tot Ion: 99 Resp: 709299

Ion Ratio Lower Upper

99 100

42 16.5 13.5 20.3




71 32.2 24.5 36.7

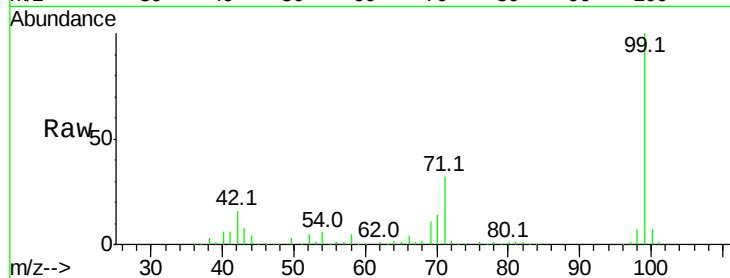

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

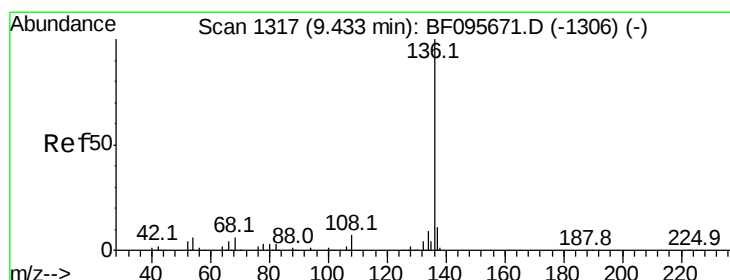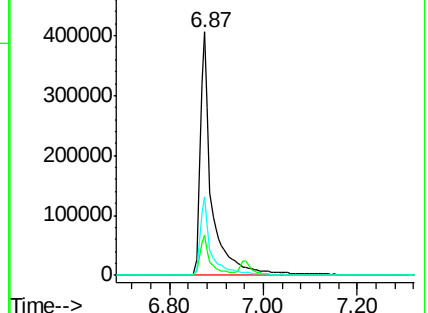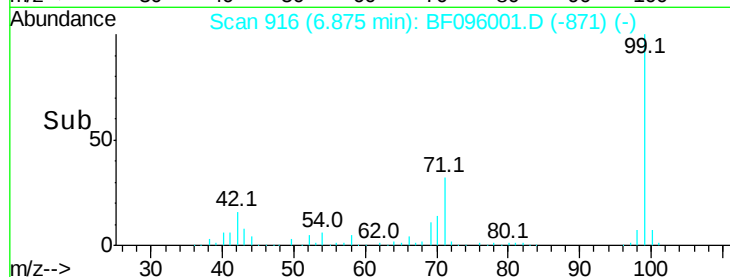

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.33 min Scan# 1334

Delta R.T. -0.02 min

Lab File: BF096001.D

Acq: 19 Jun 2017 12:25

Tgt Ion: 136 Resp: 298553


Ion Ratio Lower Upper

136 100

137 11.5 8.5 12.7

54 6.4 4.9 7.3

68 5.8 4.1 6.1


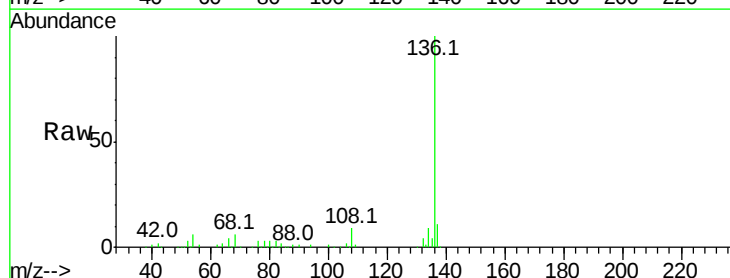


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



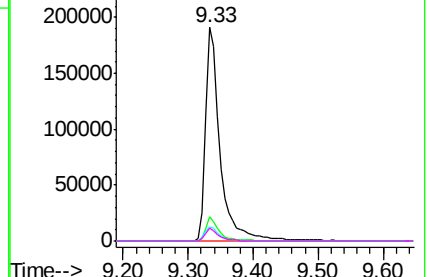
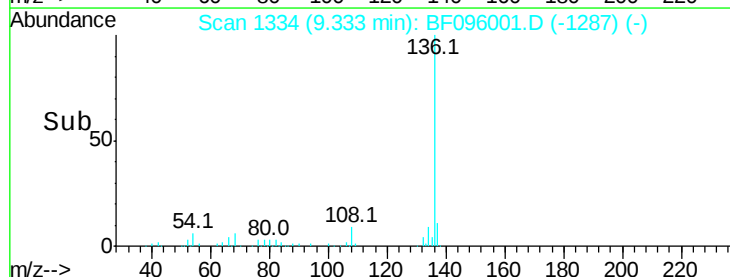




#23
Nitrobenzene-d5
Concen: 85.36 ng
RT: 8.22 min Scan# 1145
Delta R.T. -0.03 min
Lab File: BF096001.D
Acq: 19 Jun 2017 12:25




Instrument :
BNA_F
ClientSampleId :
PB99832BL

Tot Ion: 82 Resp: 410332
Ion Ratio Lower Upper
82 100
128 47.0 34.0 51.0
54 47.1 42.2 63.2

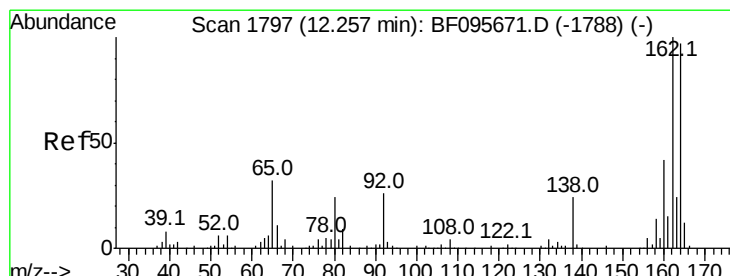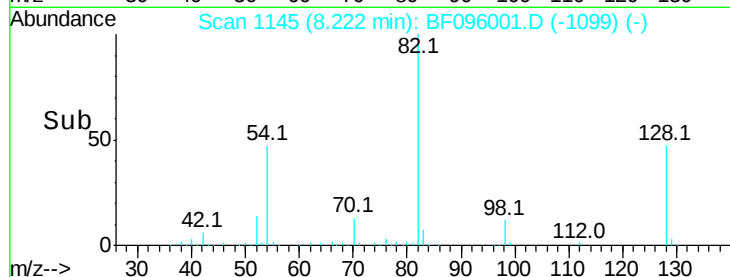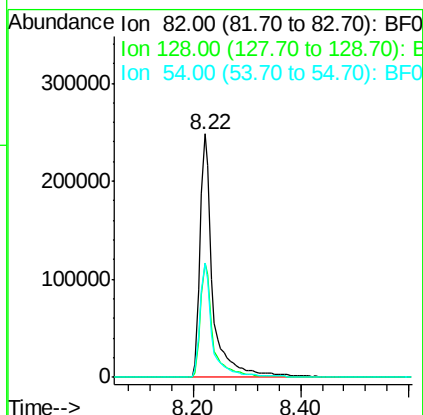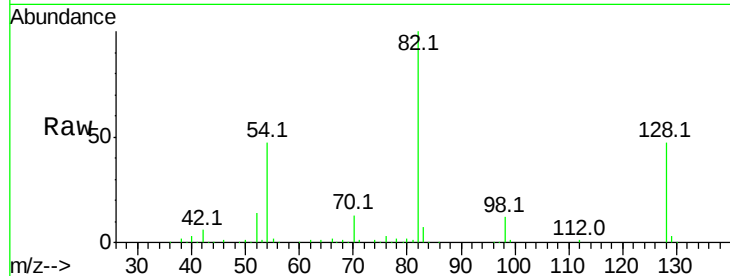

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.15 min Scan# 1813
Delta R.T. -0.03 min
Lab File: BF096001.D
Acq: 19 Jun 2017 12:25

Tgt Ion:164 Resp: 138592
Ion Ratio Lower Upper
164 100
162 104.2 82.6 123.8
160 44.2 36.2 54.2

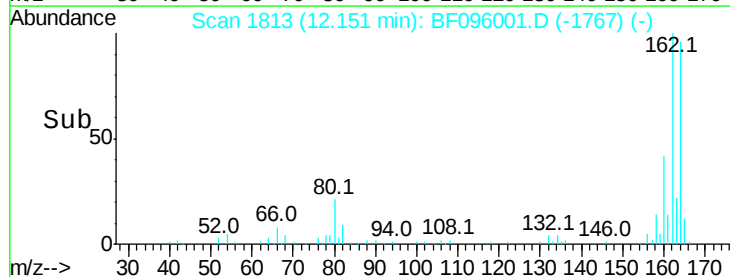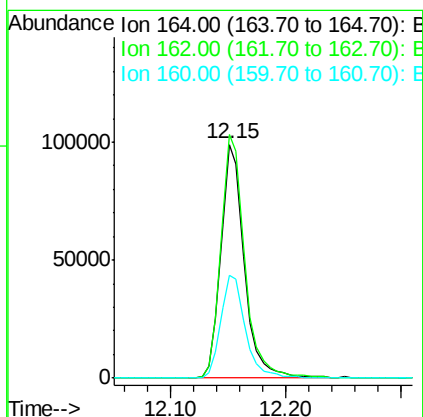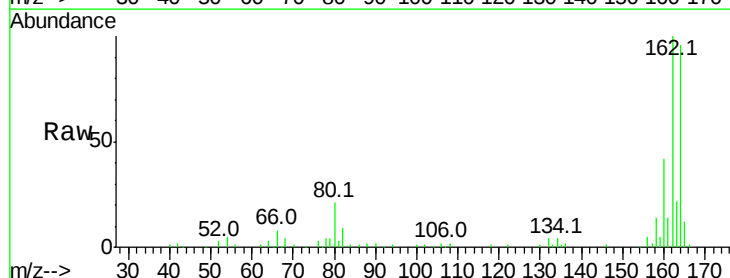






#41
 2,4,6-Tribromophenol
 Concen: 117.07 ng
 RT: 13.45 min Scan# 2034
 Delta R.T. -0.03 min
 Lab File: BF096001.D
 Acq: 19 Jun 2017 12:25

Instrument :
 BNA_F
 ClientSampleId :
 PB99832BL

Tot Ion:330 Resp: 143548
 Ion Ratio Lower Upper
 330 100
 332 96.3 76.6 115.0
 141 39.3 31.4 47.2

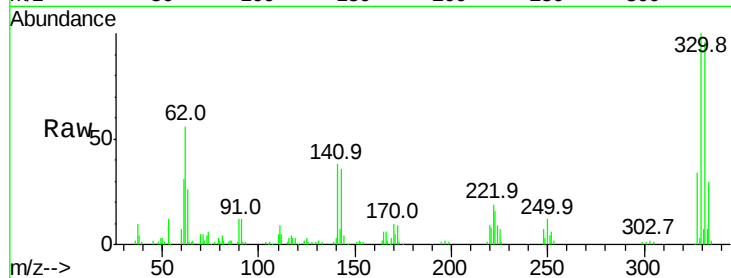


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

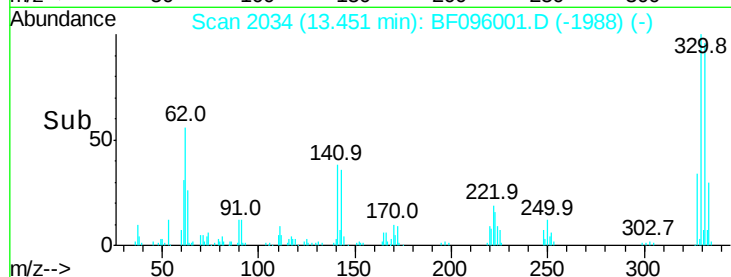
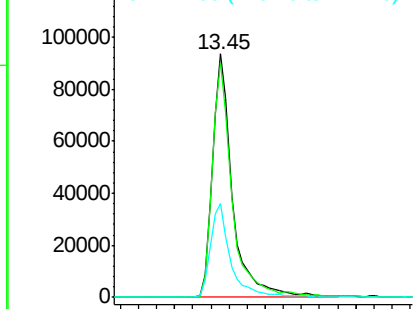



#44
 2-Fluorobiphenyl
 Concen: 85.03 ng
 RT: 11.12 min Scan# 1637
 Delta R.T. -0.02 min
 Lab File: BF096001.D
 Acq: 19 Jun 2017 12:25

Tgt Ion:172 Resp: 846840
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.6 44.4
 170 23.5 19.8 29.8

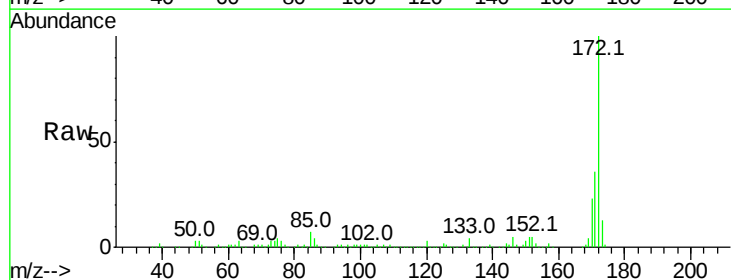

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


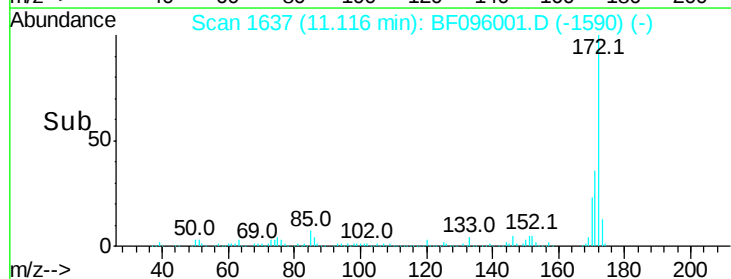
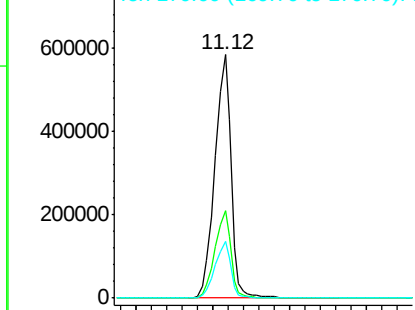


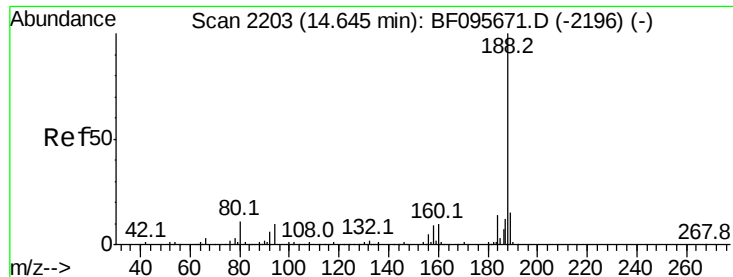

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.54 min Scan# 2220
Delta R.T. -0.02 min
Lab File: BF096001.D
Acq: 19 Jun 2017 12:25




Instrument :
BNA_F
ClientSampleId :
PB99832BL


Tot Ion:188 Resp: 261143
Ion Ratio Lower Upper
188 100
94 10.5 9.4 14.2
80 11.2 10.2 15.2

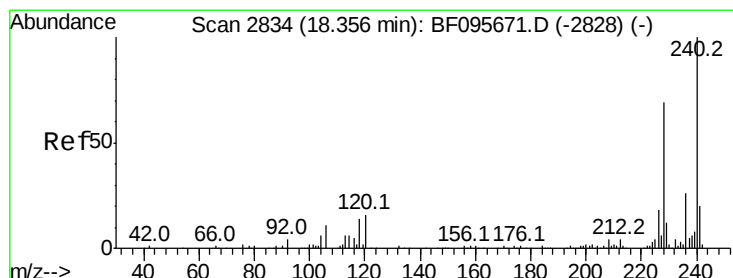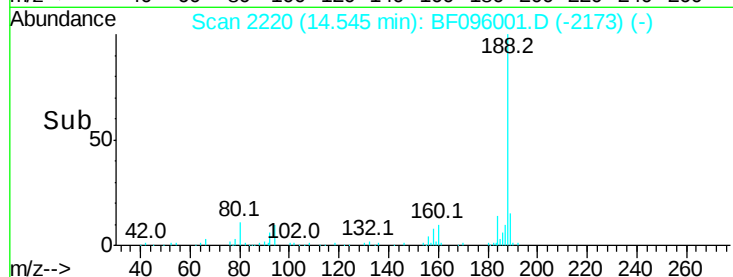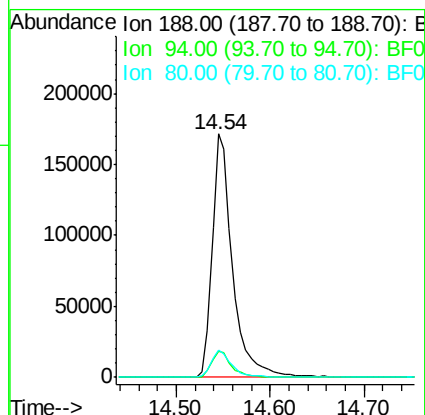

#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.27 min Scan# 2854
Delta R.T. -0.02 min
Lab File: BF096001.D
Acq: 19 Jun 2017 12:25

Tgt Ion:240 Resp: 195173
Ion Ratio Lower Upper
240 100
120 14.8 5.8 8.8#
236 24.9 20.5 30.7

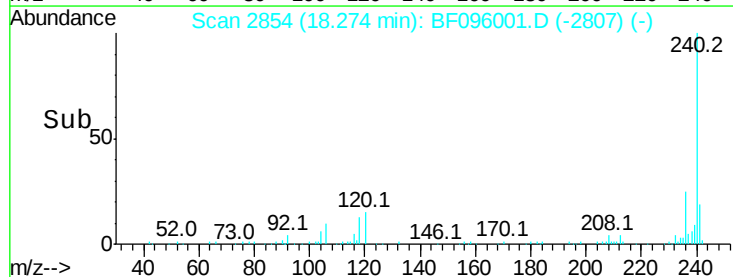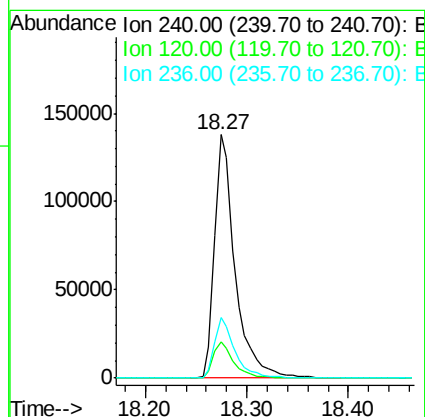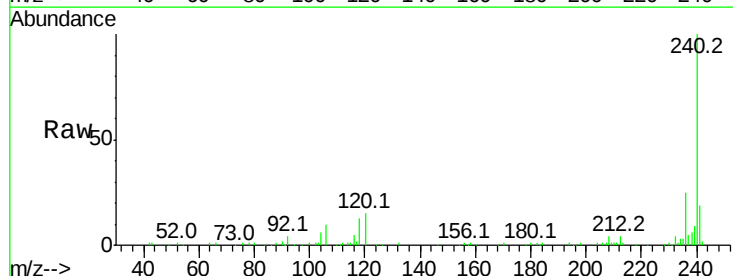


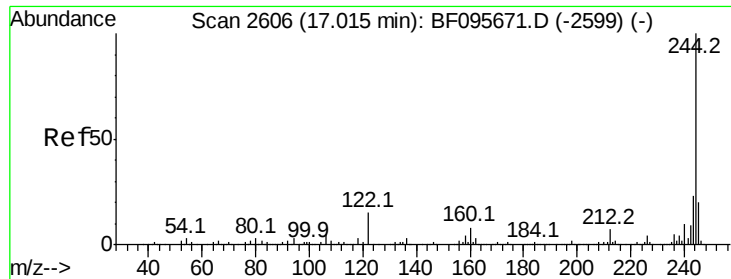




#78
 Terphenyl-d14
 Concen: 89.91 ng
 RT: 16.93 min Scan# 2626
 Delta R.T. -0.02 min
 Lab File: BF096001.D
 Acq: 19 Jun 2017 12:25

Instrument :
 BNA_F
 ClientSampleId :
 PB99832BL

Tot Ion:244 Resp: 707079
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 14.2 10.3 15.5

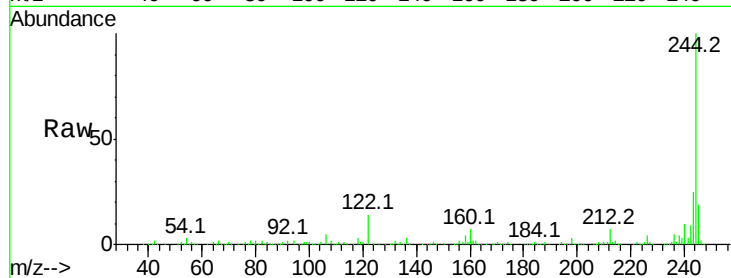


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

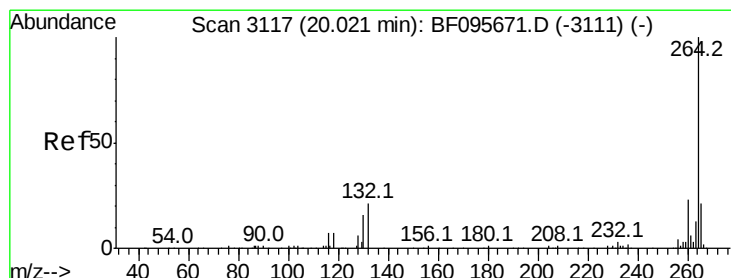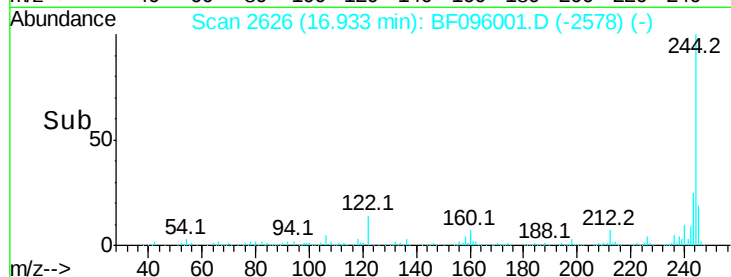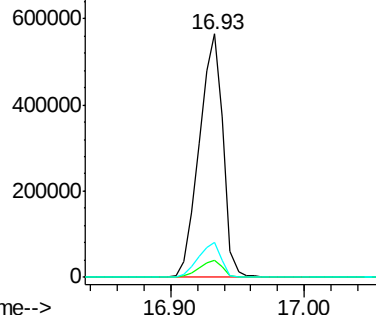

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 19.95 min Scan# 3139
 Delta R.T. -0.01 min
 Lab File: BF096001.D
 Acq: 19 Jun 2017 12:25

Tgt Ion:264 Resp: 135946
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.5 29.3
 265 22.3 17.2 25.8

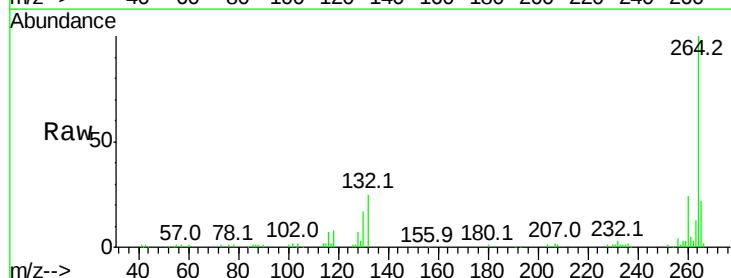

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

