

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
 Data File : BF096038.D
 Acq On : 20 Jun 2017 10:39
 Operator : SJ/MA
 Sample : I3688-01 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G23-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	10	13	39	rBV	902222	1735163	100.00%	35.823%
2	6.981	929	934	936	rBV3	14294	23592	1.36%	0.487%
3	7.010	936	939	949	rVV4	35743	86902	5.01%	1.794%
4	7.304	986	989	1006	rBV	284086	428001	24.67%	8.836%
5	7.551	1027	1031	1042	rBV	56007	90189	5.20%	1.862%
6	9.339	1331	1335	1355	rBV	387363	538028	31.01%	11.108%
7	11.121	1634	1638	1654	rBV	81856	113560	6.54%	2.344%
8	12.163	1810	1815	1827	rBV2	355752	490826	28.29%	10.133%
9	14.557	2218	2222	2238	rVB	292348	422501	24.35%	8.723%
10	16.845	2604	2611	2619	rBV2	16318	37700	2.17%	0.778%
11	16.933	2623	2626	2631	rBV	105159	114197	6.58%	2.358%
12	18.286	2852	2856	2863	rBV	377482	463735	26.73%	9.574%
13	19.962	3137	3141	3146	rBV	249221	299382	17.25%	6.181%


Sum of corrected areas: 4843776

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
Data File : BF096038.D
Acq On : 20 Jun 2017 10:39
Operator : SJ/MA
Sample : I3688-01 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G23-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

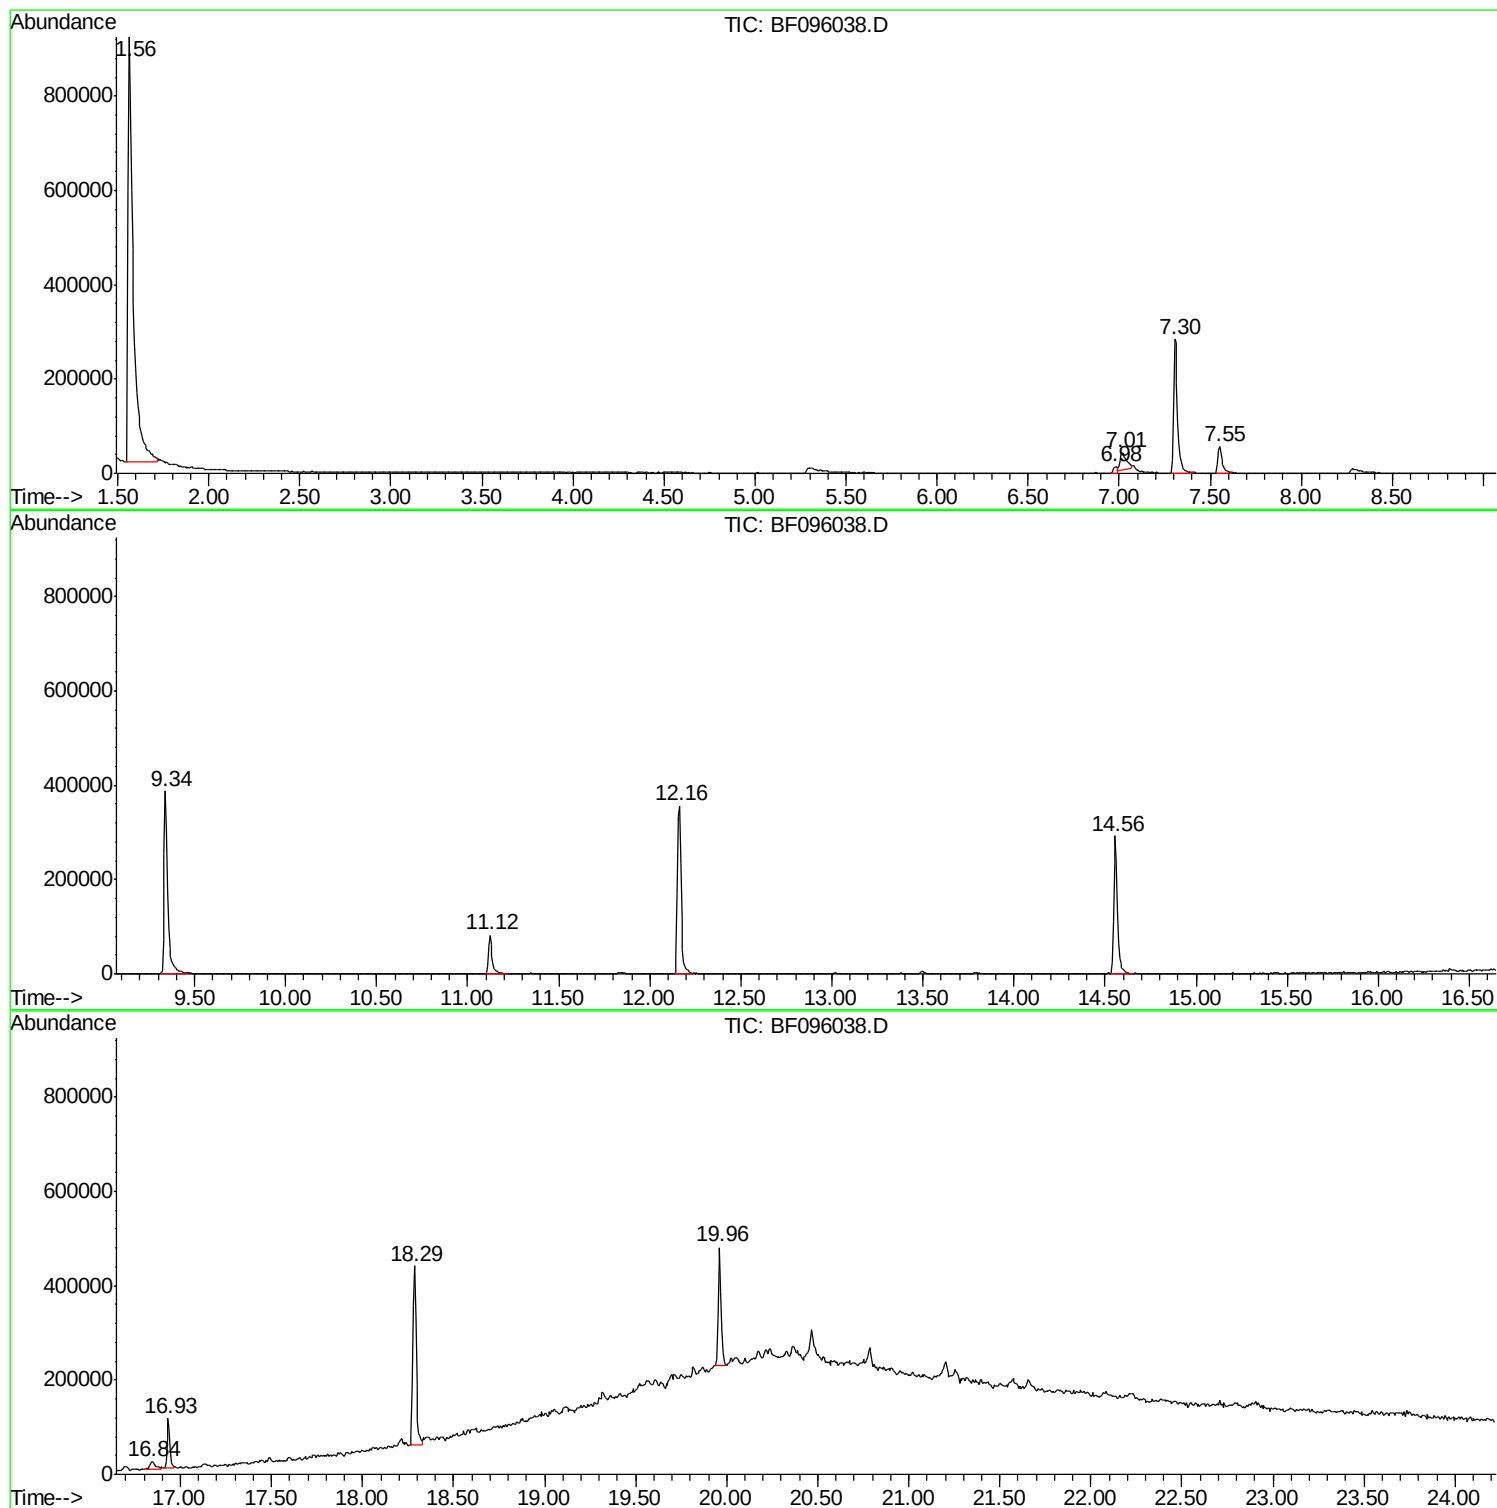

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
Data File : BF096038.D
Acq On : 20 Jun 2017 10:39
Operator : SJ/MA
Sample : I3688-01 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G23-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
Data File : BF096038.D
Acq On : 20 Jun 2017 10:39
Operator : SJ/MA
Sample : I3688-01 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G23-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc