

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
 Data File : BF096039.D
 Acq On : 20 Jun 2017 11:11
 Operator : SJ/MA
 Sample : I3688-12 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G15-0-1.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	11	13	34	rBV	126815	235050	50.81%	5.926%
2	1.840	57	60	65	rVB3	4385	5707	1.23%	0.144%
3	5.287	642	646	655	rBV4	13205	44849	9.70%	1.131%
4	6.975	928	933	936	rBV4	18241	38781	8.38%	0.978%
5	7.010	936	939	955	rVB3	50474	149361	32.29%	3.765%
6	7.310	985	990	1003	rBV	246934	357162	77.21%	9.004%
7	7.551	1027	1031	1044	rBV	62542	102985	22.26%	2.596%
8	8.269	1150	1153	1165	rBV2	11996	36753	7.95%	0.927%
9	8.351	1165	1167	1172	rVB3	3792	5011	1.08%	0.126%
10	9.339	1331	1335	1350	rBV	321269	462587	100.00%	11.662%
11	9.439	1350	1352	1359	rVB	4414	5833	1.26%	0.147%
12	10.428	1517	1520	1526	rBB3	4792	5858	1.27%	0.148%
13	10.528	1533	1537	1547	rBB	7284	13687	2.96%	0.345%
14	10.675	1558	1562	1565	rBV2	4598	7035	1.52%	0.177%
15	11.122	1634	1638	1651	rBV	109820	140703	30.42%	3.547%
16	11.345	1672	1676	1680	rVB2	5116	6688	1.45%	0.169%
17	11.651	1724	1728	1733	rBV2	2996	5028	1.09%	0.127%
18	11.827	1754	1758	1762	rBV	9697	15385	3.33%	0.388%
19	11.863	1762	1764	1768	rVB2	5214	5205	1.13%	0.131%
20	11.951	1775	1779	1785	rBB	4182	5378	1.16%	0.136%
21	12.163	1810	1815	1821	rBV2	314469	418353	90.44%	10.547%
22	12.210	1821	1823	1830	rVB3	15926	20680	4.47%	0.521%
23	12.522	1874	1876	1886	rBB2	4961	9993	2.16%	0.252%
24	13.016	1955	1960	1966	rBB	9393	13009	2.81%	0.328%
25	13.069	1966	1969	1976	rBB2	5770	8879	1.92%	0.224%
26	13.480	2035	2039	2046	rBV4	20452	37488	8.10%	0.945%
27	13.792	2086	2092	2093	rBV	12287	16260	3.52%	0.410%
28	14.316	2177	2181	2185	rBV2	3104	5441	1.18%	0.137%
29	14.515	2211	2215	2218	rBV2	11793	13396	2.90%	0.338%
30	14.557	2218	2222	2227	rVV	297760	396195	85.65%	9.988%
31	14.598	2227	2229	2238	rVB2	29716	39743	8.59%	1.002%
32	14.692	2241	2245	2251	rBV	15686	23453	5.07%	0.591%
33	14.821	2258	2267	2268	rBV4	2773	5502	1.19%	0.139%
34	15.027	2298	2302	2306	rBV5	3922	6887	1.49%	0.174%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061917\
 Data File : BF096039.D
 Acq On : 20 Jun 2017 11:11
 Operator : SJ/MA
 Sample : I3688-12 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G15-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.198	2326	2331	2338	rVB3	8218	10730	2.32%	0.271%
36	15.374	2358	2361	2364	rVB	6881	6067	1.31%	0.153%
37	15.415	2364	2368	2372	rBV2	8310	11103	2.40%	0.280%
38	15.521	2379	2386	2390	rBV2	14155	24127	5.22%	0.608%
39	15.568	2390	2394	2400	rVB7	5154	12160	2.63%	0.307%
40	15.810	2432	2435	2436	rBV	6653	7018	1.52%	0.177%
41	16.039	2469	2474	2476	rBV6	3393	4944	1.07%	0.125%
42	16.115	2485	2487	2491	rVB6	3360	4679	1.01%	0.118%
43	16.180	2494	2498	2502	rBV	8536	12838	2.78%	0.324%
44	16.386	2529	2533	2538	rVB	76478	79377	17.16%	2.001%
45	16.633	2571	2575	2576	rBV4	5750	7303	1.58%	0.184%
46	16.692	2581	2585	2591	rVV2	66868	89320	19.31%	2.252%
47	16.845	2608	2611	2613	rBV2	11524	14587	3.15%	0.368%
48	16.933	2622	2626	2633	rVB	126558	151398	32.73%	3.817%
49	17.133	2656	2660	2662	rBV4	11992	17095	3.70%	0.431%
50	17.162	2663	2665	2668	rVB4	11425	13364	2.89%	0.337%
51	17.251	2678	2680	2683	rBV3	11965	11041	2.39%	0.278%
52	17.298	2685	2688	2692	rVV6	10248	14870	3.21%	0.375%
53	17.409	2705	2707	2711	rVB4	7745	7266	1.57%	0.183%
54	17.492	2718	2721	2723	rBV4	9531	9912	2.14%	0.250%
55	18.027	2810	2812	2814	rBV3	13039	11291	2.44%	0.285%
56	18.139	2829	2831	2835	rVB3	22404	22635	4.89%	0.571%
57	18.286	2851	2856	2860	rBV	330962	425214	91.92%	10.720%
58	19.562	3070	3073	3081	rBV	45443	85793	18.55%	2.163%
59	19.962	3137	3141	3145	rBV	202427	248213	53.66%	6.257%


Sum of corrected areas: 3966670

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
Data File : BF096039.D
Acq On : 20 Jun 2017 11:11
Operator : SJ/MA
Sample : I3688-12 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G15-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

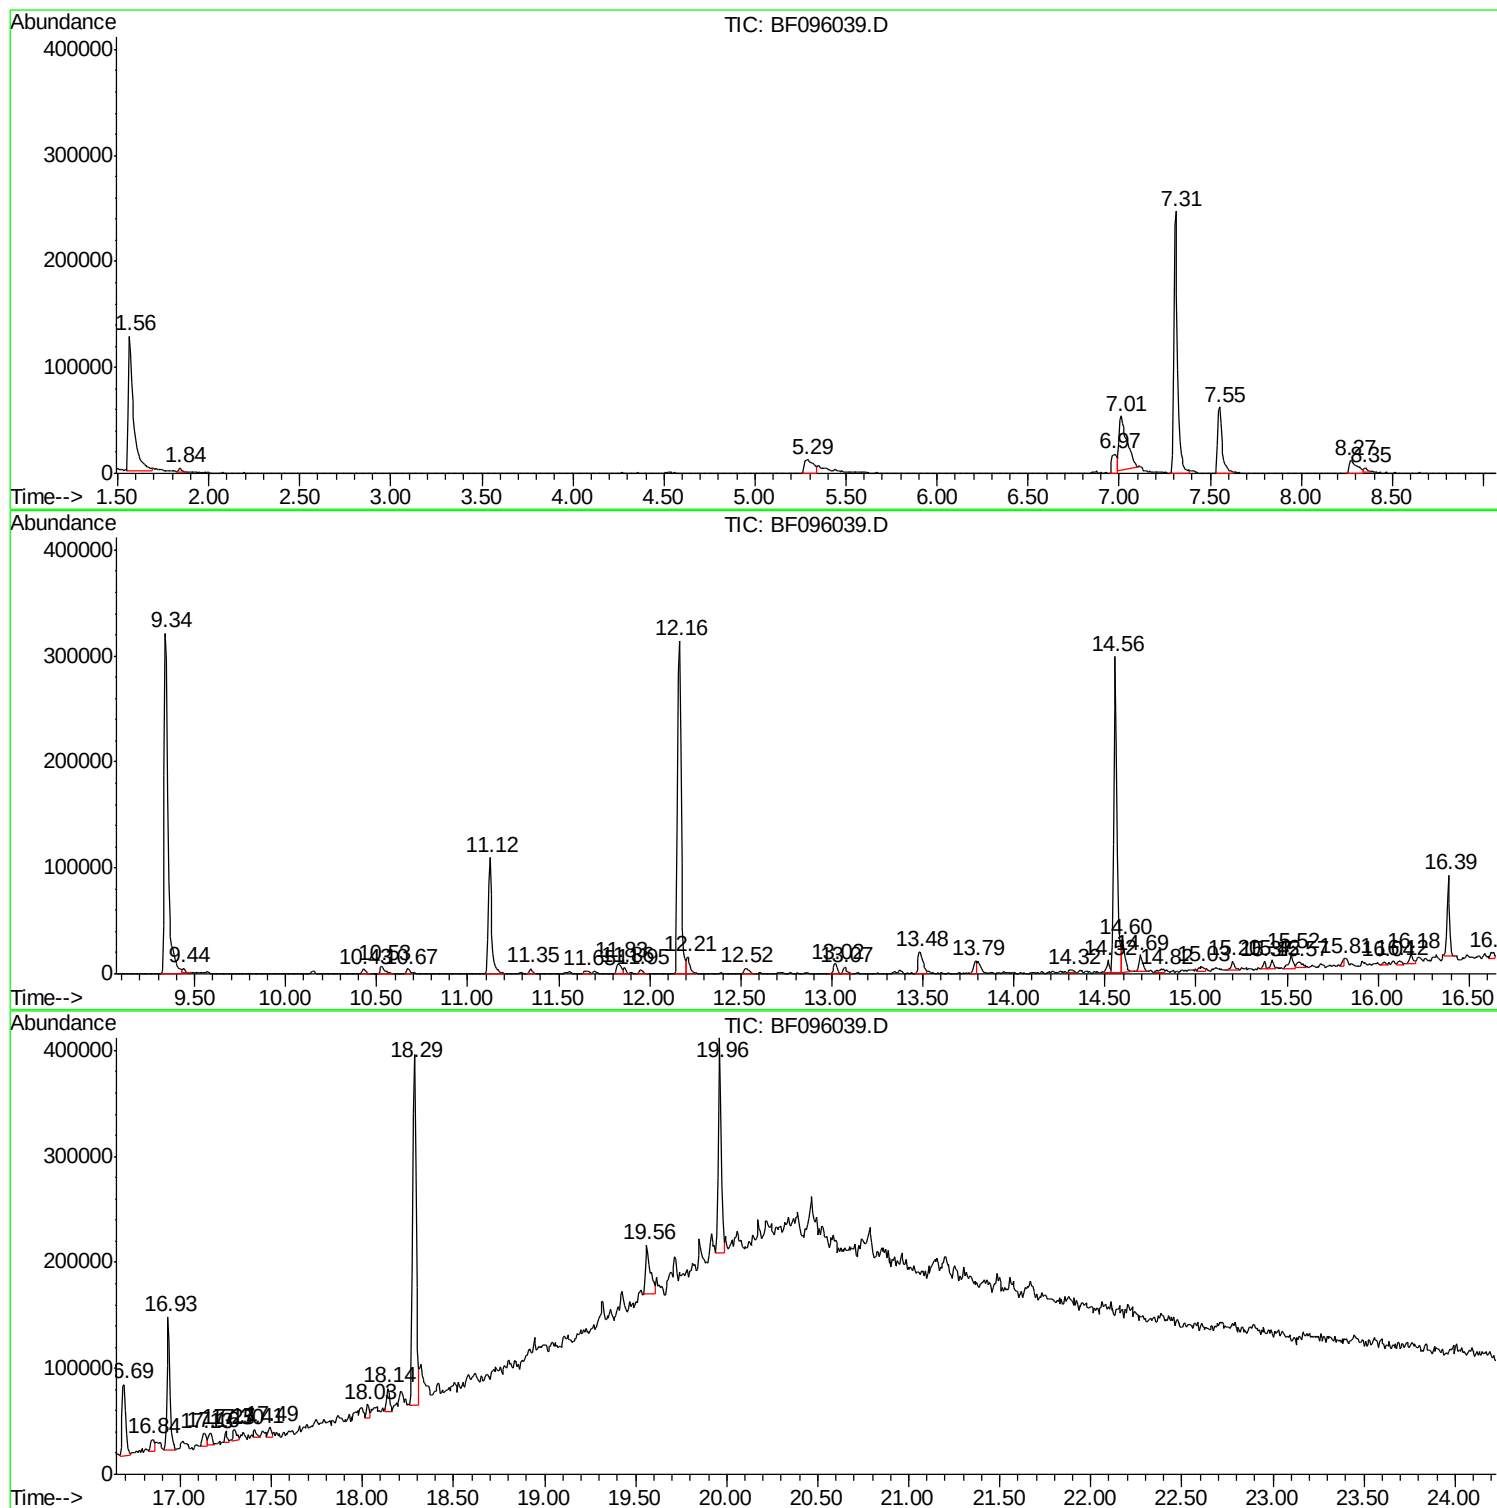

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
Data File : BF096039.D
Acq On : 20 Jun 2017 11:11
Operator : SJ/MA
Sample : I3688-12 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G15-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
Data File : BF096039.D
Acq On : 20 Jun 2017 11:11
Operator : SJ/MA
Sample : I3688-12 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G15-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc