


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
 Data File : BF095998.D
 Acq On : 19 Jun 2017 10:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

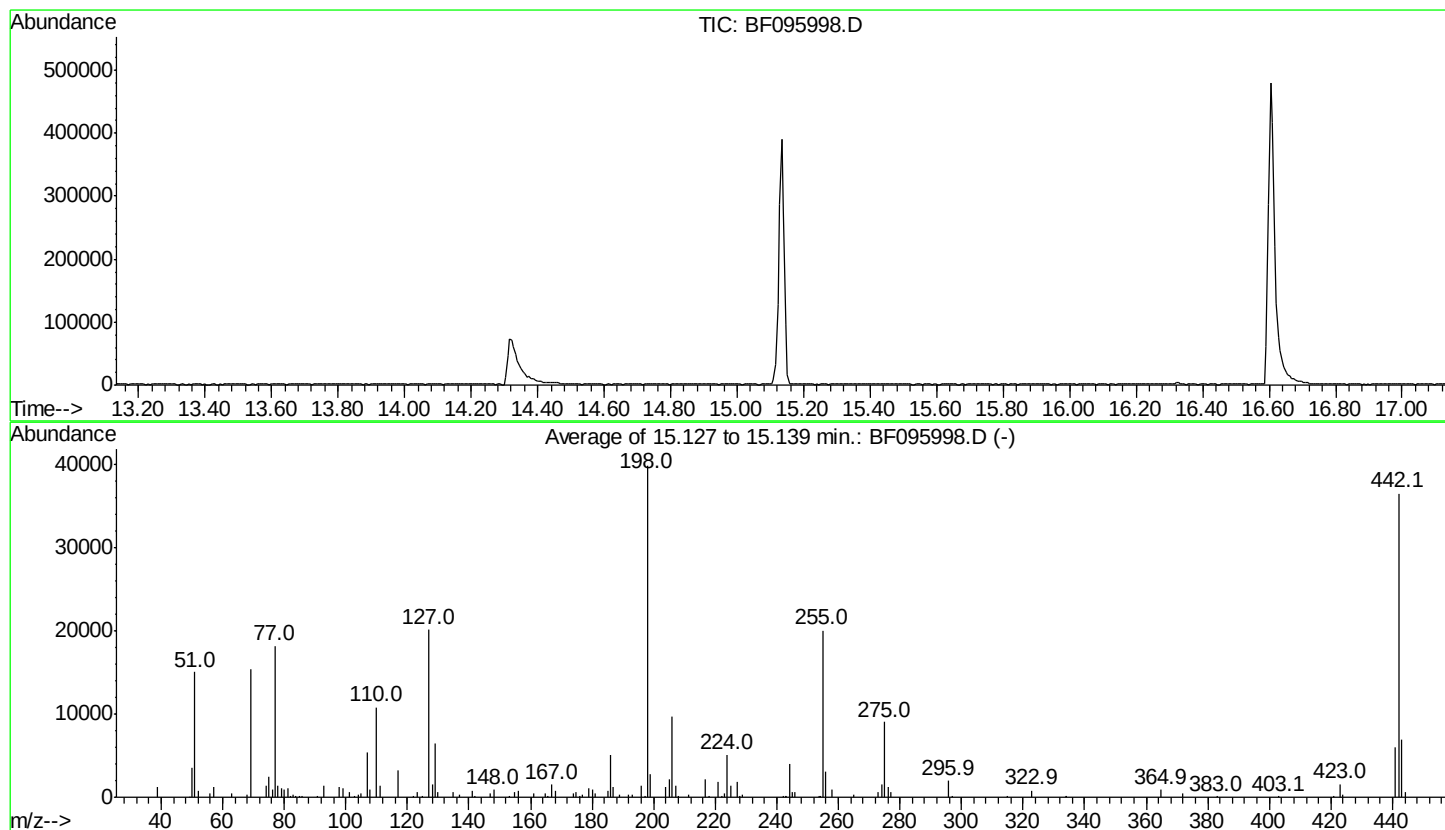

AutoFind: Scans 2302, 2303, 2304; Background Corrected with Scan 2296

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	15051	PASS
68	69	0.00	2	1.6	252	PASS
69	198	0.00	100	38.6	15416	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	20139	PASS
197	198	0.00	2	0.4	161	PASS
198	198	100	100	100.0	39906	PASS
199	198	5	9	6.9	2752	PASS
275	198	10	60	22.6	9027	PASS
365	198	1	100	2.3	920	PASS
441	442	0.01	24	16.3	5939	PASS
442	198	50	100	91.5	36514	PASS
443	442	15	24	18.8	6871	PASS