


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061917\
 Data File : BF096021.D
 Acq On : 20 Jun 2017 1:13
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

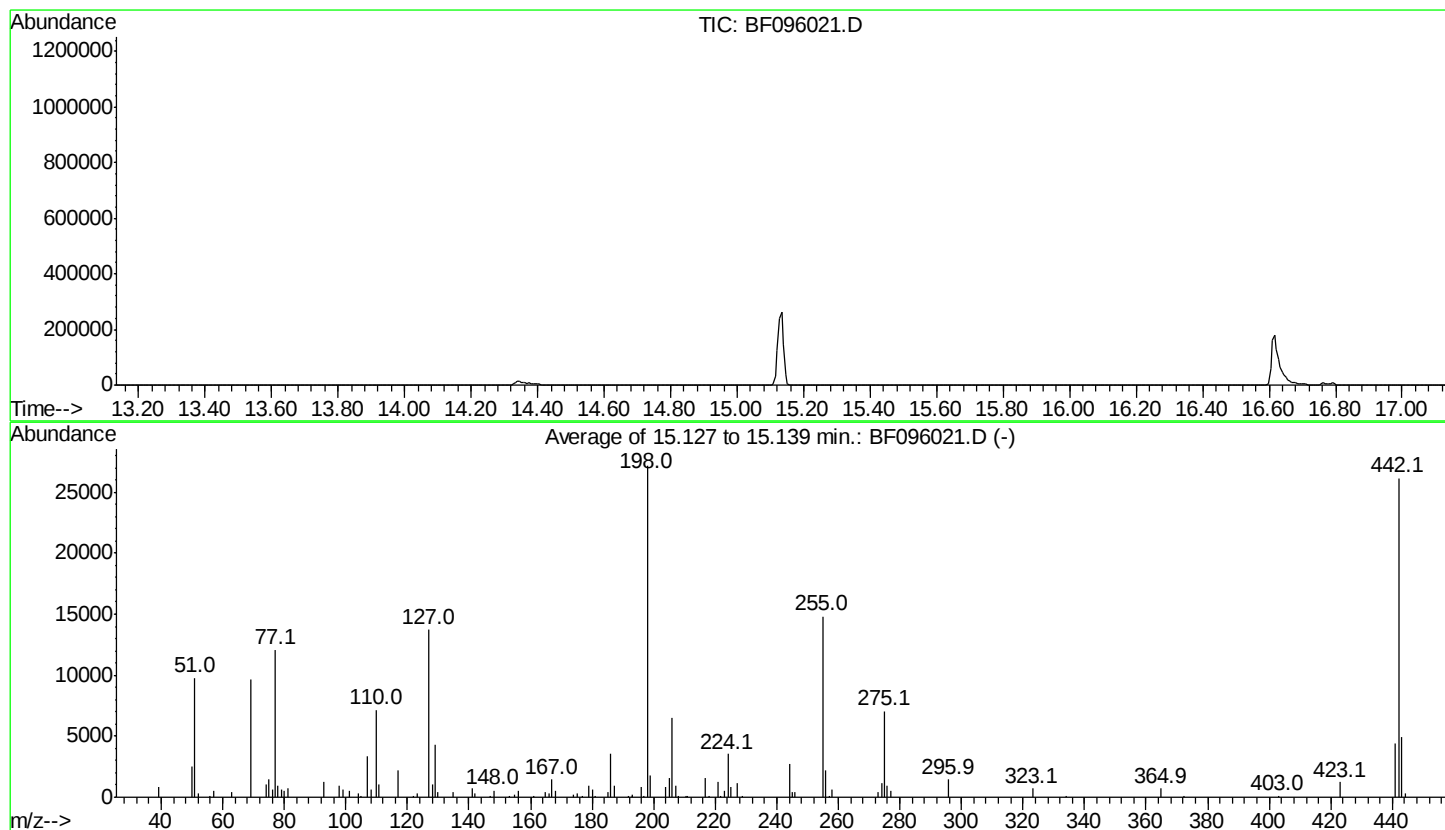

AutoFind: Scans 2319, 2320, 2321; Background Corrected with Scan 2313

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	9802	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	9662	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	13719	PASS
197	198	0.00	2	0.5	136	PASS
198	198	100	100	100.0	27170	PASS
199	198	5	9	6.4	1740	PASS
275	198	10	60	25.9	7041	PASS
365	198	1	100	2.5	691	PASS
441	442	0.01	24	16.7	4369	PASS
442	198	50	100	96.3	26165	PASS
443	442	15	24	18.7	4889	PASS