
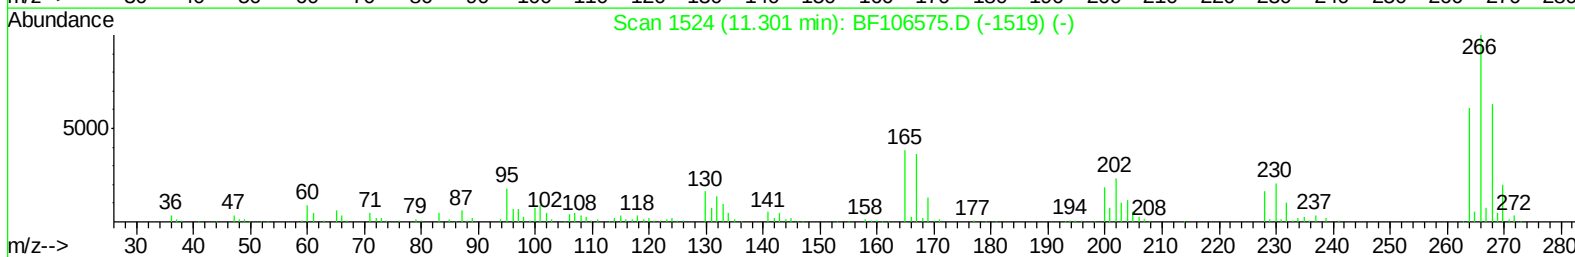
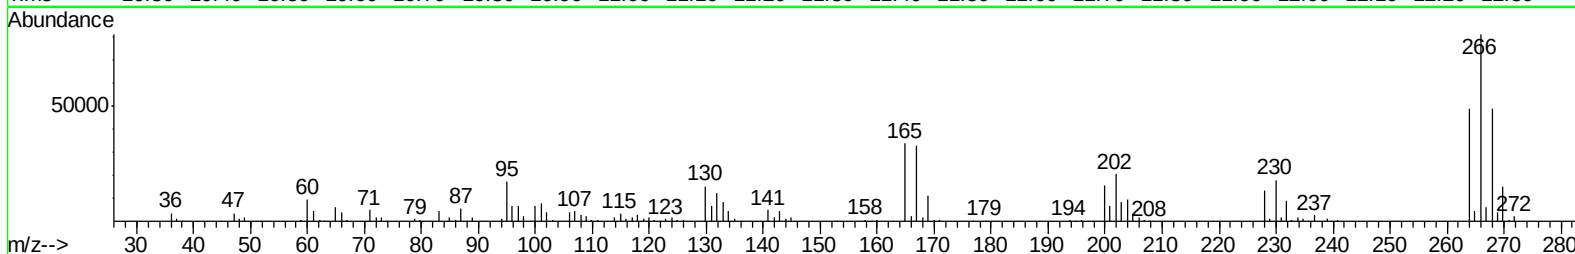


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061918\
Data File : BF106580.D
Acq On : 19 Jun 2018 14:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 08:41:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 19 14:32:09 2018
Response via : Initial Calibration

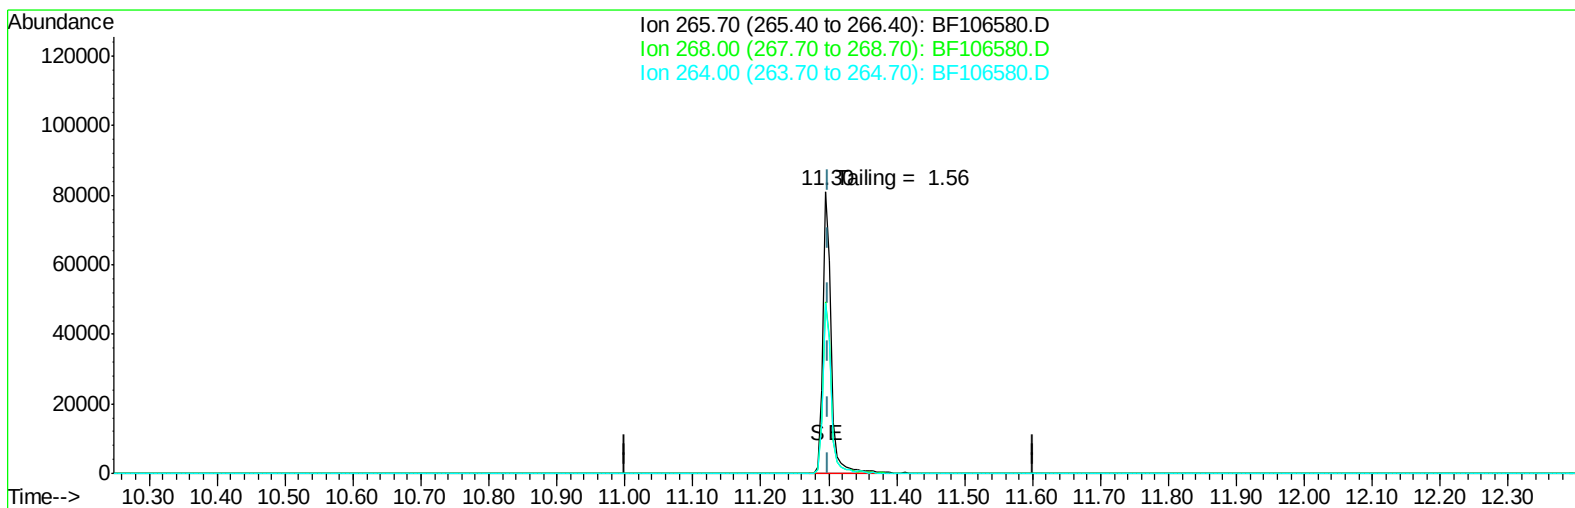

TIC: BF106580.D

(69) Pentachlorophenol (C)




11.295min (-0.006) 84656.47ng

response 70702

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.77
264.00	61.90	60.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061918\
Data File : BF106580.D
Acq On : 19 Jun 2018 14:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 08:41:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 19 14:32:09 2018
Response via : Initial Calibration

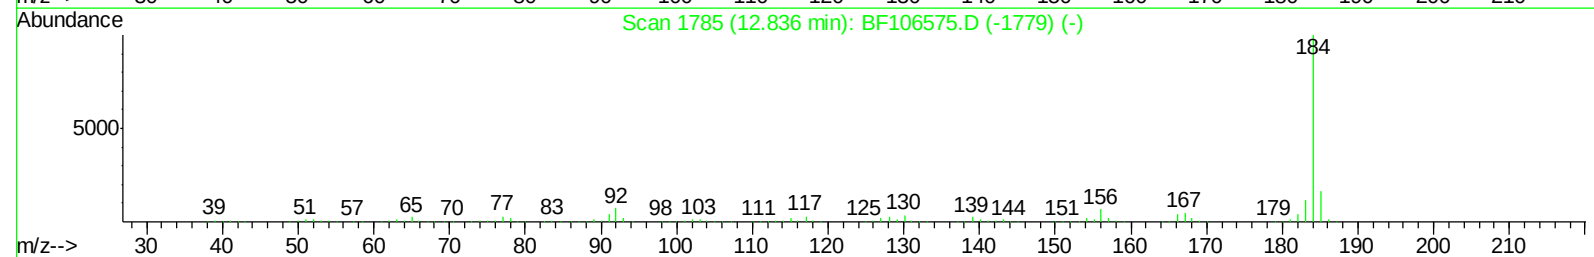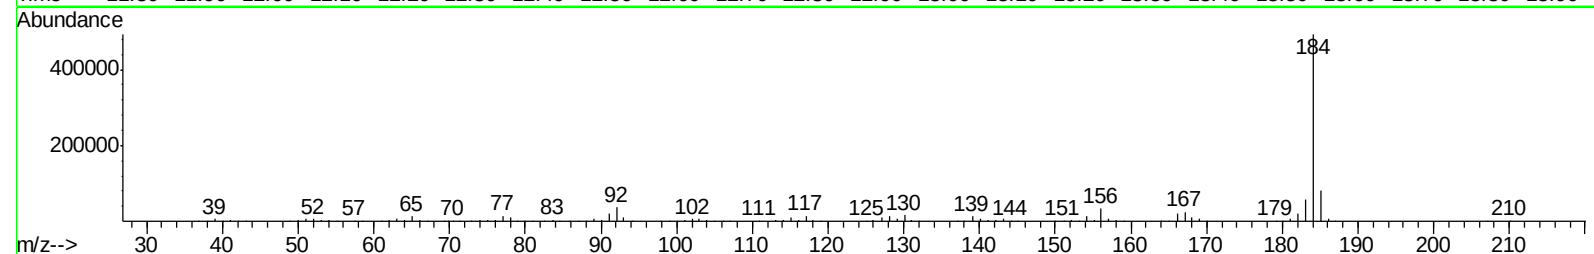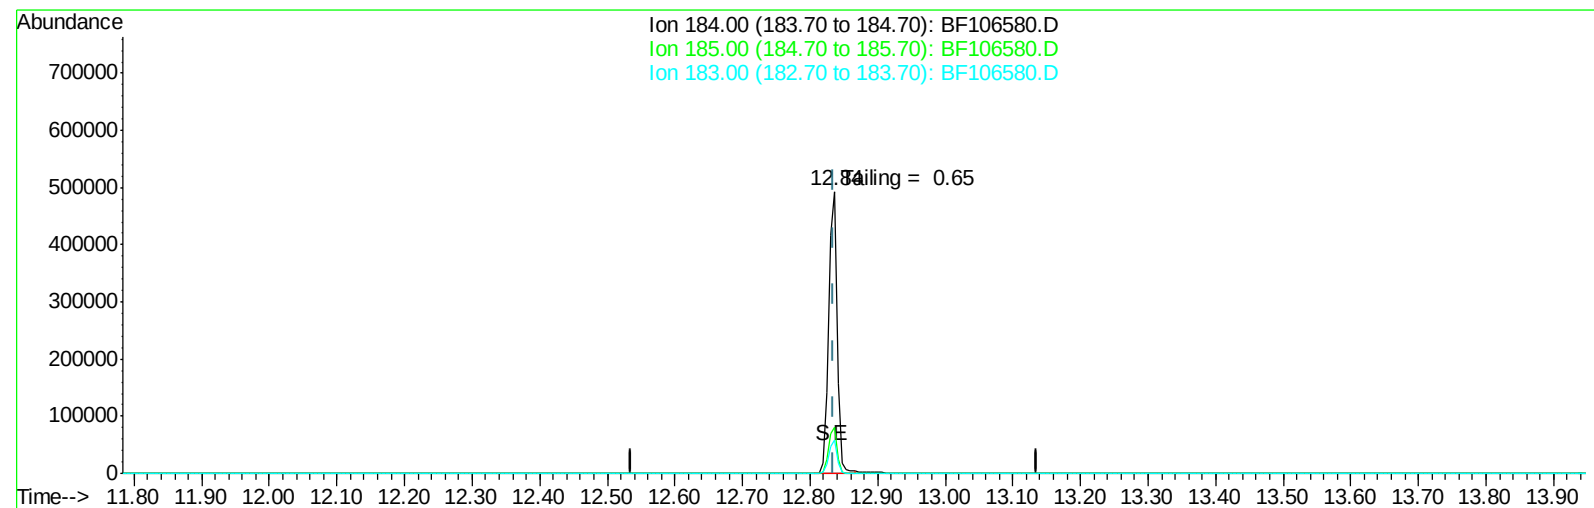

TIC: BF106580.D

(76) Benzidine

12.836min (+0.000) 0.00ng

response 452373

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.35
183.00	11.60	11.96
0.00	0.00	0.00