


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF061918\  
 Data File : BF106571.D  
 Acq On : 19 Jun 2018 9:56  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jun 19 14:32:09 2018

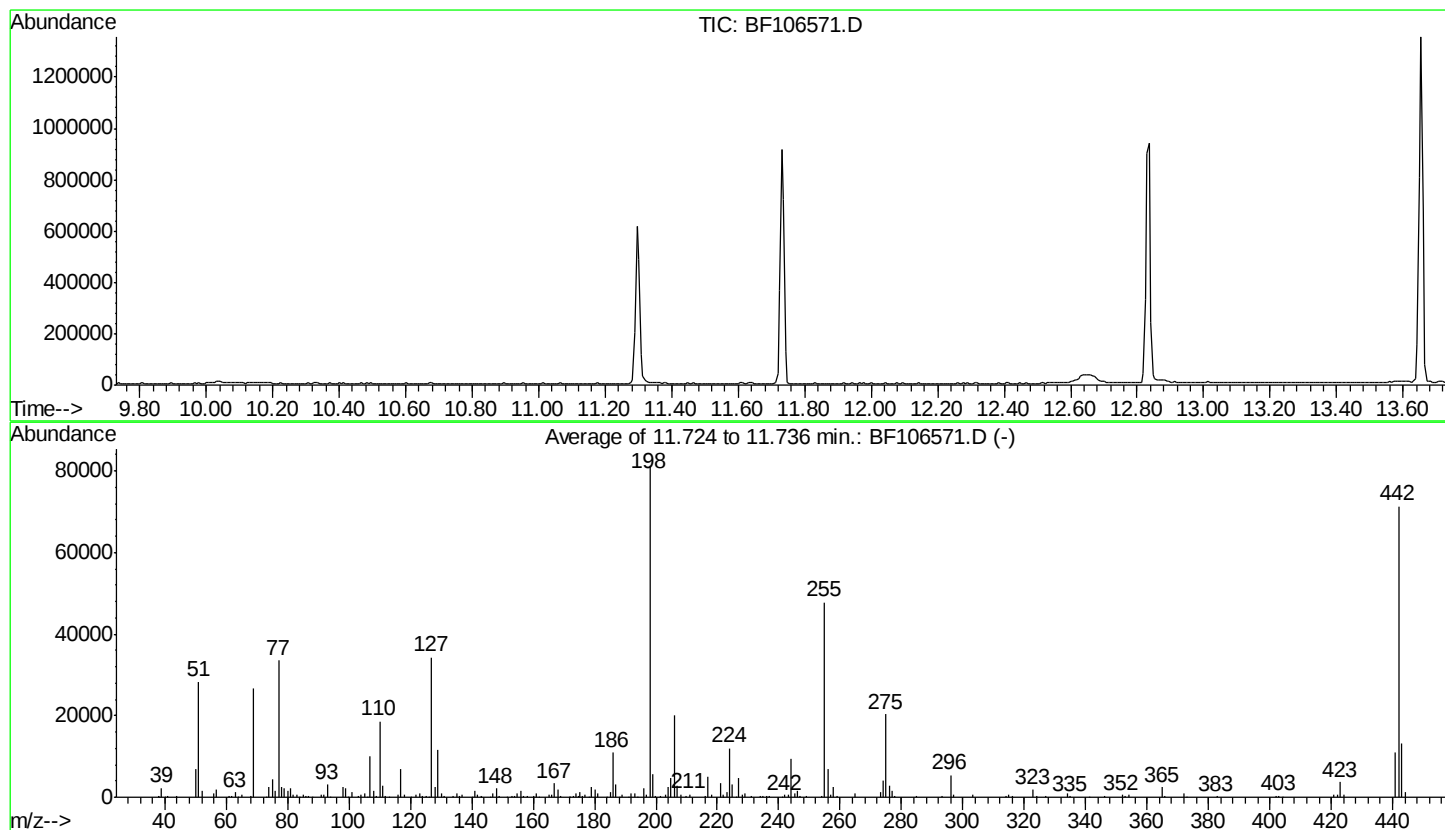

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.8      | 28296   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.2       | 320     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.8      | 26634   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 42.2      | 34277   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 521     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 81296   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 5526    | PASS             |
| 275         | 198          | 10           | 60           | 25.0      | 20342   | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 2414    | PASS             |
| 441         | 443          | 0.01         | 100          | 85.2      | 11124   | PASS             |
| 442         | 198          | 50           | 100          | 87.6      | 71241   | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 13057   | PASS             |