


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061918\
Data File : BF106580.D
Acq On : 19 Jun 2018 14:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 19 14:32:09 2018

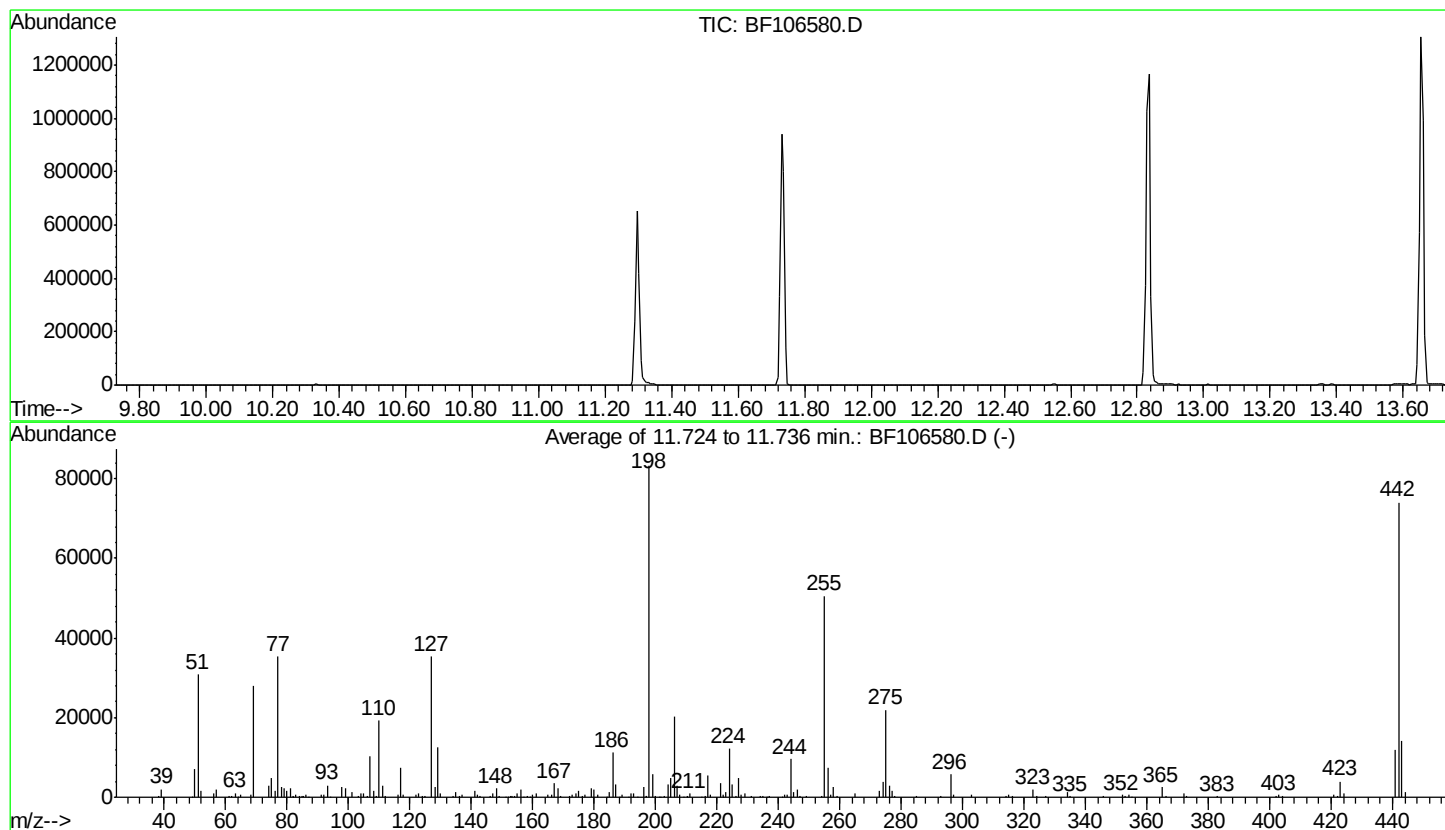

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	30786	PASS
68	69	0.00	2	1.8	512	PASS
69	198	0.00	100	33.7	28040	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	35344	PASS
197	198	0.00	2	0.3	225	PASS
198	198	100	100	100.0	83325	PASS
199	198	5	9	7.1	5879	PASS
275	198	10	60	26.3	21909	PASS
365	198	1	100	2.9	2431	PASS
441	443	0.01	100	84.2	11799	PASS
442	198	50	100	88.9	74101	PASS
443	442	15	24	18.9	14021	PASS