
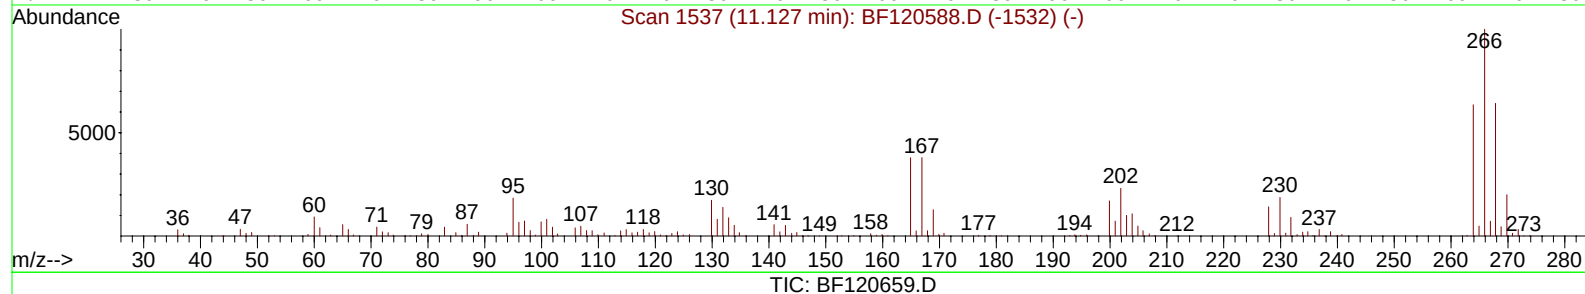
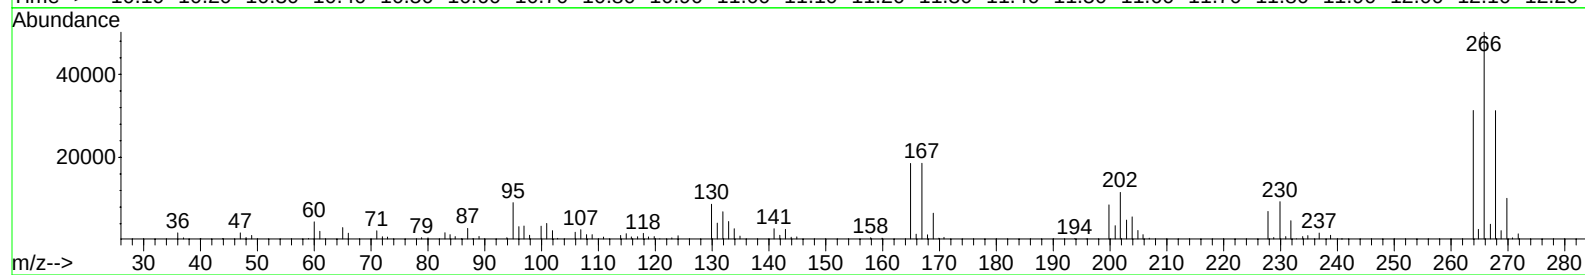


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061920\
Data File : BF120659.D
Acq On : 19 Jun 2020 12:23
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 19:11:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 11:28:22 2020
Response via : Initial Calibration

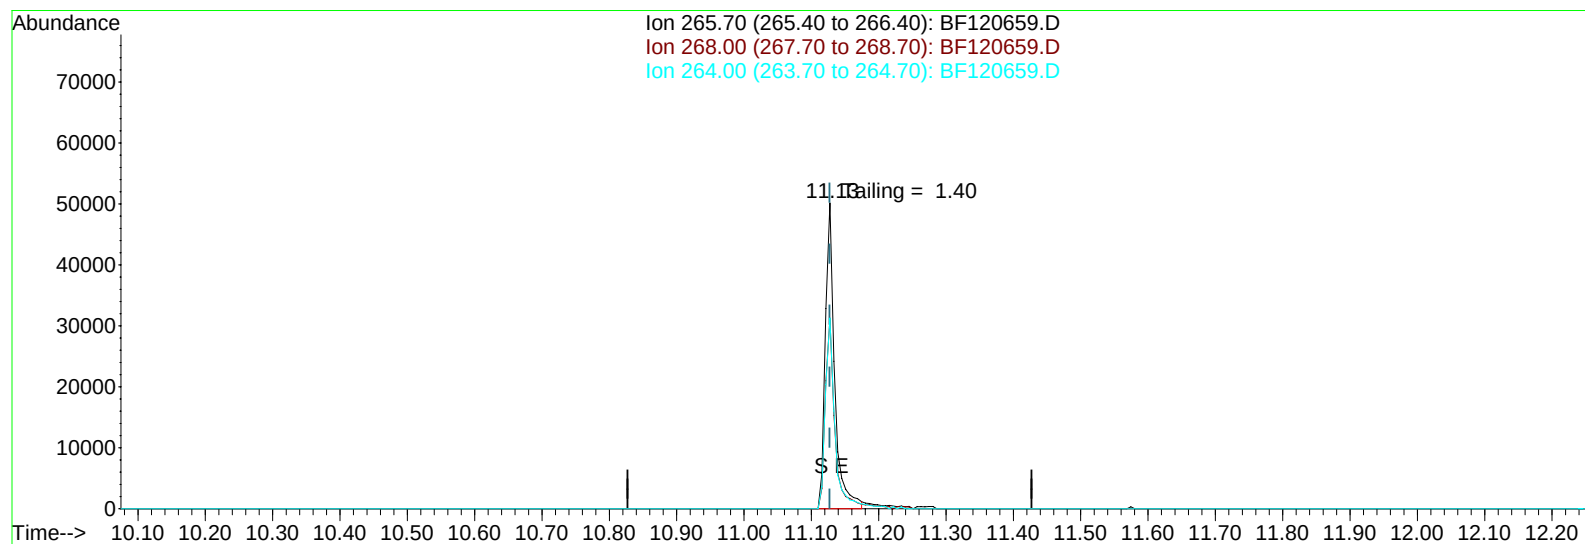

(70) Pentachlorophenol (C)




11.128min (+0.000) 50311.40ng

response 50855

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	62.33
264.00	63.50	62.38
0.00	0.00	0.00

```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061920\  
Data File   : BF120659.D  
Acq On      : 19 Jun 2020   12:23  
Operator    : JU/CG  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 19 19:11:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 11:28:22 2020
Response via : Initial Calibration

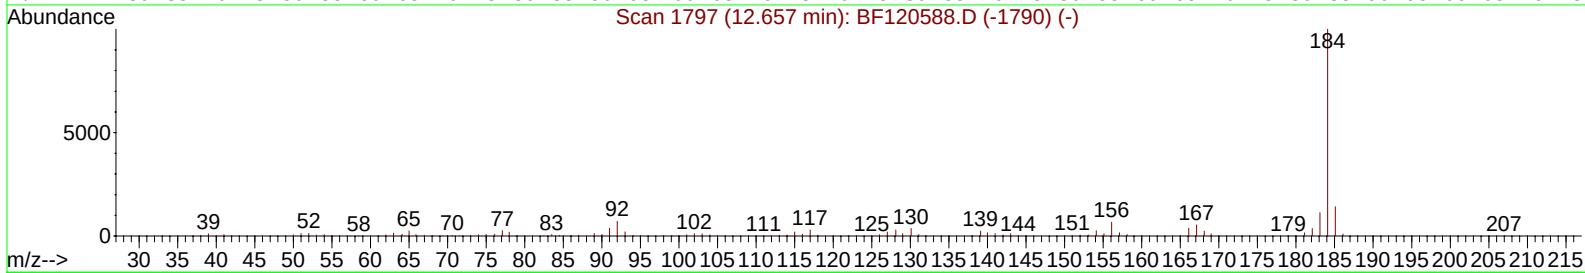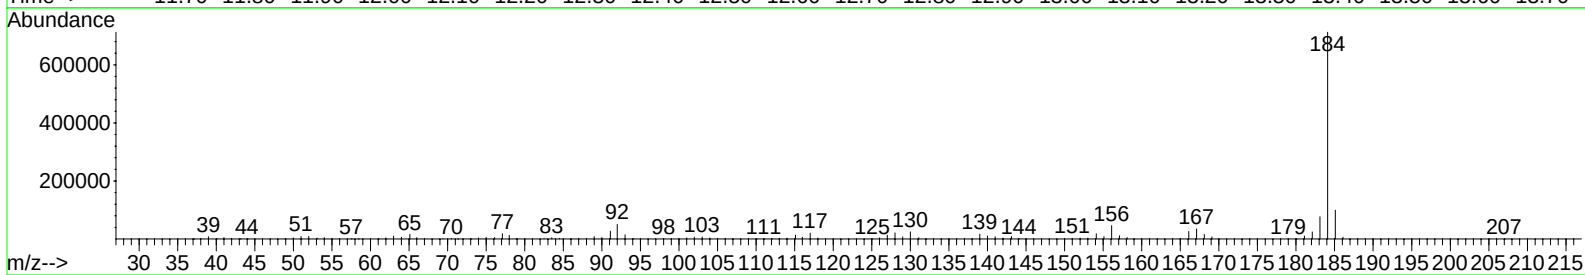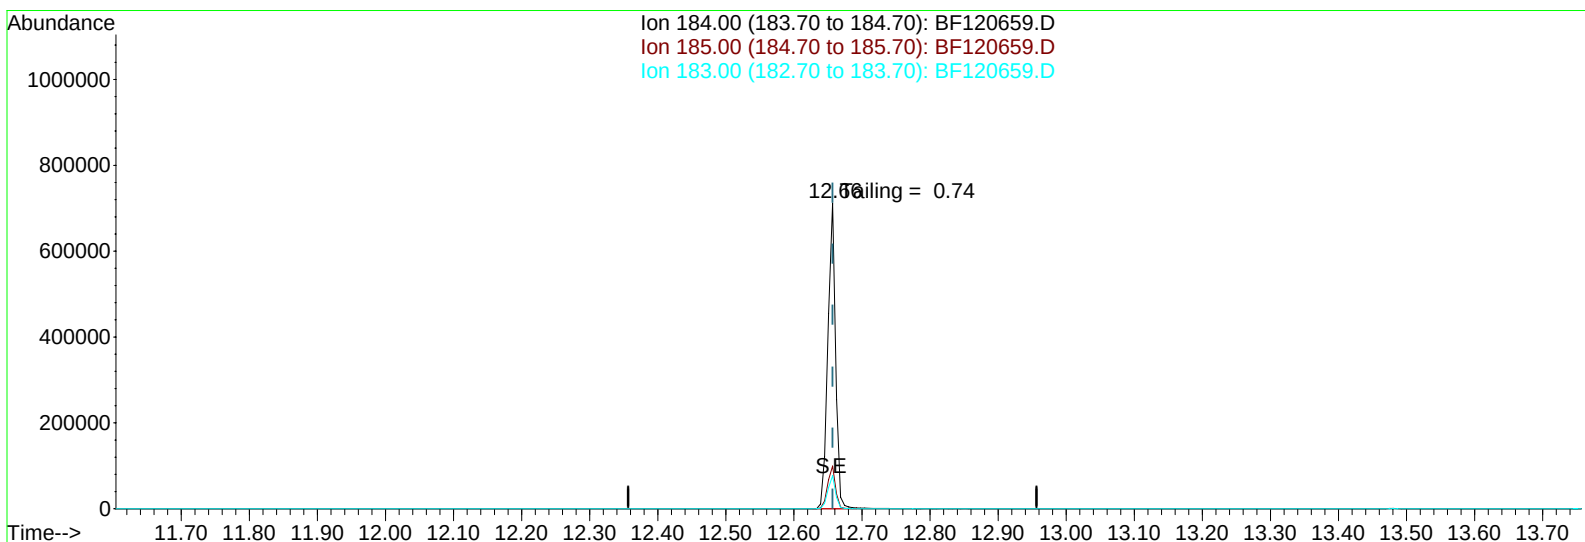

TIC: BF120659.D

(77) Benzidine

12.657min (+0.000) 0.00ng

response 567043

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.96
183.00	11.30	10.79
0.00	0.00	0.00