


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061920\
 Data File : BF120659.D
 Acq On : 19 Jun 2020 12:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 11:28:22 2020

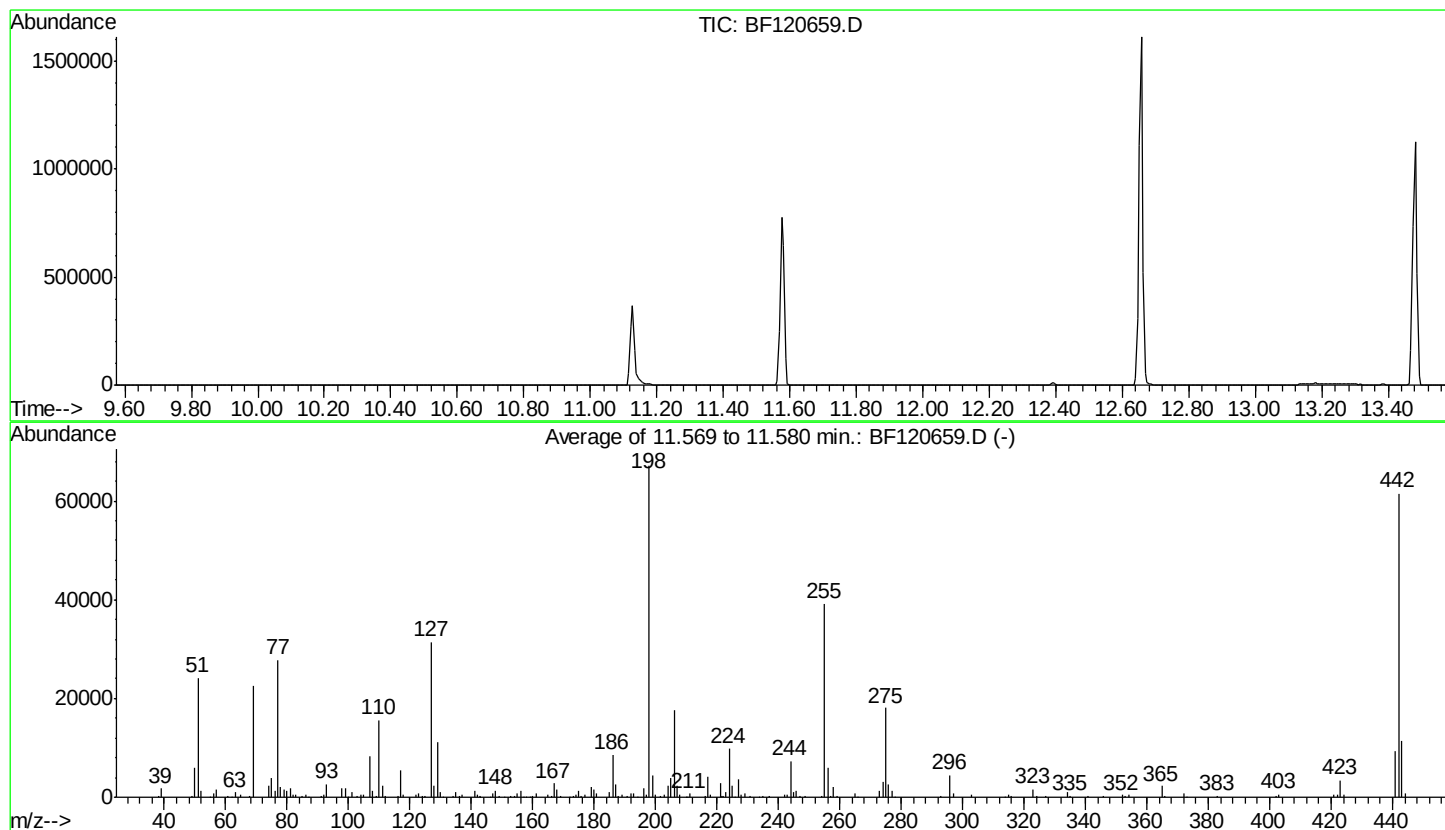

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	24186	PASS
68	69	0.00	2	1.5	330	PASS
69	198	0.00	100	33.6	22534	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	31381	PASS
197	198	0.00	2	0.7	440	PASS
198	198	100	100	100.0	67160	PASS
199	198	5	9	6.7	4493	PASS
275	198	10	60	27.0	18125	PASS
365	198	1	100	3.3	2221	PASS
441	198	0.01	100	14.0	9431	PASS
442	198	50	100	91.7	61560	PASS
443	442	15	24	18.6	11423	PASS