
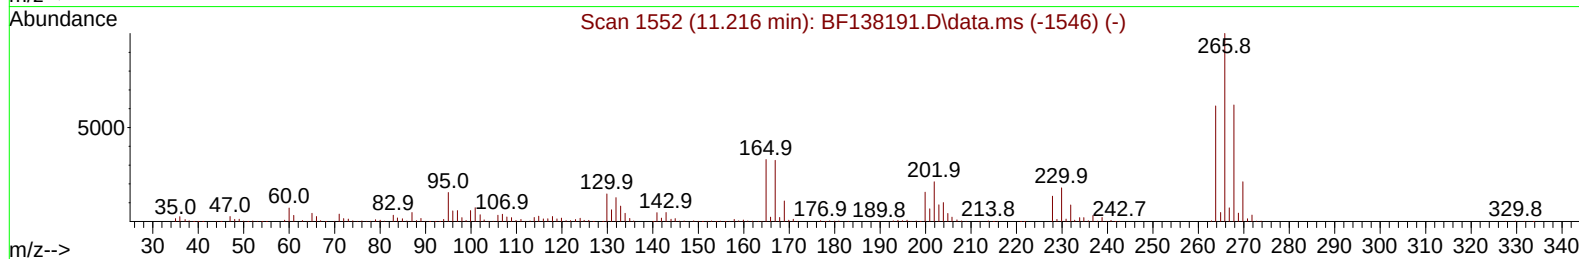
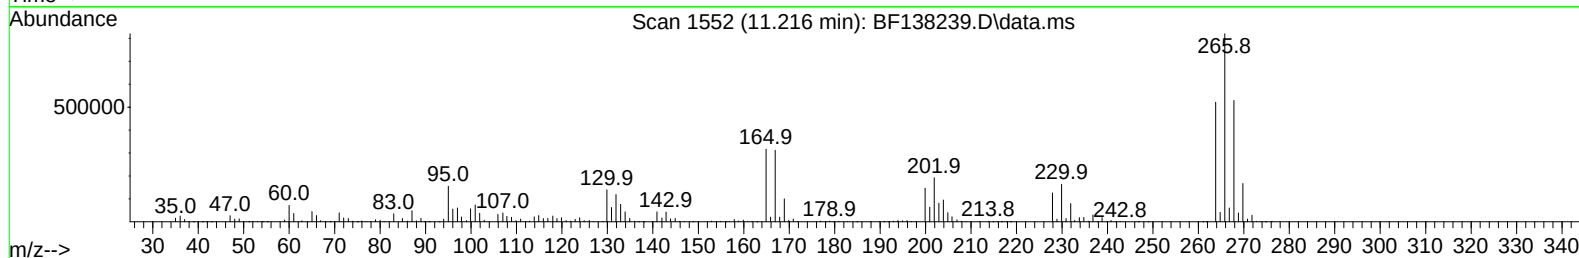


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138239.D
Acq On : 19 Jun 2024 10:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 12:19:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

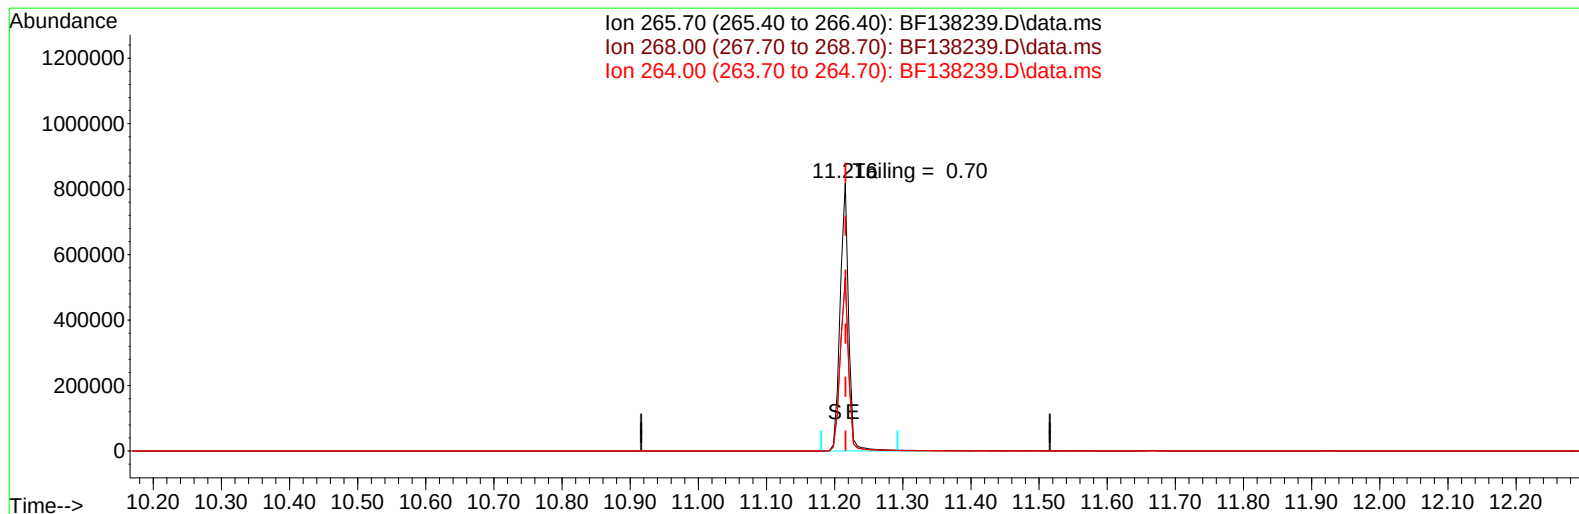

TIC: BF138239.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 263271.21 ng

response 702642

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.49
264.00	61.50	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138239.D
Acq On : 19 Jun 2024 10:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 12:19:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

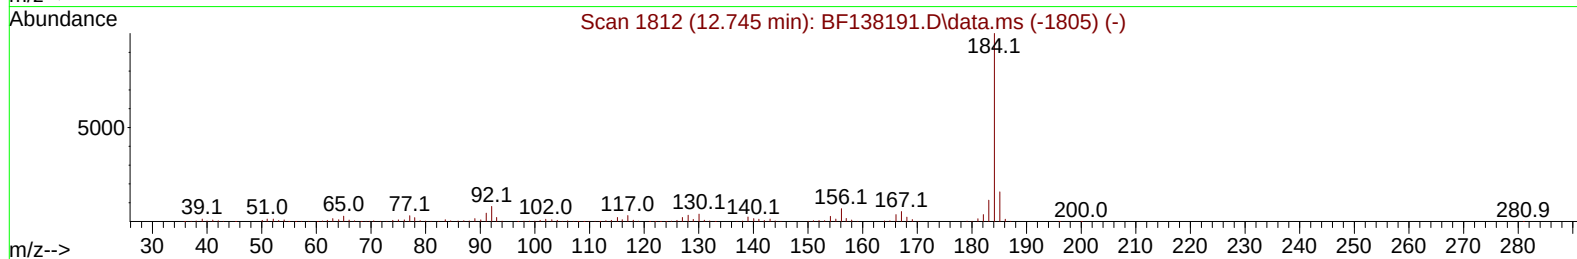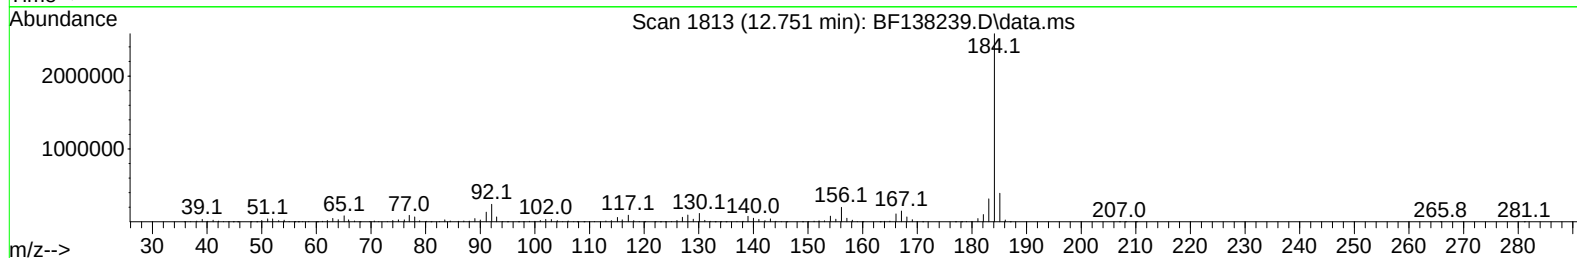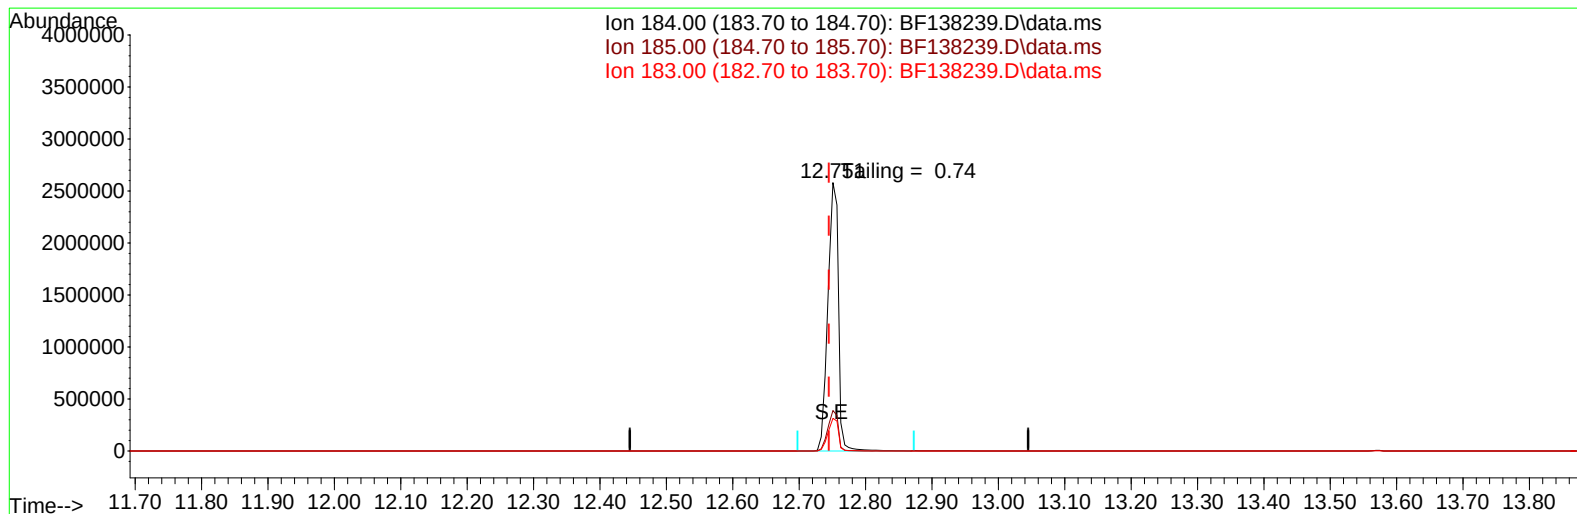

TIC: BF138239.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 12274.59 ng m

response 2850182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.13
183.00	11.30	12.17
0.00	0.00	0.00