
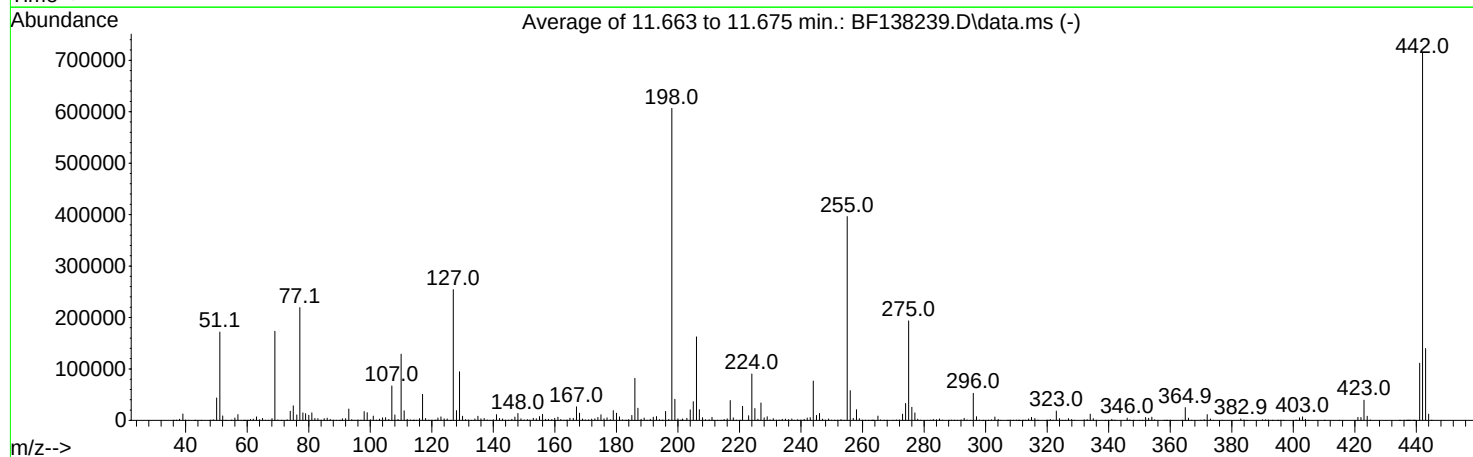


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138239.D
Acq On : 19 Jun 2024 10:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

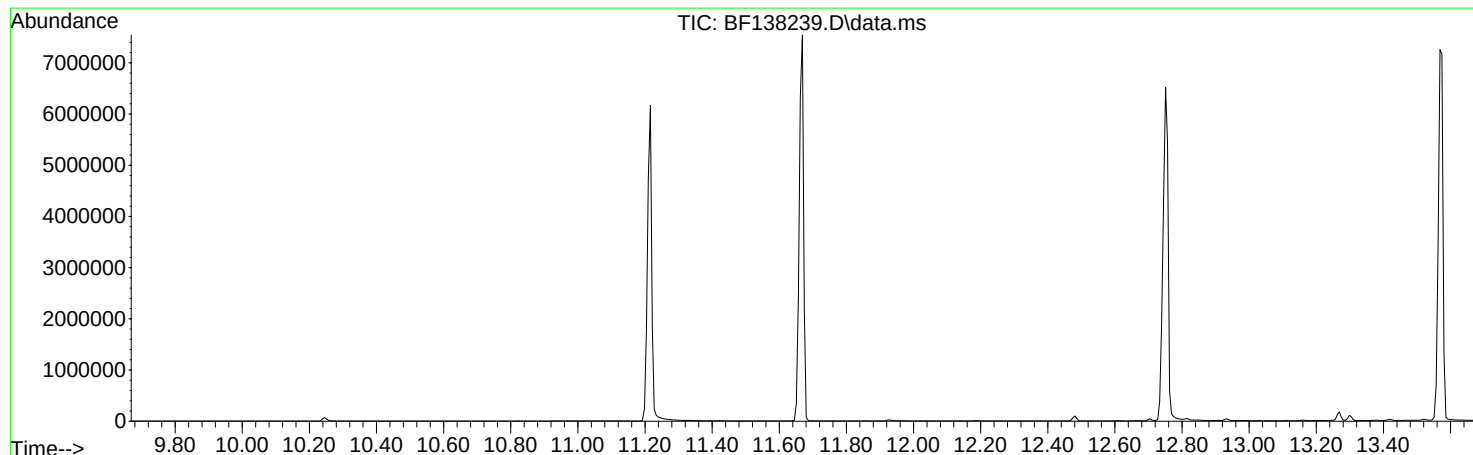

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	171760	PASS
68	69	0.00	2	1.9	3341	PASS
69	198	0.00	100	28.6	173285	PASS
70	69	0.00	2	0.6	998	PASS
127	198	10	80	41.9	254195	PASS
197	198	0.00	2	0.3	1985	PASS
198	198	100	100	100.0	606464	PASS
199	198	5	9	6.8	41119	PASS
275	198	10	60	31.9	193373	PASS
365	198	1	100	4.1	24919	PASS
441	198	0.01	100	18.3	111149	PASS
442	442	50	100	100.0	715093	PASS
443	442	15	24	19.5	139584	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2024	BNA_F	<u>BF138239.D</u>
Compound Name	Response	Retention Time
DDT	1408532	13.574
DDD	43177	13.269
DDE	4735	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47912	1456444	3.29

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138239.D
Acq On : 19 Jun 2024 10:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 19 12:19:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

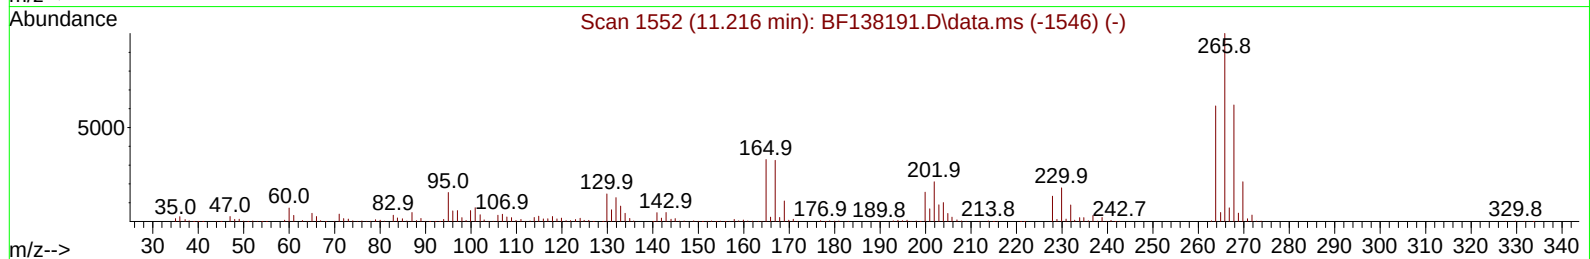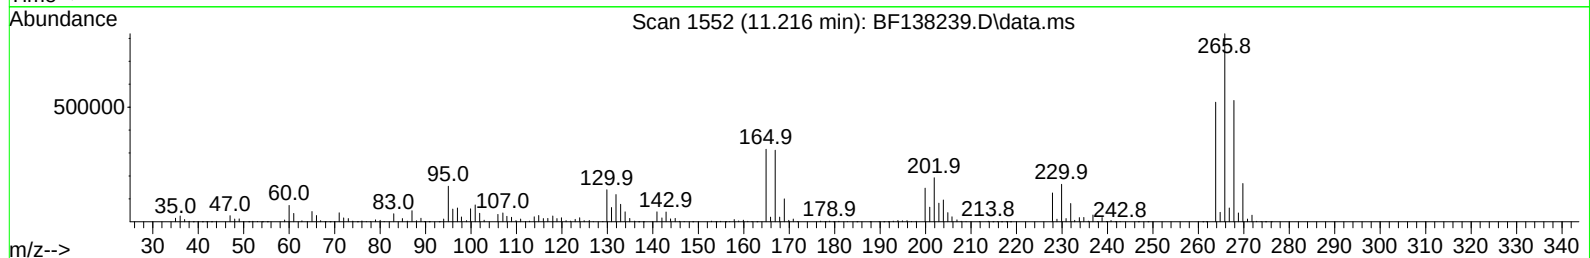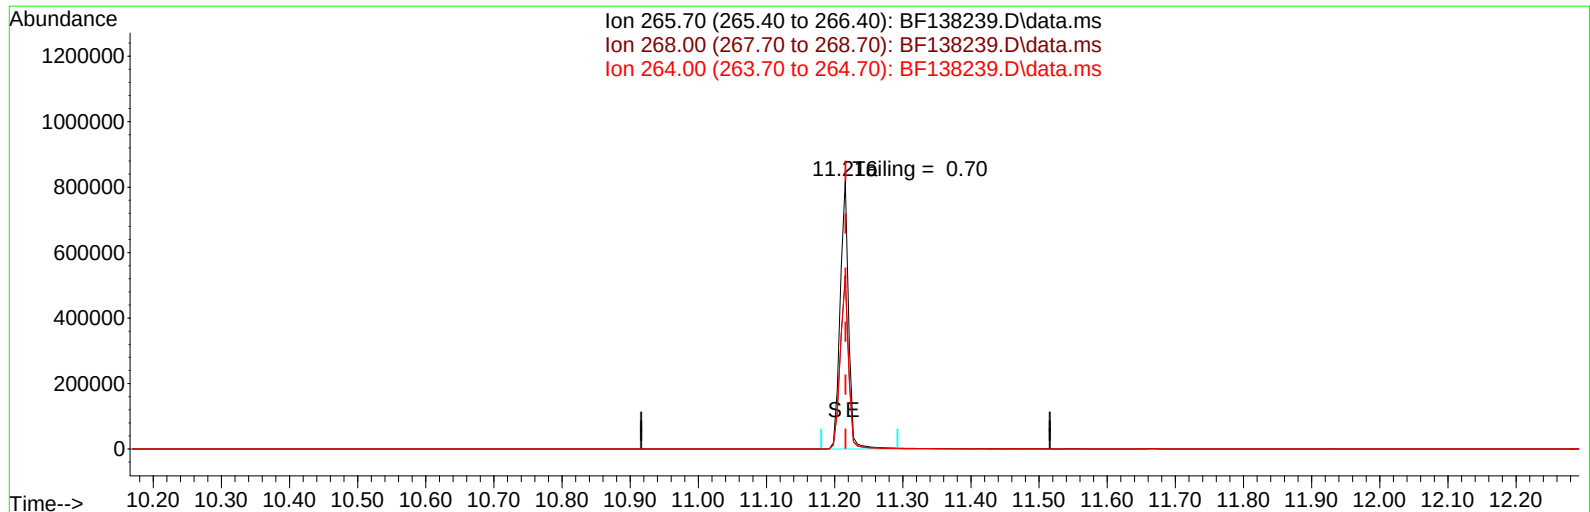

TIC: BF138239.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 263271.21 ng




response 702642

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.49
264.00	61.50	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138239.D
Acq On : 19 Jun 2024 10:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 19 12:19:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

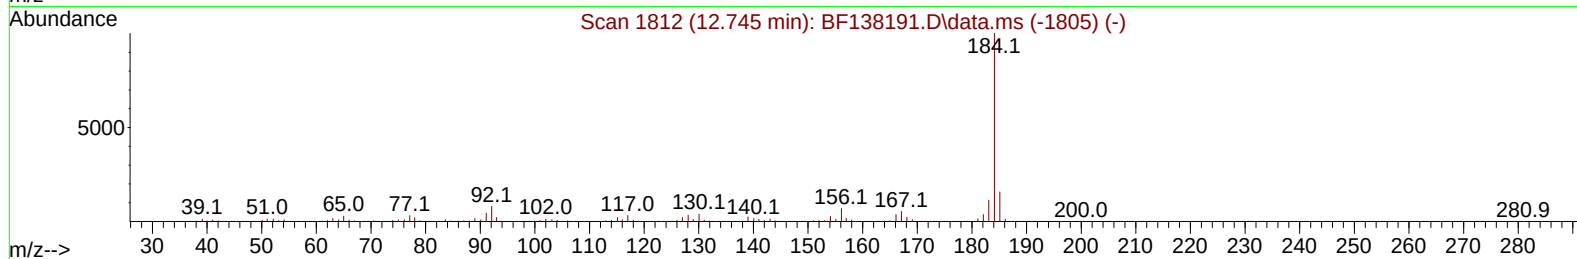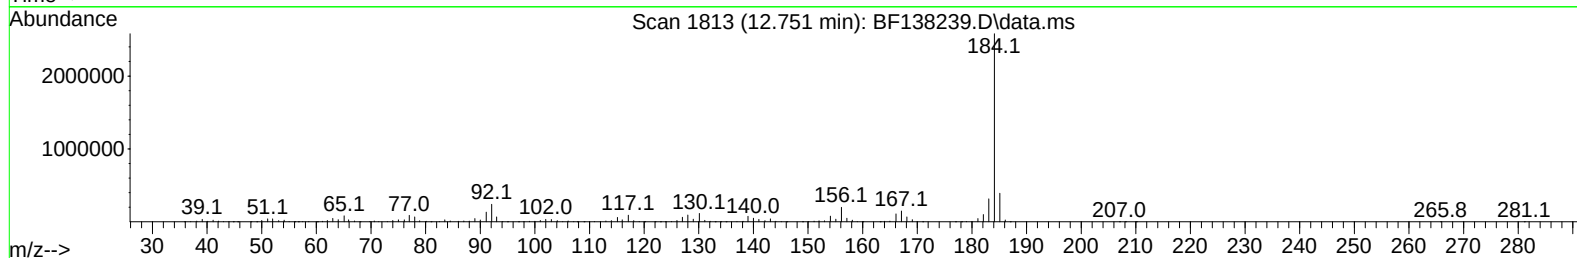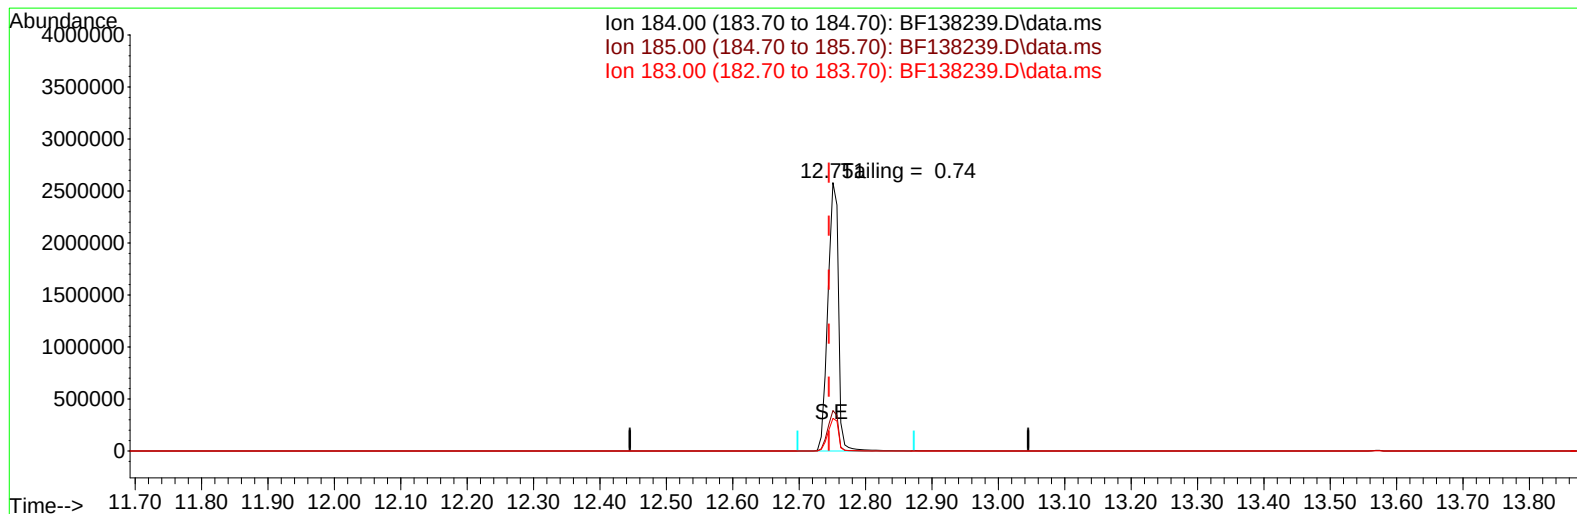

TIC: BF138239.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 12274.59 ng m

response 2850182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.13
183.00	11.30	12.17
0.00	0.00	0.00