
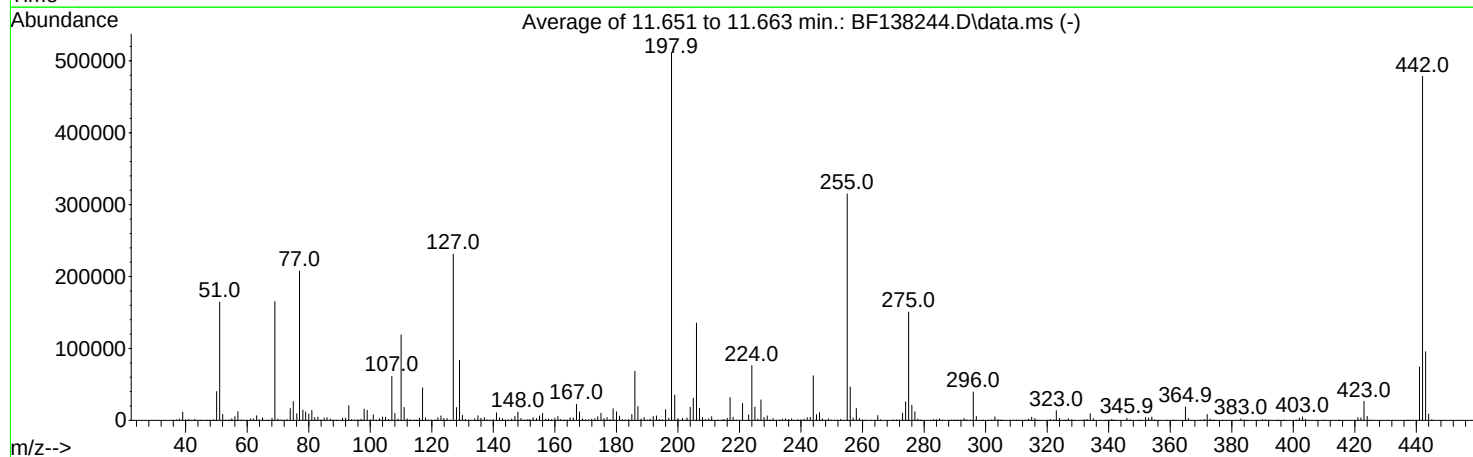


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138244.D
Acq On : 19 Jun 2024 14:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

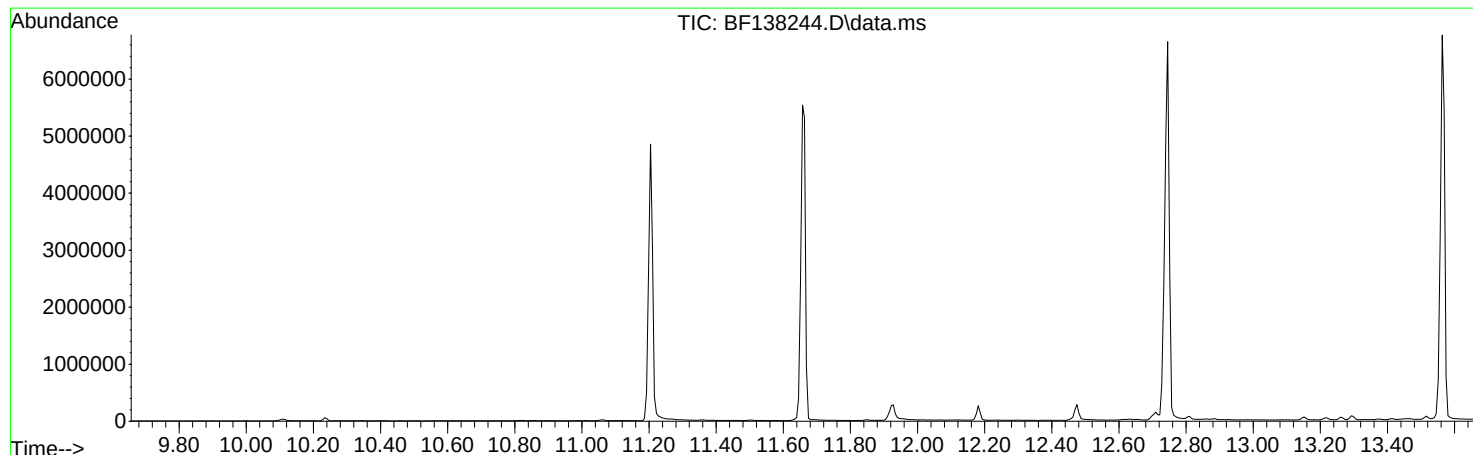

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	164787	PASS
68	69	0.00	2	2.0	3226	PASS
69	198	0.00	100	32.3	165293	PASS
70	69	0.00	2	1.1	1778	PASS
127	198	10	80	45.2	231317	PASS
197	198	0.00	2	0.6	2871	PASS
198	198	100	100	100.0	511616	PASS
199	198	5	9	6.9	35291	PASS
275	198	10	60	29.5	150728	PASS
365	198	1	100	3.6	18663	PASS
441	198	0.01	100	14.5	74392	PASS
442	442	50	100	100.0	478400	PASS
443	442	15	24	19.9	95405	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2024	BNA_F	<u>BF138244.D</u>
Compound Name	Response	Retention Time
DDT	1164577	13.563
DDD	19469	13.292
DDE	1549	12.928
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21018	1185595	1.77

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138244.D
Acq On : 19 Jun 2024 14:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 19 15:33:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

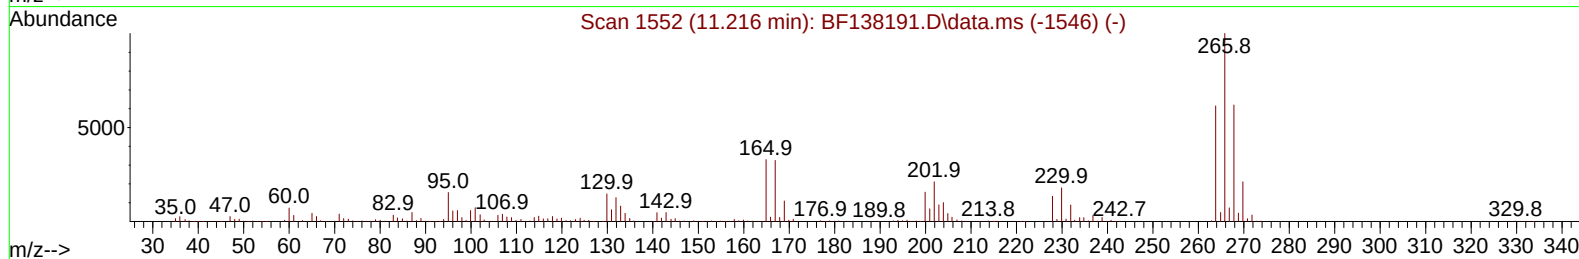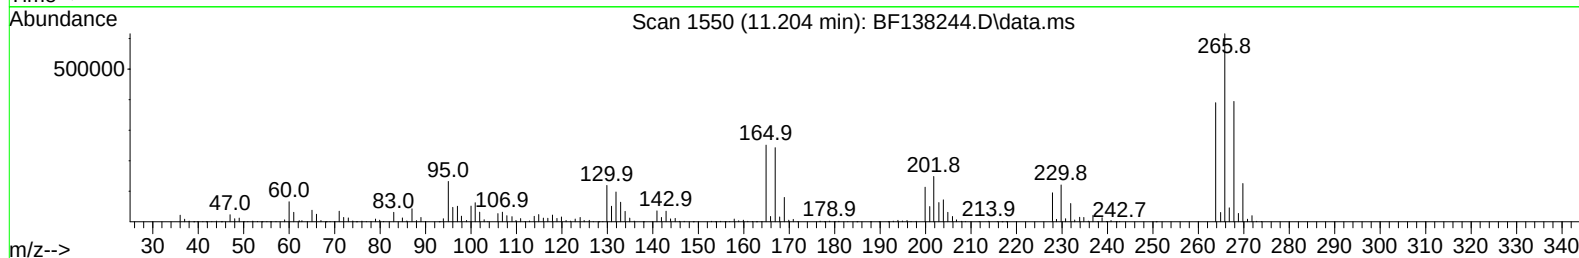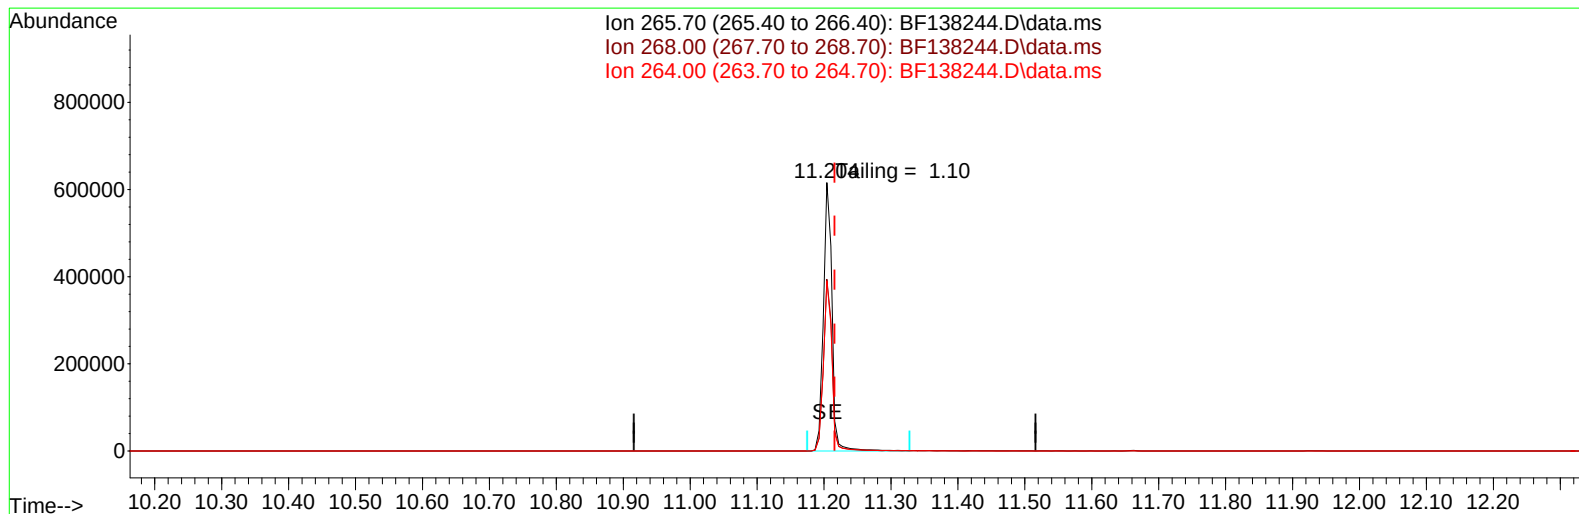

TIC: BF138244.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 245843.80 ng




response 550546

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.98
264.00	61.50	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061924\
Data File : BF138244.D
Acq On : 19 Jun 2024 14:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 19 15:33:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

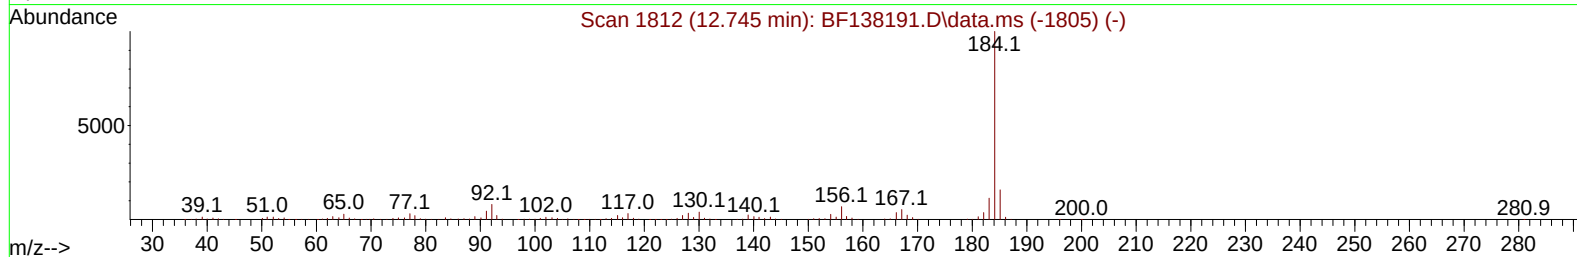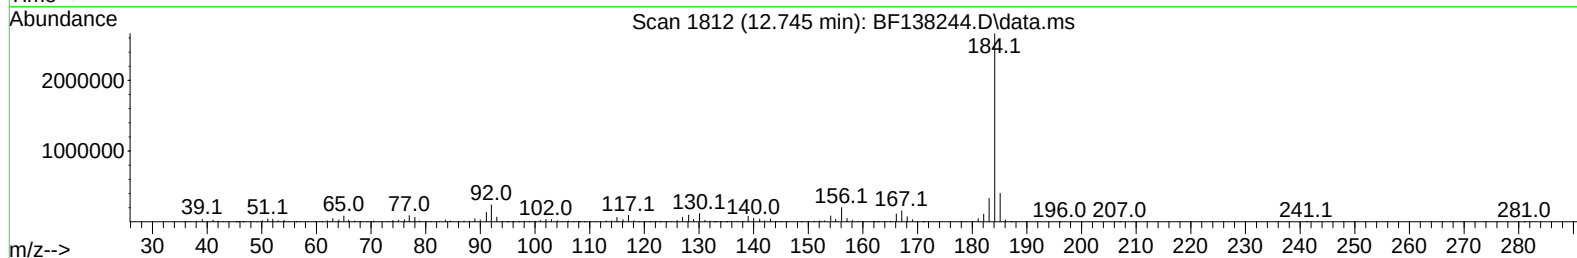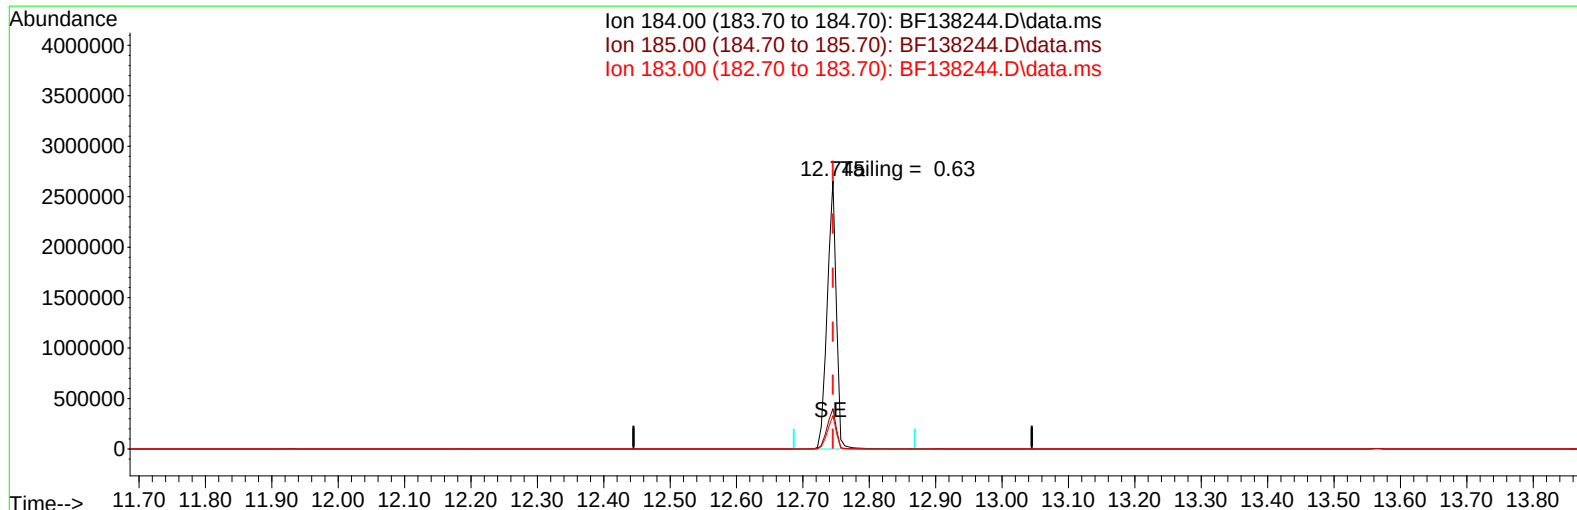

TIC: BF138244.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 324211.99 ng

response 2542545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.06
183.00	11.30	12.46
0.00	0.00	0.00