
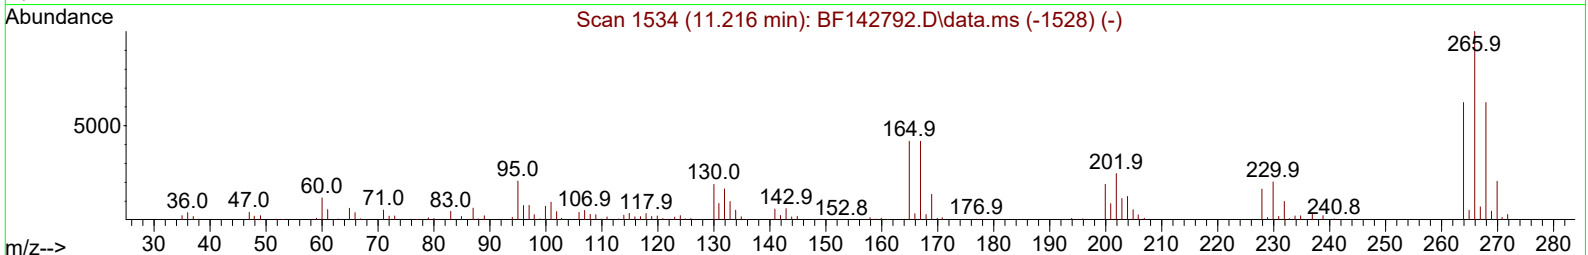
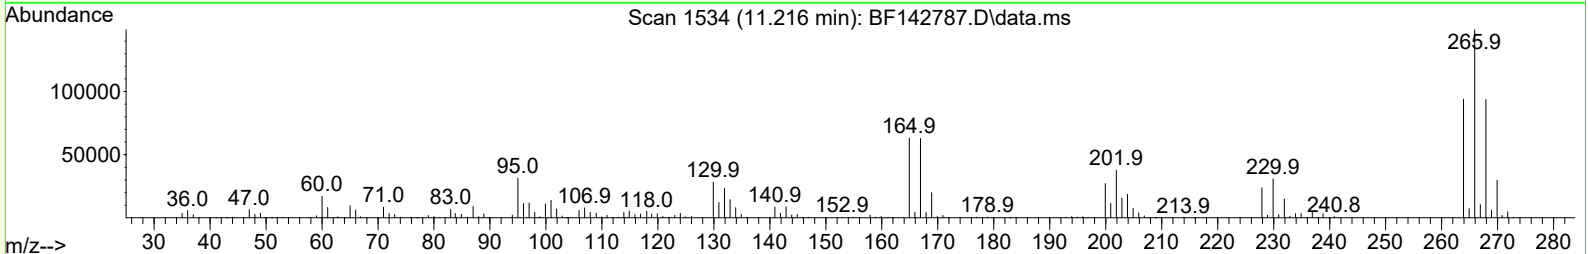


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061925\
 Data File : BF142787.D
 Acq On : 19 Jun 2025 16:37
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 05:38:32 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 20 05:06:14 2025
 Response via : Initial Calibration

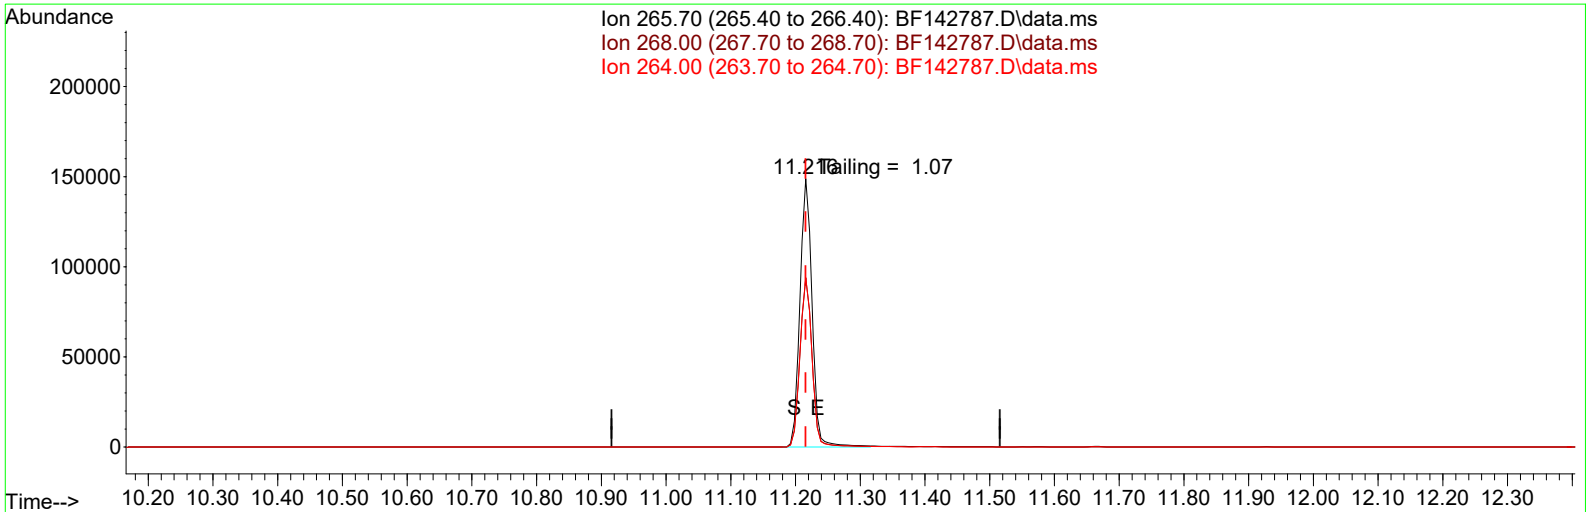

TIC: BF142787.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.000) 37164.56 ng

response 195787

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.94
264.00	62.40	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061925\
 Data File : BF142787.D
 Acq On : 19 Jun 2025 16:37
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 05:38:32 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 20 05:06:14 2025
 Response via : Initial Calibration

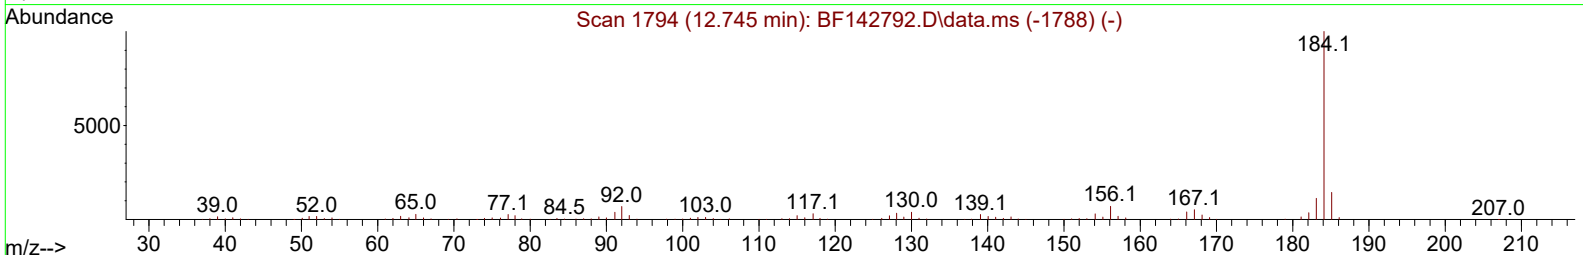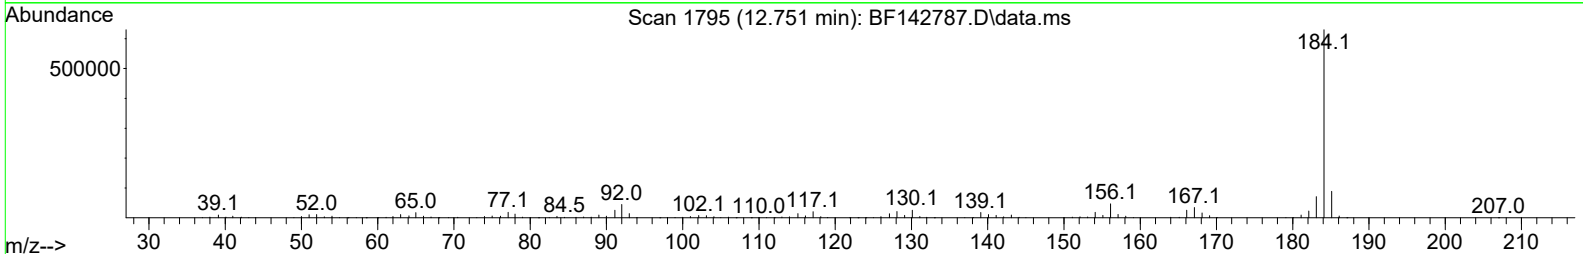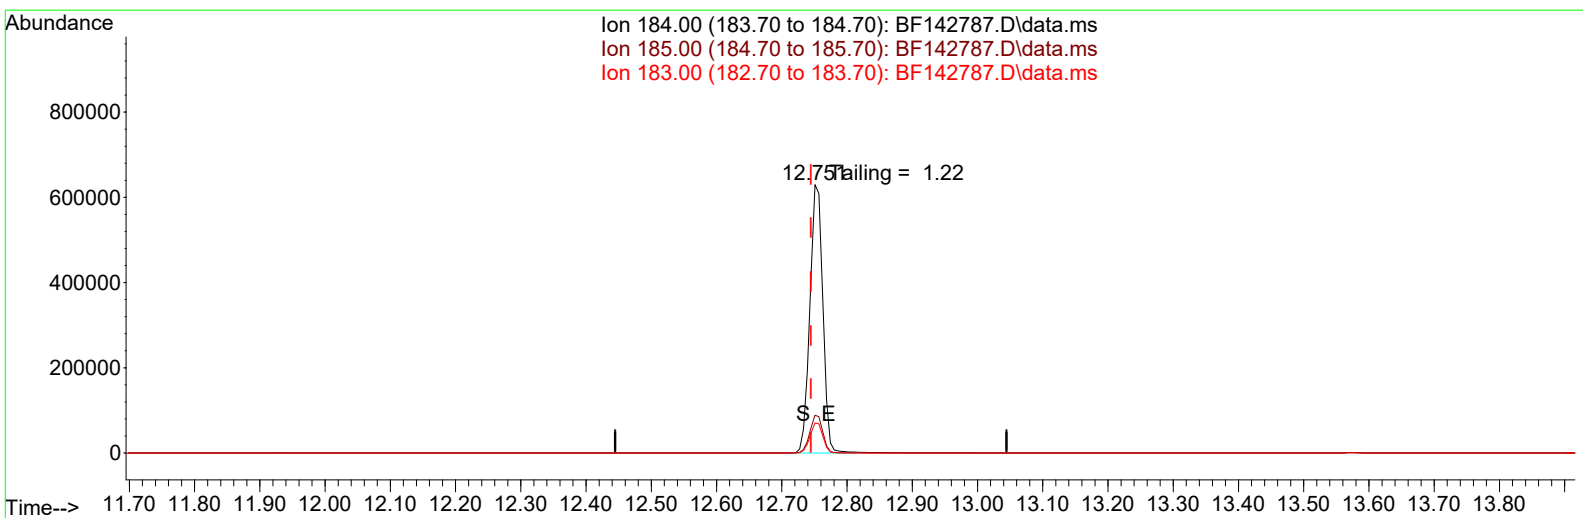

TIC: BF142787.D\data.ms

(77) Benzidine

12.751min (+ 0.006)	0.00 ng
response	874127
Ion	Exp% Act%
184.00	100.00 100.00
185.00	14.40 14.11
183.00	11.20 11.25
0.00	0.00 0.00