

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062016\
 Data File : BF088206.D
 Acq On : 21 Jun 2016 8:30
 Operator : UM/SJ
 Sample : H3580-17
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 08-B1(0-12)C

Quant Time: Jun 21 12:50:20 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 17:39:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	88748	20.00	ng	-0.01
21) Naphthalene-d8	7.95	136	363788	20.00	ng	0.00
38) Acenaphthene-d10	9.70	164	164328	20.00	ng	0.00
63) Phenanthrene-d10	11.18	188	311280	20.00	ng	0.00
75) Chrysene-d12	13.81	240	227941	20.00	ng	0.00
86) Perylene-d12	15.18	264	176034	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.27	112	577777	111.30	ng	0.01
7) Phenol-d6	6.32	99	617202	98.10	ng	-0.01
23) Nitrobenzene-d5	7.23	82	375091	60.21	ng	-0.01
41) 2,4,6-Tribromophenol	10.49	330	162967	93.92	ng	0.00
44) 2-Fluorobiphenyl	9.03	172	685412	64.17	ng	-0.01
78) Terphenyl-d14	12.75	244	569336	56.84	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.43	163	280554	23.57	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062016\
Data File : BF088206.D
Acq On : 21 Jun 2016 8:30
Operator : UM/SJ
Sample : H3580-17
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
08-B1(0-12)C

Quant Time: Jun 21 12:50:20 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 17:39:32 2016
Response via : Initial Calibration

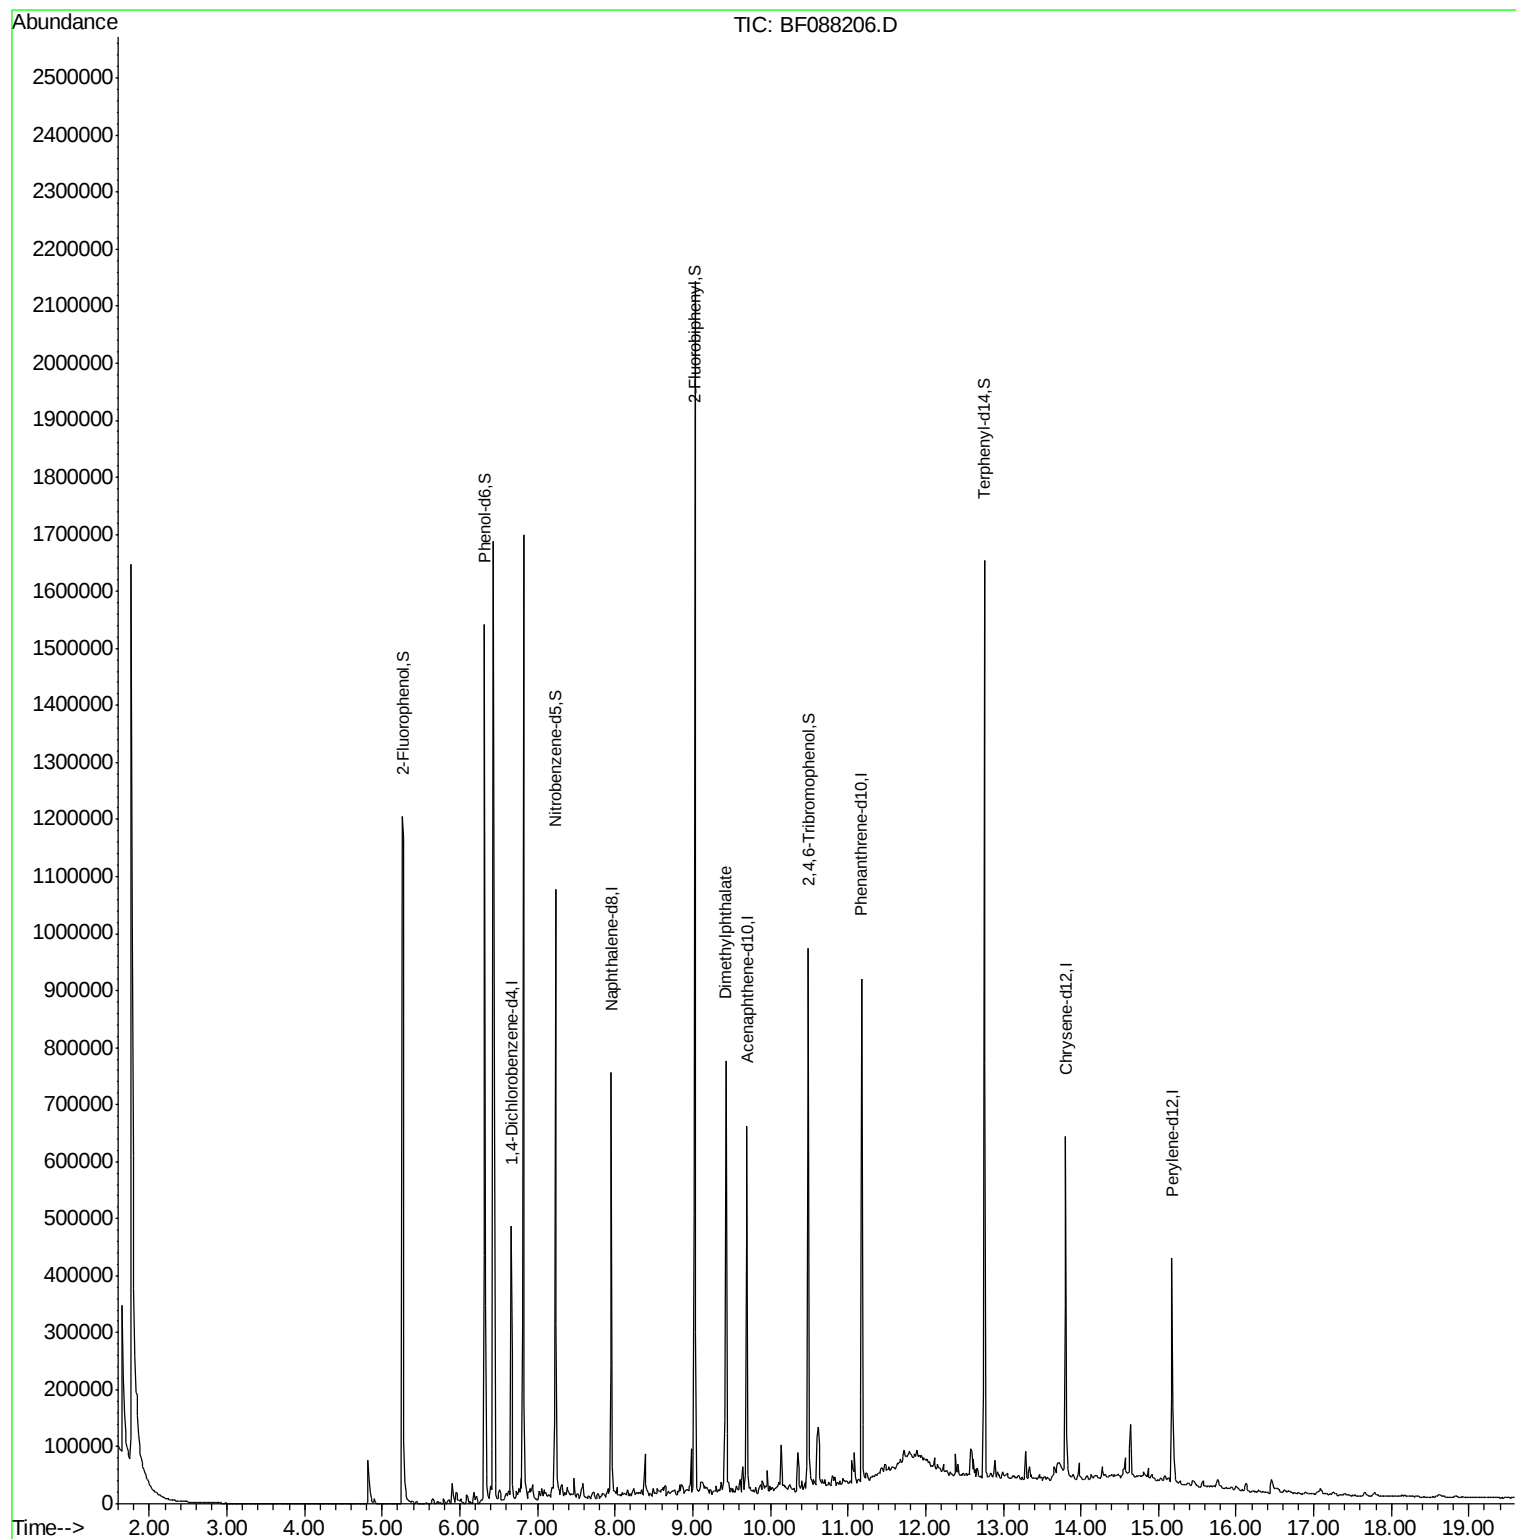

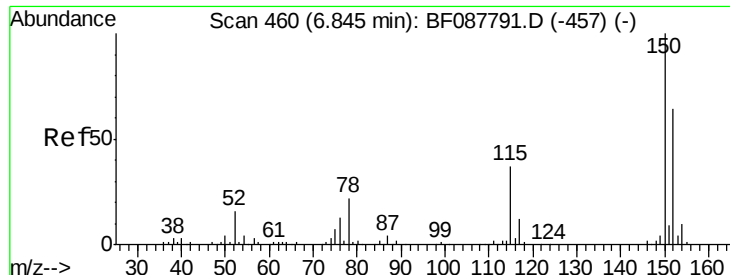

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.66 min Scan# 444

Delta R.T. -0.01 min

Lab File: BF088206.D

Acq: 21 Jun 2016 8:30

Instrument :

BNA_F

ClientSampleId :

08-B1(0-12)C


Tot Ion:152 Resp: 88748

Ion Ratio Lower Upper

152 100

150 160.2 123.8 185.6



115 68.0 39.6 59.4#

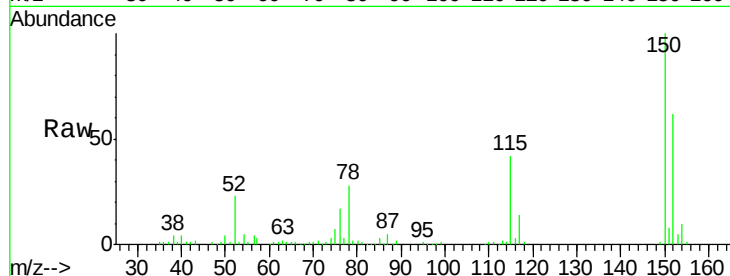

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

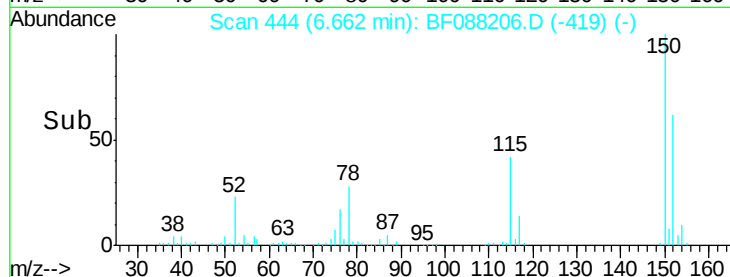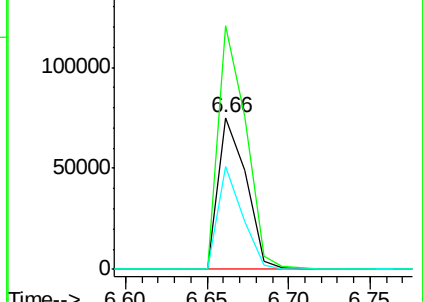

#5

2-Fluorophenol

Concen: 111.30 ng

RT: 5.27 min Scan# 322

Delta R.T. 0.01 min

Lab File: BF088206.D

Acq: 21 Jun 2016 8:30


Tgt Ion:112 Resp: 577777

Ion Ratio Lower Upper

112 100

64 44.4 42.2 63.2



63 22.3 21.8 32.8

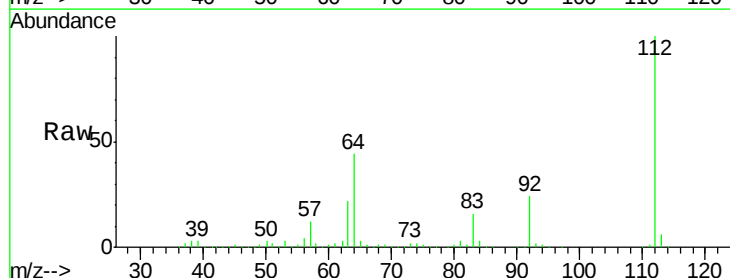

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

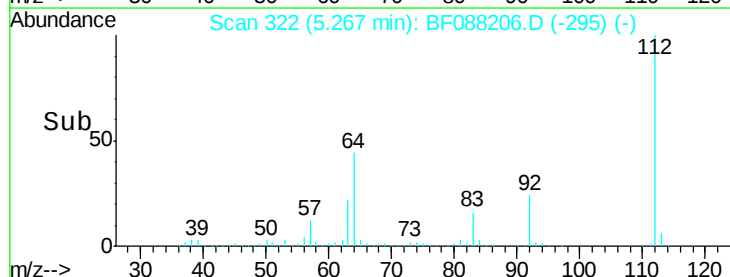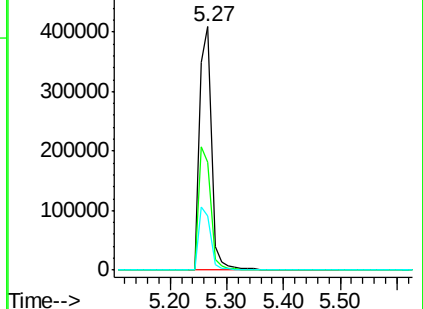



#7

Phenol-d6

Concen: 98.10 ng

RT: 6.32 min Scan# 414

Delta R.T. -0.01 min

Lab File: BF088206.D

Acq: 21 Jun 2016 8:30

Instrument :

BNA_F

ClientSampleId :

08-B1(0-12)C


Tot Ion: 99 Resp: 617202

Ion Ratio Lower Upper




99 100

42 15.5 12.2 18.2

71 33.8 23.4 35.0

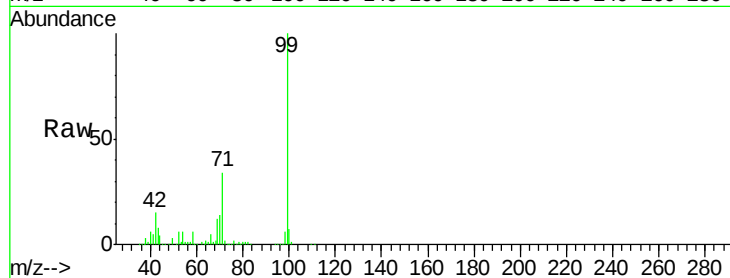

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

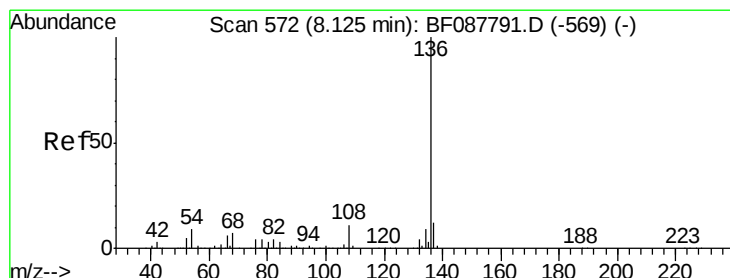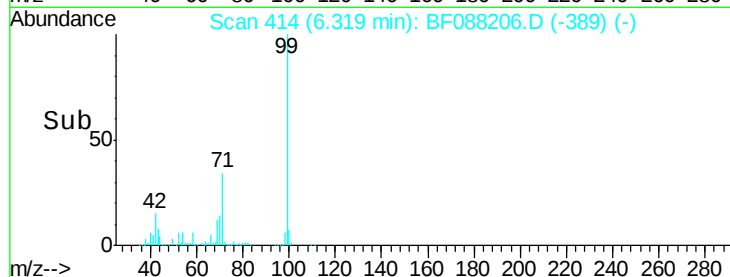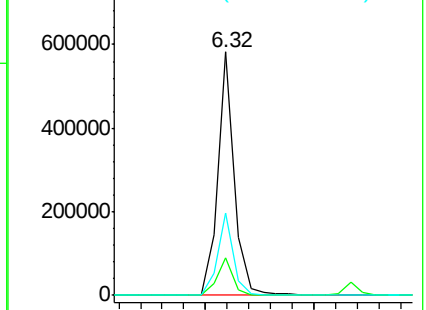

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 557

Delta R.T. -0.00 min

Lab File: BF088206.D

Acq: 21 Jun 2016 8:30

Tgt Ion: 136 Resp: 363788


Ion Ratio Lower Upper

136 100



137 10.7 9.1 13.7

54 5.9 6.6 10.0#

68 5.1 5.1 7.7#

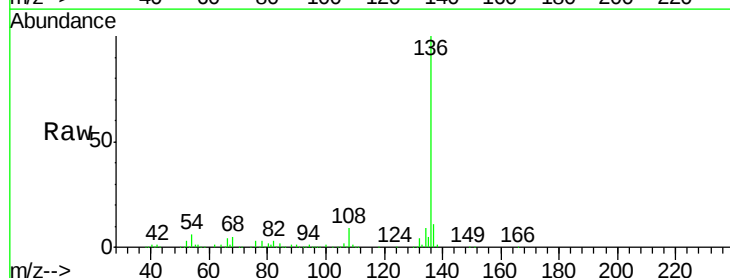

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

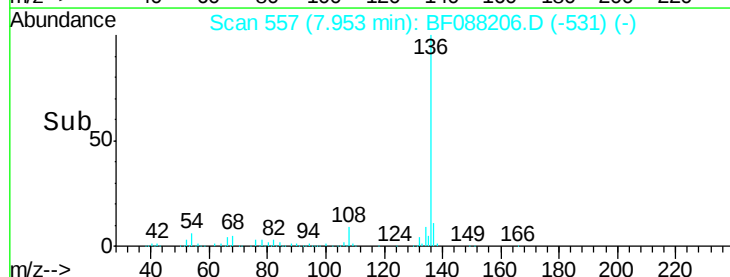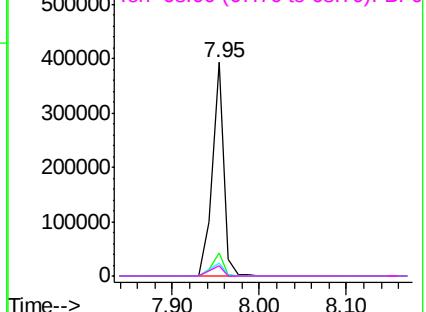







#23
Nitrobenzene-d5
Concen: 60.21 ng
RT: 7.23 min Scan# 494
Delta R.T. -0.01 min
Lab File: BF088206.D
Acq: 21 Jun 2016 8:30

Instrument :
BNA_F
ClientSampleId :
08-B1(0-12)C

Tot Ion: 82 Resp: 375091
Ion Ratio Lower Upper
82 100
128 46.2 35.9 53.9
54 46.8 40.9 61.3

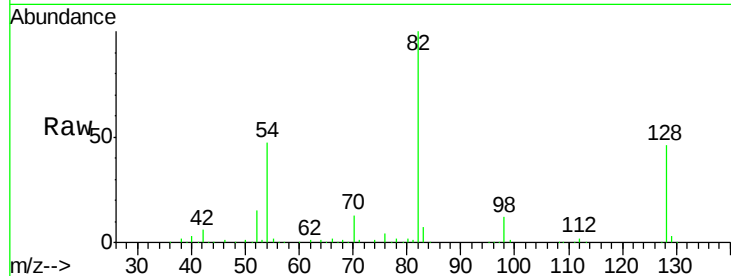


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

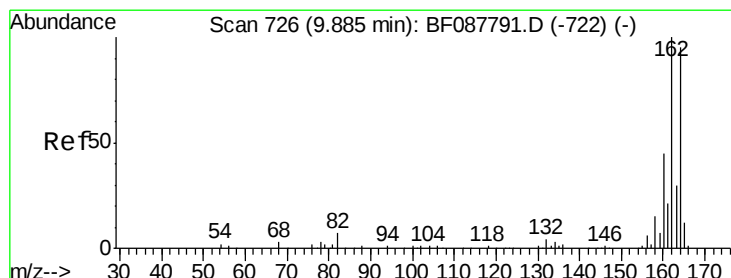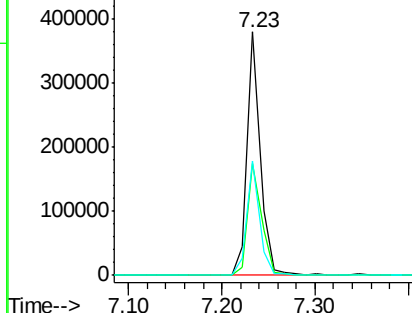
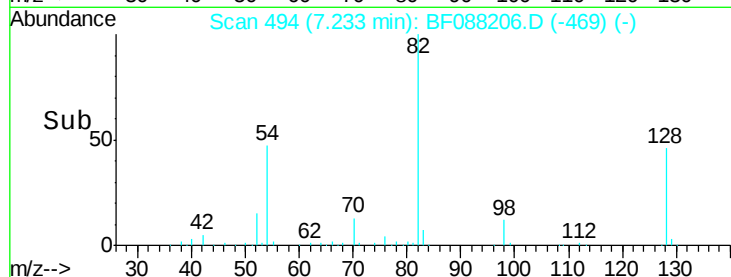


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.70 min Scan# 710
Delta R.T. -0.00 min
Lab File: BF088206.D
Acq: 21 Jun 2016 8:30

Tgt Ion:164 Resp: 164328
Ion Ratio Lower Upper
164 100
162 106.8 85.4 128.2
160 48.7 39.5 59.3

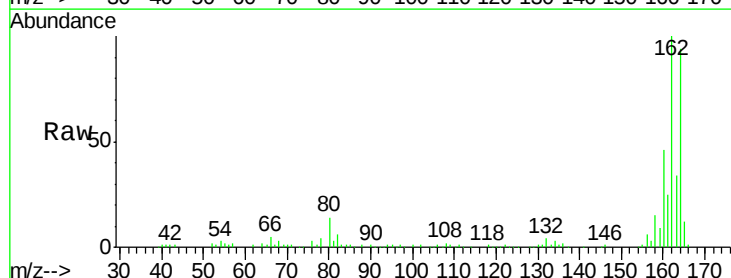

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

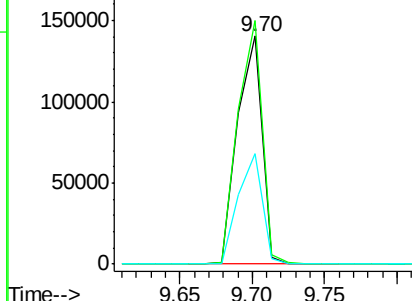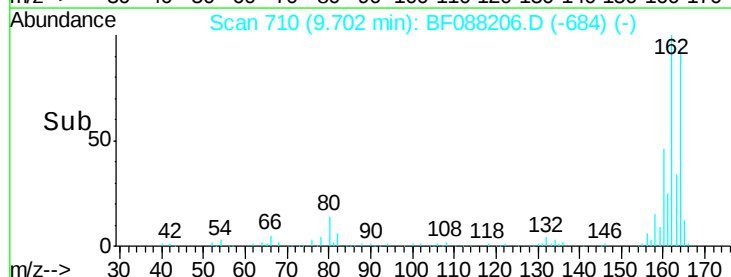






#41
 2,4,6-Tribromophenol
 Concen: 93.92 ng
 RT: 10.49 min Scan# 779
 Delta R.T. -0.00 min
 Lab File: BF088206.D
 Acq: 21 Jun 2016 8:30

Instrument :
 BNA_F
 ClientSampleId :
 08-B1(0-12)C

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	0.0	0.0#
141	36.8	0.0	0.0#

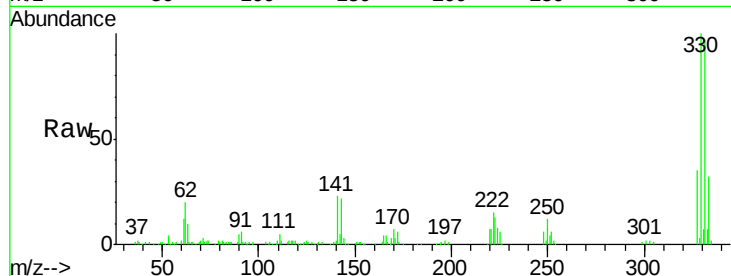


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

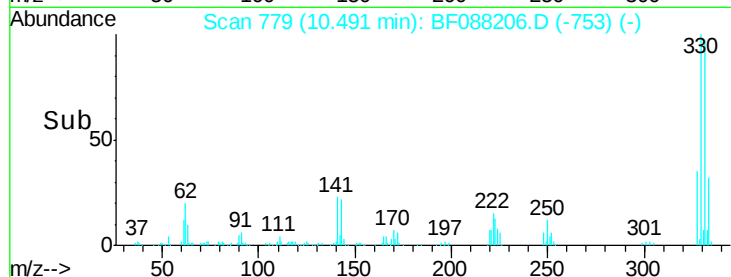
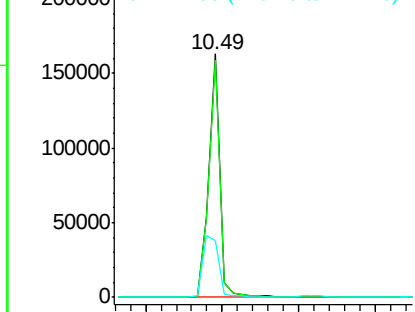



#44
 2-Fluorobiphenyl
 Concen: 64.17 ng
 RT: 9.03 min Scan# 651
 Delta R.T. -0.01 min
 Lab File: BF088206.D
 Acq: 21 Jun 2016 8:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	28.6	43.0
170	24.1	19.2	28.8

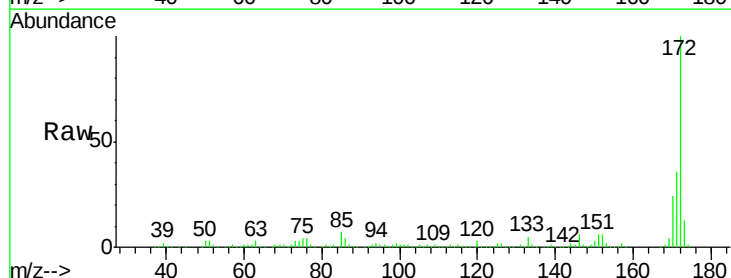

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

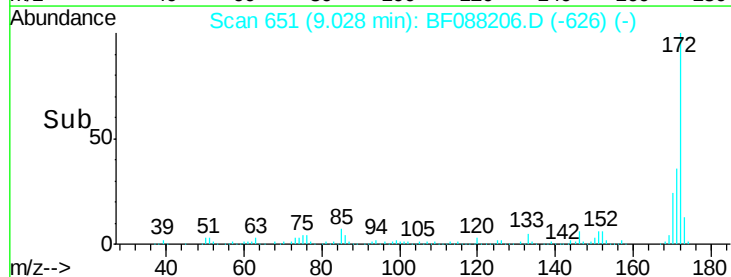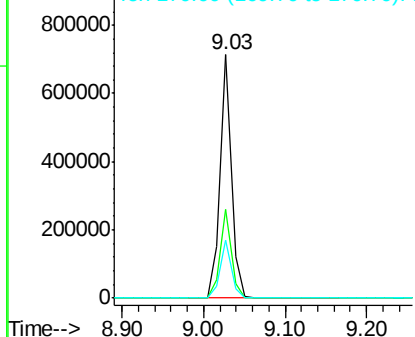

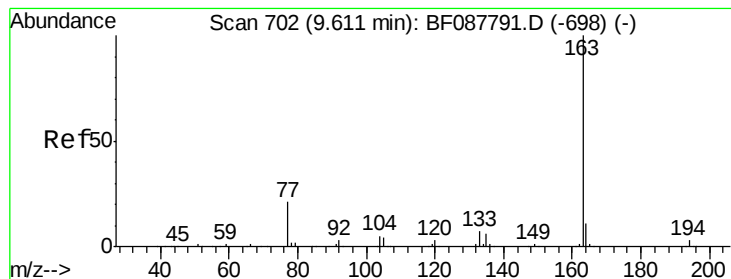

#49

Dimethylphthalate

Concen: 23.57 ng

RT: 9.43 min Scan# 686

Delta R.T. -0.01 min

Lab File: BF088206.D

Acq: 21 Jun 2016 8:30

Instrument :

BNA_F

ClientSampleId :

08-B1(0-12)C


Tot Ion:163 Resp: 280554

Ion Ratio Lower Upper

163 100

194 3.4 2.8 4.2




164 10.2 8.3 12.5

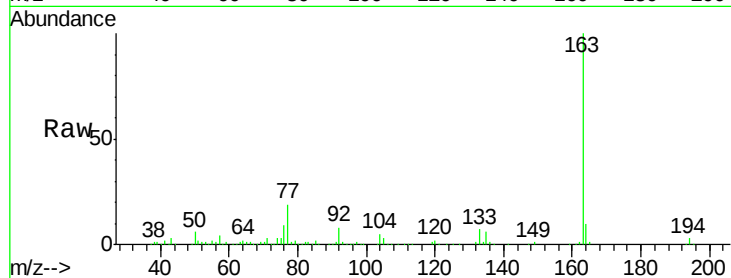

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

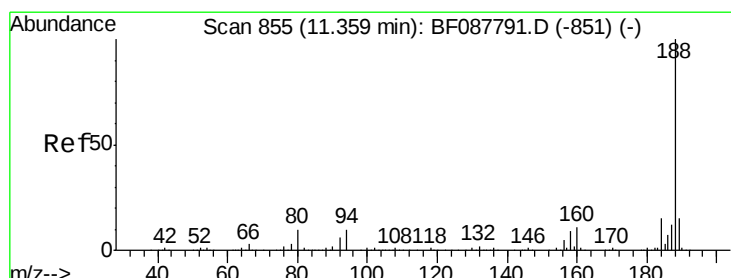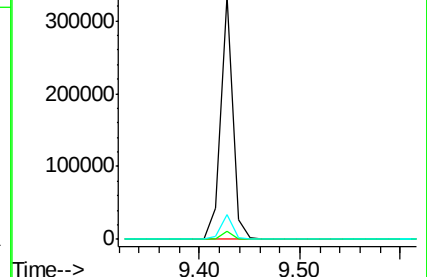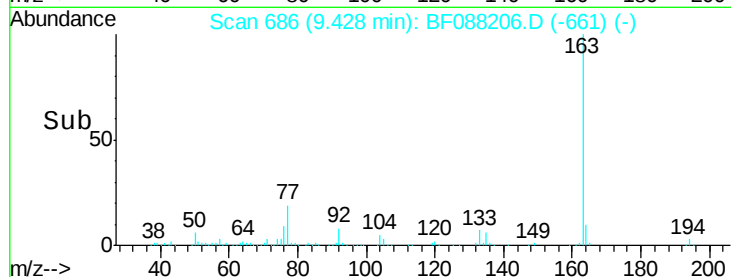

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.18 min Scan# 839

Delta R.T. -0.00 min

Lab File: BF088206.D

Acq: 21 Jun 2016 8:30


Tgt Ion:188 Resp: 311280

Ion Ratio Lower Upper

188 100

94 9.2 9.0 13.6



80 9.3 10.0 15.0#

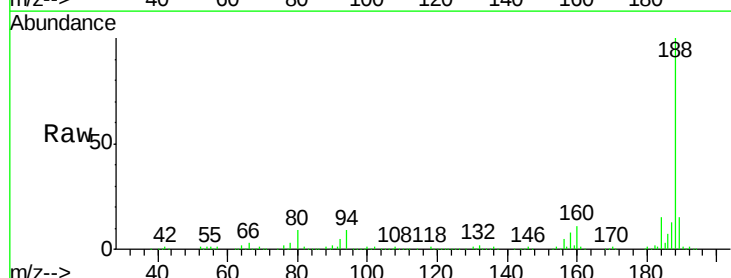

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



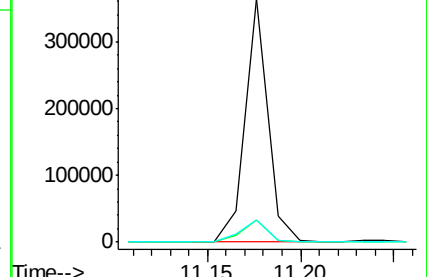
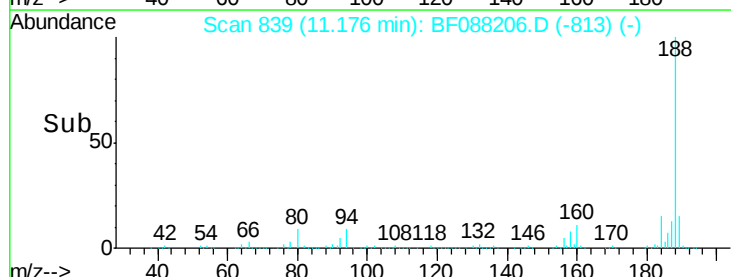




#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.81 min Scan# 1069
Delta R.T. -0.00 min
Lab File: BF088206.D
Acq: 21 Jun 2016 8:30




Instrument :
BNA_F
ClientSampleId :
08-B1(0-12)C




Tot Ion:240 Resp: 227941
Ion Ratio Lower Upper
240 100
120 9.8 6.8 10.2
236 25.1 20.2 30.2

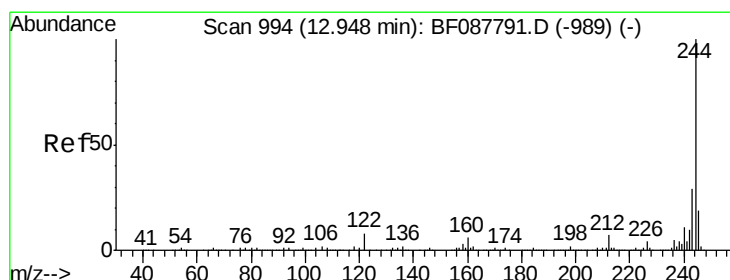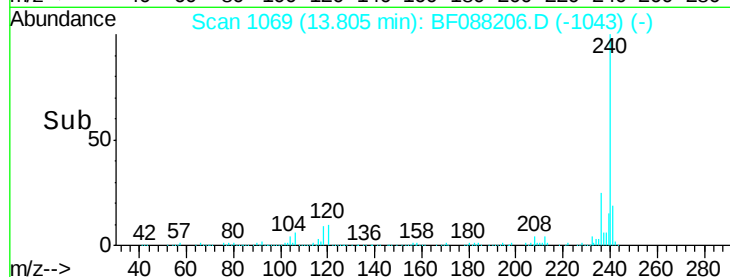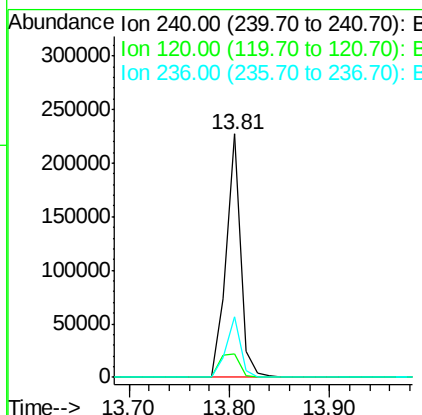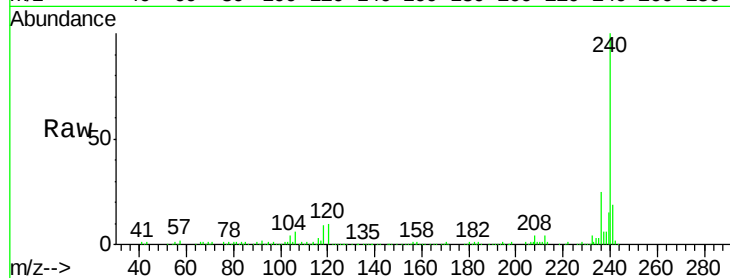

#78
Terphenyl-d14
Concen: 56.84 ng
RT: 12.75 min Scan# 977
Delta R.T. -0.01 min
Lab File: BF088206.D
Acq: 21 Jun 2016 8:30

Tgt Ion:244 Resp: 569336
Ion Ratio Lower Upper
244 100
212 7.7 6.0 9.0
122 16.1 11.2 16.8

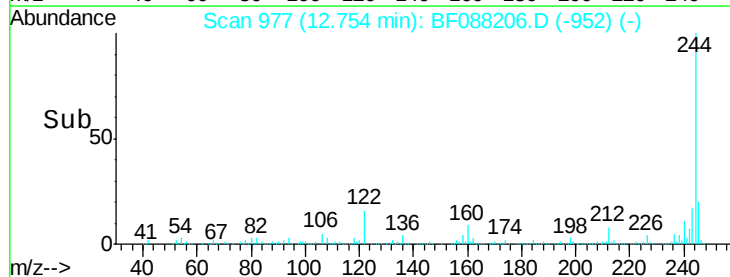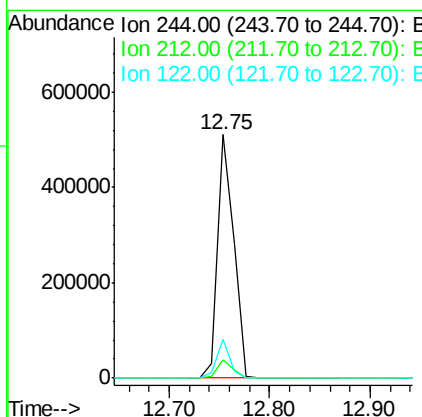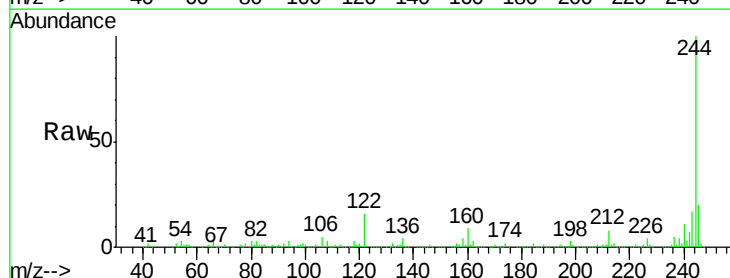

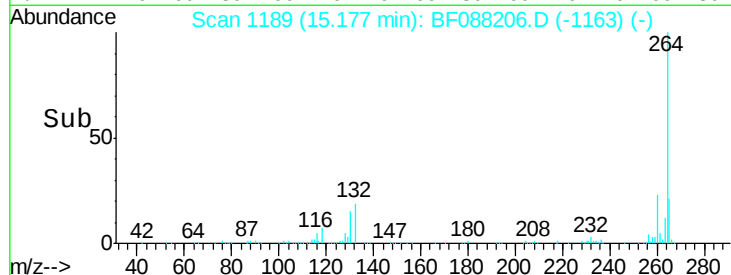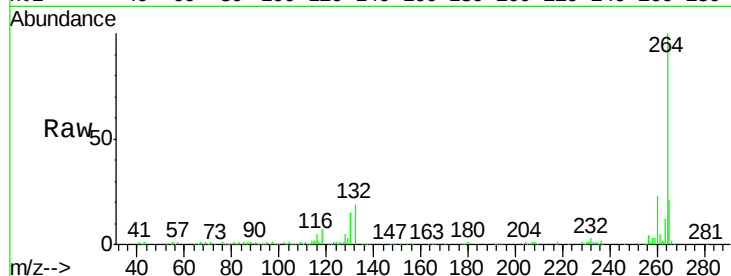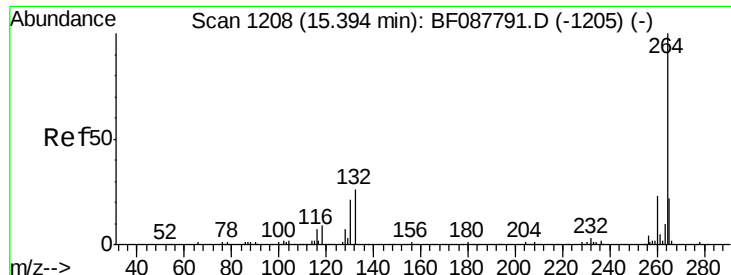

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.18 min Scan# 1189
 Delta R.T. -0.00 min
 Lab File: BF088206.D
 Acq: 21 Jun 2016 8:30

Instrument :
 BNA_F
 ClientSampleId :
 08-B1(0-12)C

Tot Ion:	264	Resp:	176034
Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.2	16.9	25.3

