

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062016\
 Data File : BF088184.D
 Acq On : 20 Jun 2016 21:22
 Operator : UM/SJ
 Sample : PB91264BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB91264BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.655	4	6	14	rVV	304350	549699	18.83%	2.270%
2	1.770	14	16	59	rVB	1043588	2226266	76.28%	9.193%
3	4.833	282	284	294	rVB	75632	119747	4.10%	0.494%
4	5.267	320	322	335	rBV	1955869	2102648	72.05%	8.682%
5	6.319	412	414	417	rBV	1528602	2046237	70.11%	8.449%
6	6.433	422	424	427	rBV	1665547	2156718	73.90%	8.906%
7	6.662	443	444	447	rBV	548243	603602	20.68%	2.492%
8	6.822	455	458	460	rBV	1985228	1764374	60.45%	7.286%
9	7.233	492	494	497	rBV	1188320	1305797	44.74%	5.392%
10	7.953	555	557	559	rBV	848621	851662	29.18%	3.517%
11	9.028	648	651	654	rBV	2388313	2584123	88.54%	10.671%
12	9.702	707	710	712	rBV	882618	957746	32.82%	3.955%
13	10.491	776	779	781	rBV	1106024	1336719	45.80%	5.520%
14	11.176	837	839	841	rBV	1164519	1003511	34.38%	4.144%
15	12.594	961	963	964	rBB	38319	45863	1.57%	0.189%
16	12.765	975	978	980	rBV	2320694	2918520	100.00%	12.051%
17	13.805	1067	1069	1071	rBV	916319	926350	31.74%	3.825%
18	15.177	1186	1189	1196	rBV	590998	717743	24.59%	2.964%


Sum of corrected areas: 24217325

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062016\
Data File : BF088184.D
Acq On : 20 Jun 2016 21:22
Operator : UM/SJ
Sample : PB91264BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91264BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

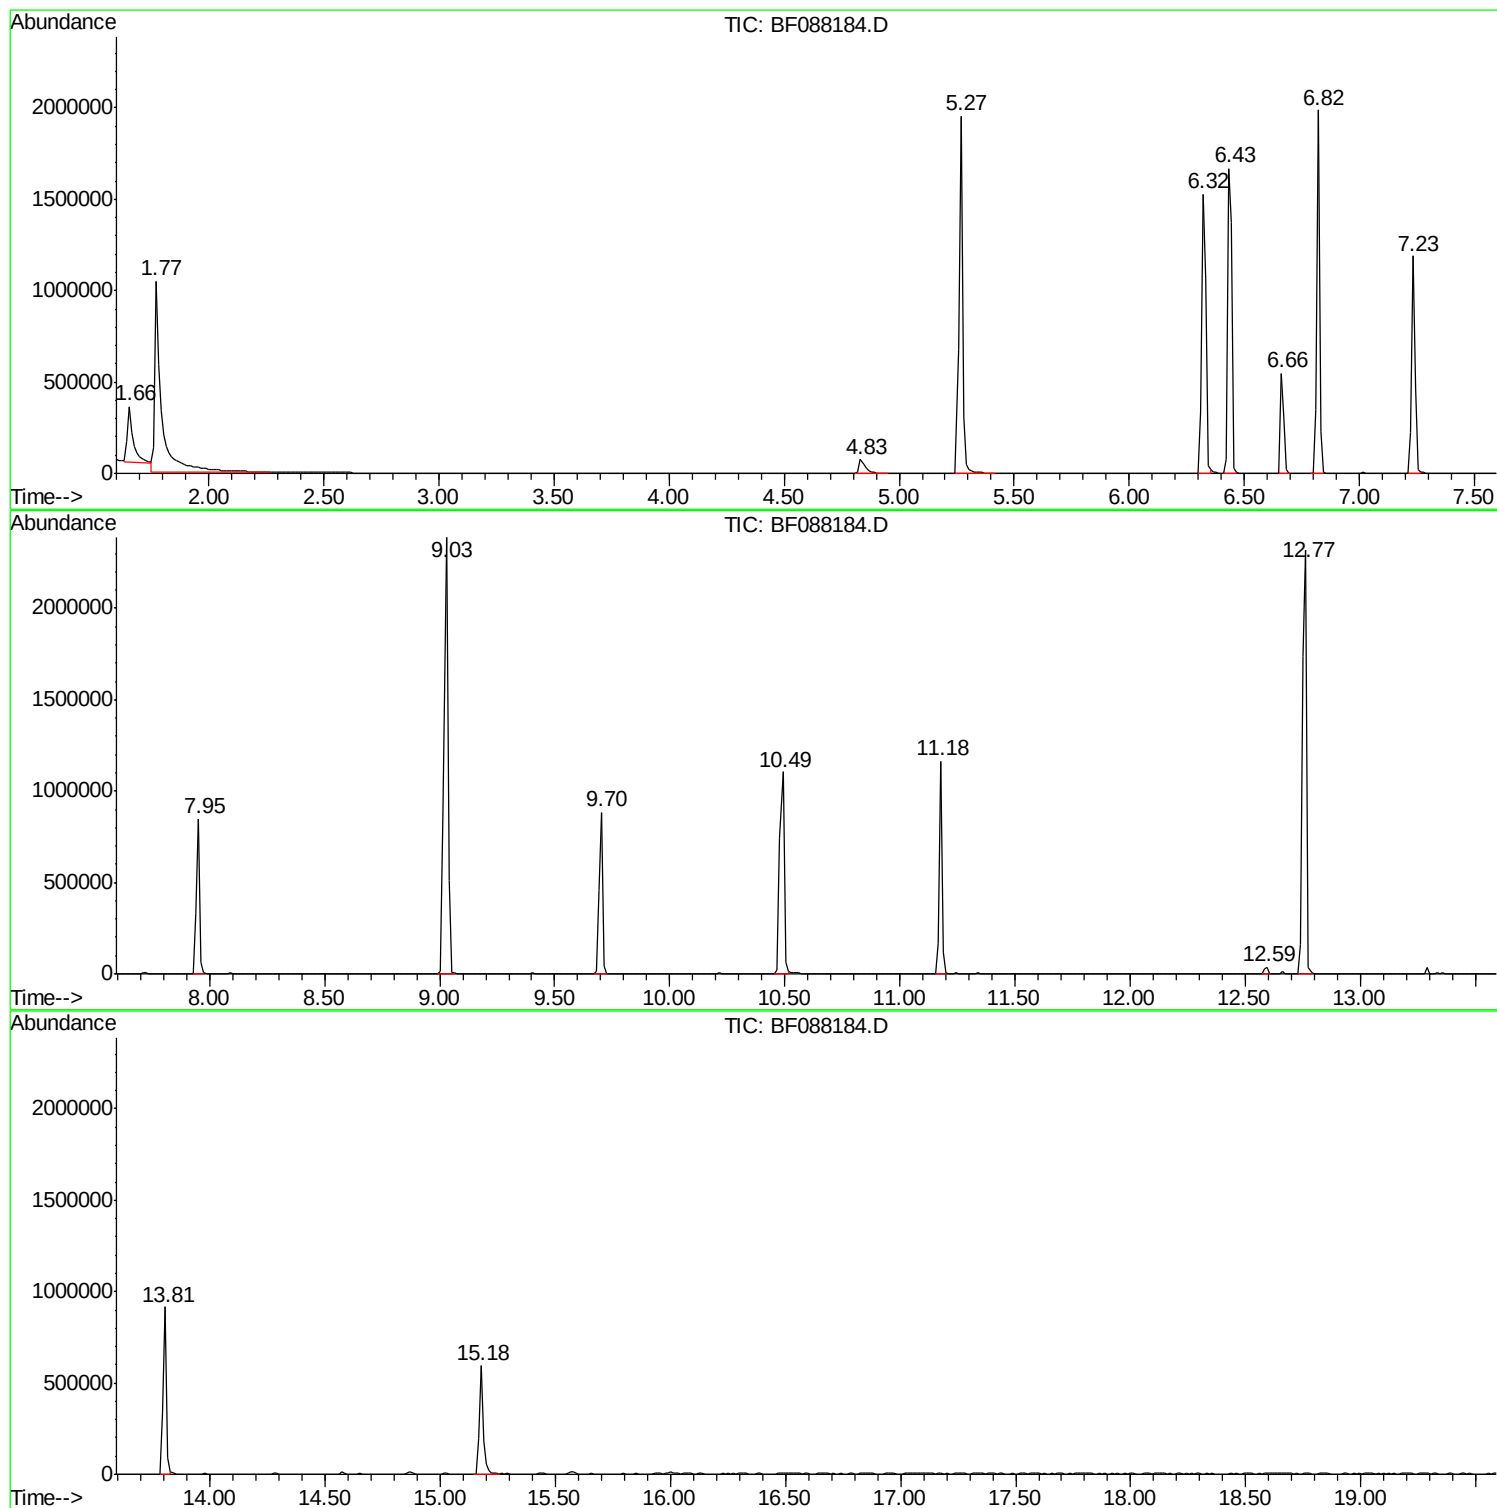

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062016\
Data File : BF088184.D
Acq On : 20 Jun 2016 21:22
Operator : UM/SJ
Sample : PB91264BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleID :
PB91264BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.83	3.97 ng	119747	1,4-Dichlorobenzene-d4	6.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
3		Acetone	58	C3H6O	000067-64-1	9
4		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

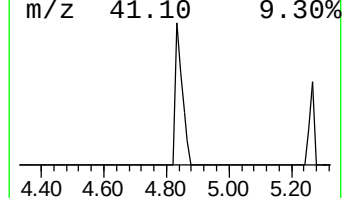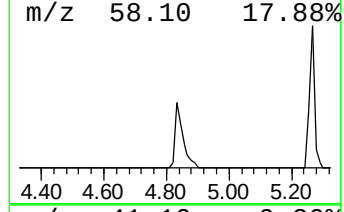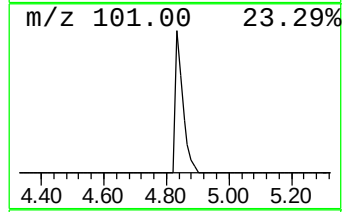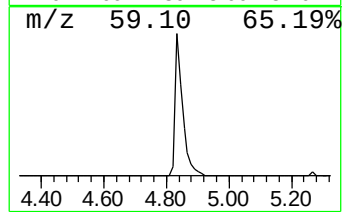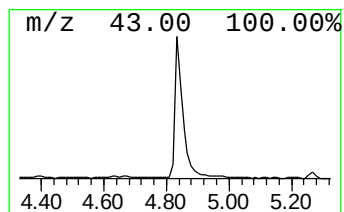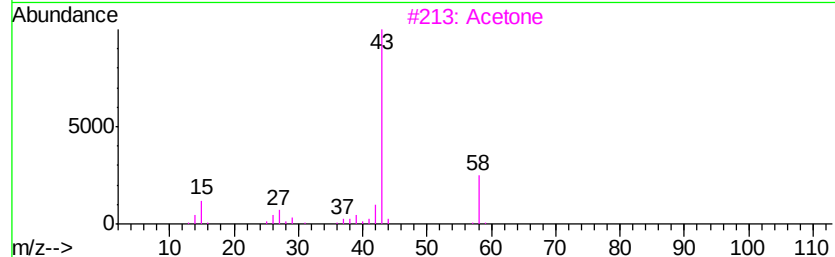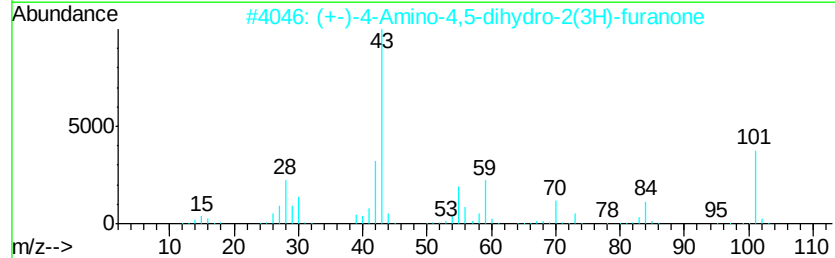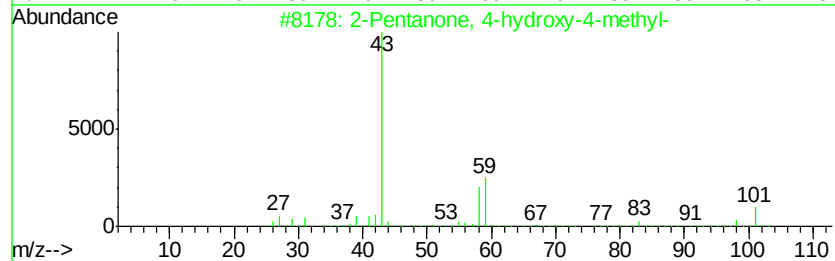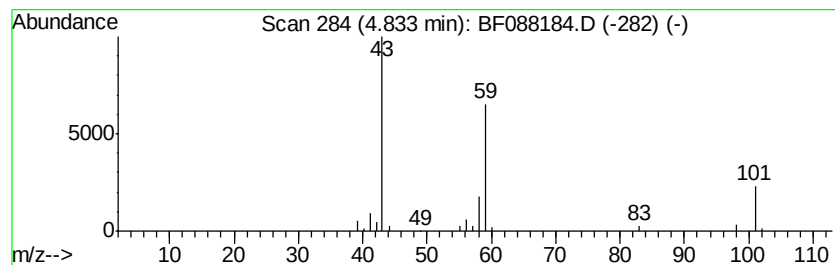

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062016\
Data File : BF088184.D
Acq On : 20 Jun 2016 21:22
Operator : UM/SJ
Sample : PB91264BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91264BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.43 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	71.46 ng	2156720	1,4-Dichlorobenzene-d4	6.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

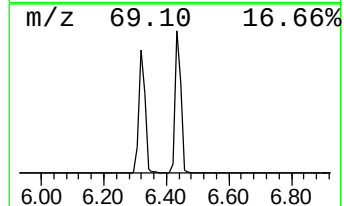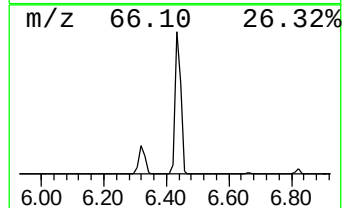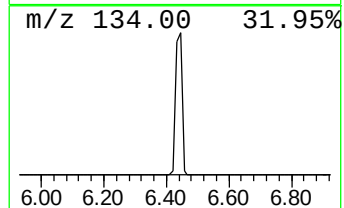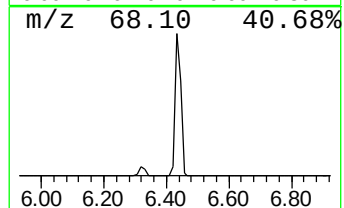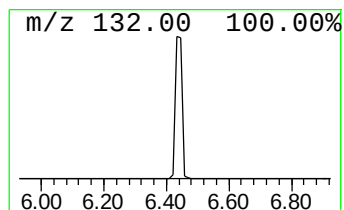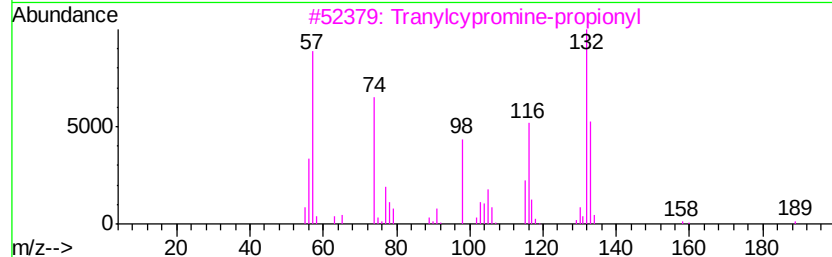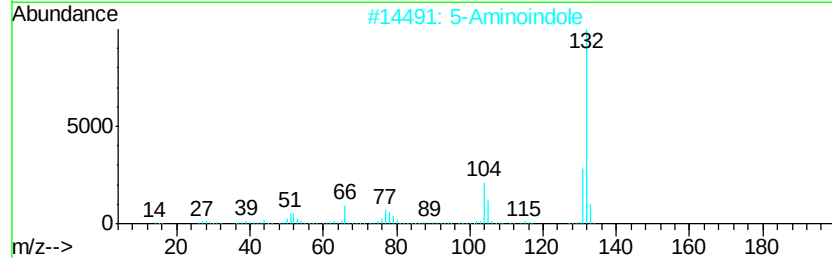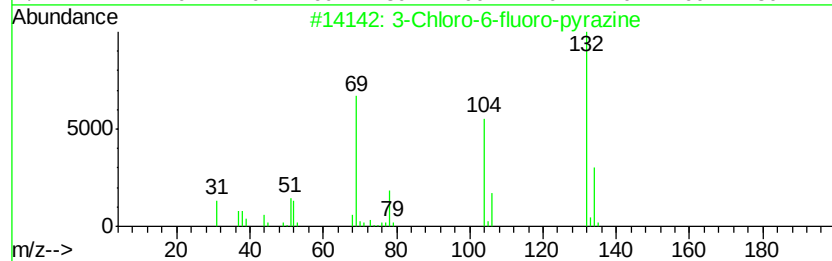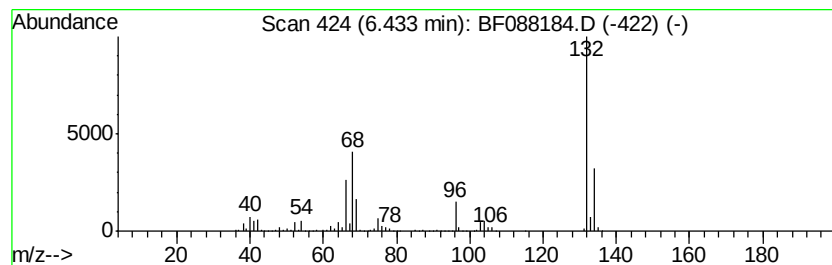

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062016\
Data File : BF088184.D
Acq On : 20 Jun 2016 21:22
Operator : UM/SJ
Sample : PB91264BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91264BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.83	4.0	ng	119747	1	6.66	603602	20.0
unknown6.43	6.43	71.5	ng	2156720	1	6.66	603602	20.0