


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062016\
 Data File : BF088171.D
 Acq On : 20 Jun 2016 14:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 20 17:39:32 2016

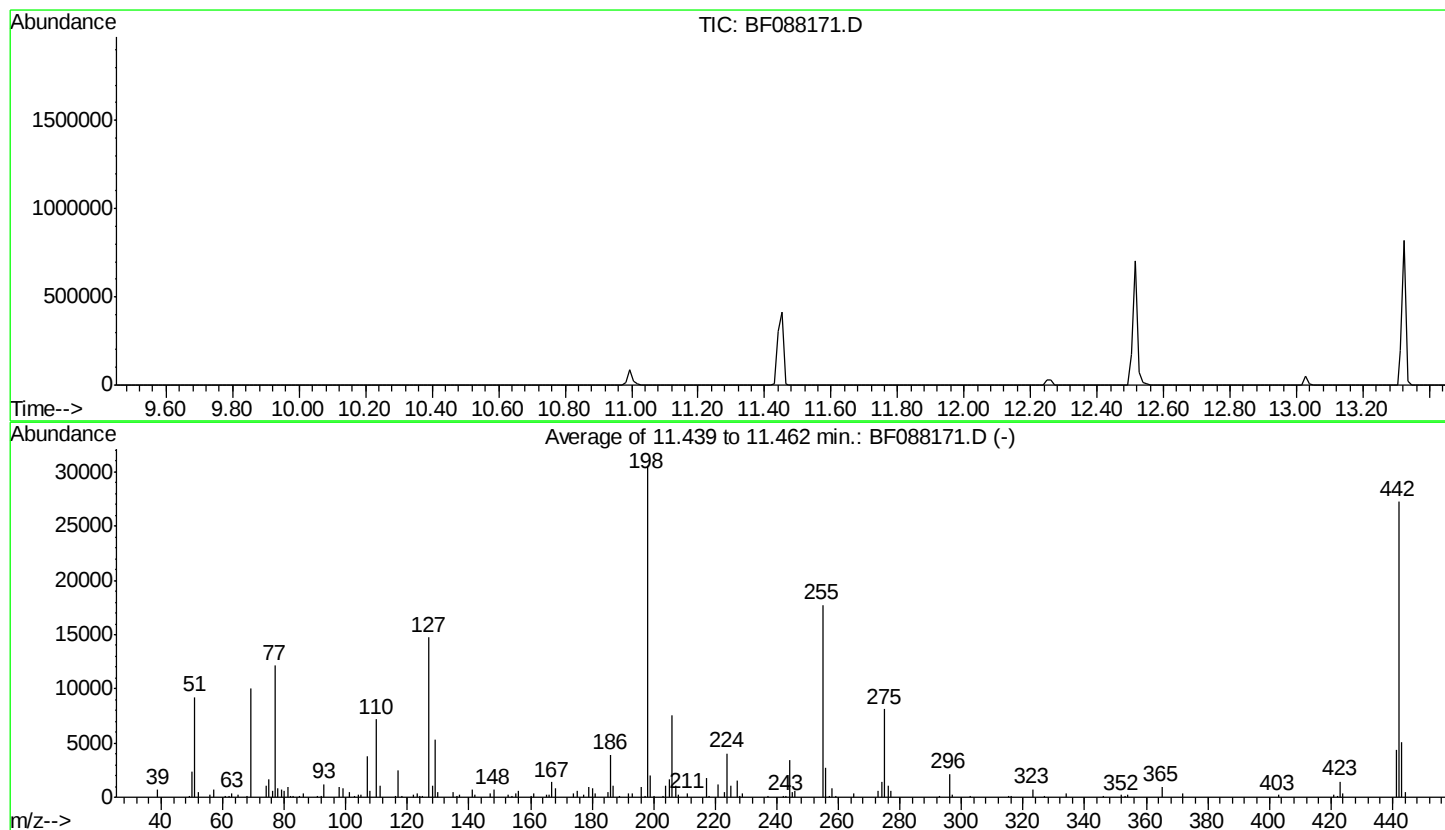

AutoFind: Scans 862, 863, 864; Background Corrected with Scan 858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	9247	PASS
68	69	0.00	2	1.3	129	PASS
69	198	0.00	100	32.8	10023	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	14733	PASS
197	198	0.00	2	0.4	109	PASS
198	198	100	100	100.0	30589	PASS
199	198	5	9	6.7	2037	PASS
275	198	10	60	26.5	8098	PASS
365	198	1	100	3.2	988	PASS
441	442	0.01	24	16.0	4360	PASS
442	198	50	100	89.1	27246	PASS
443	442	15	24	18.8	5121	PASS