
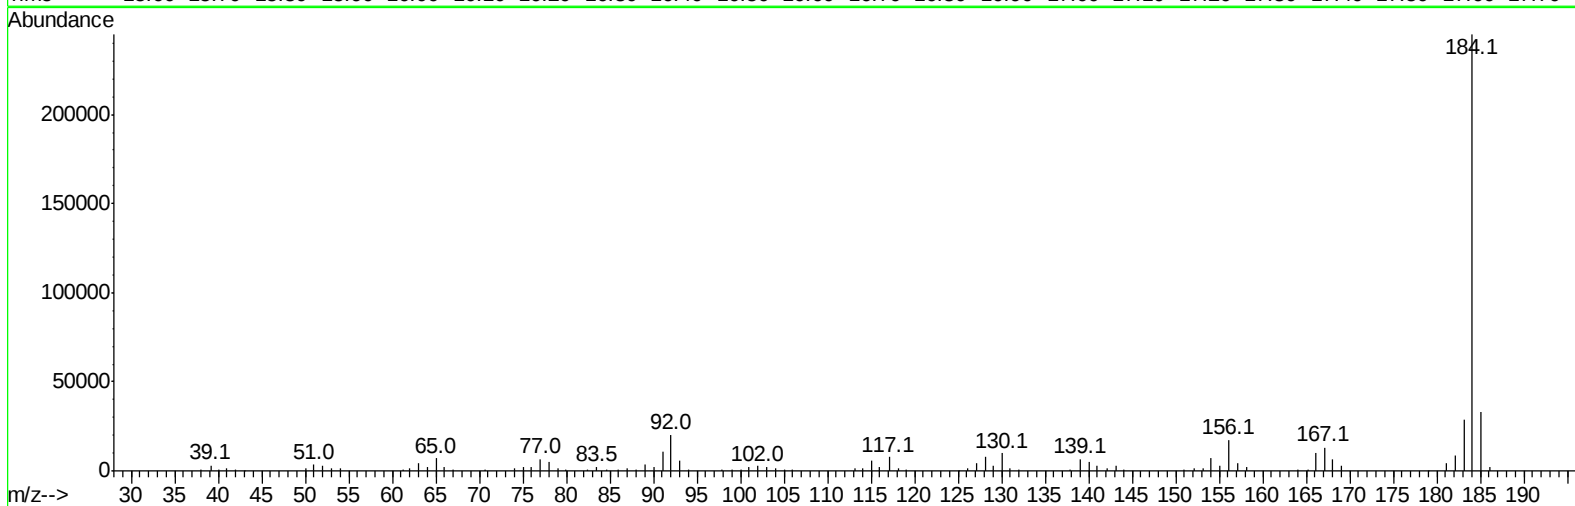


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
Data File : BF096042.D
Acq On : 20 Jun 2017 13:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 07:52:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

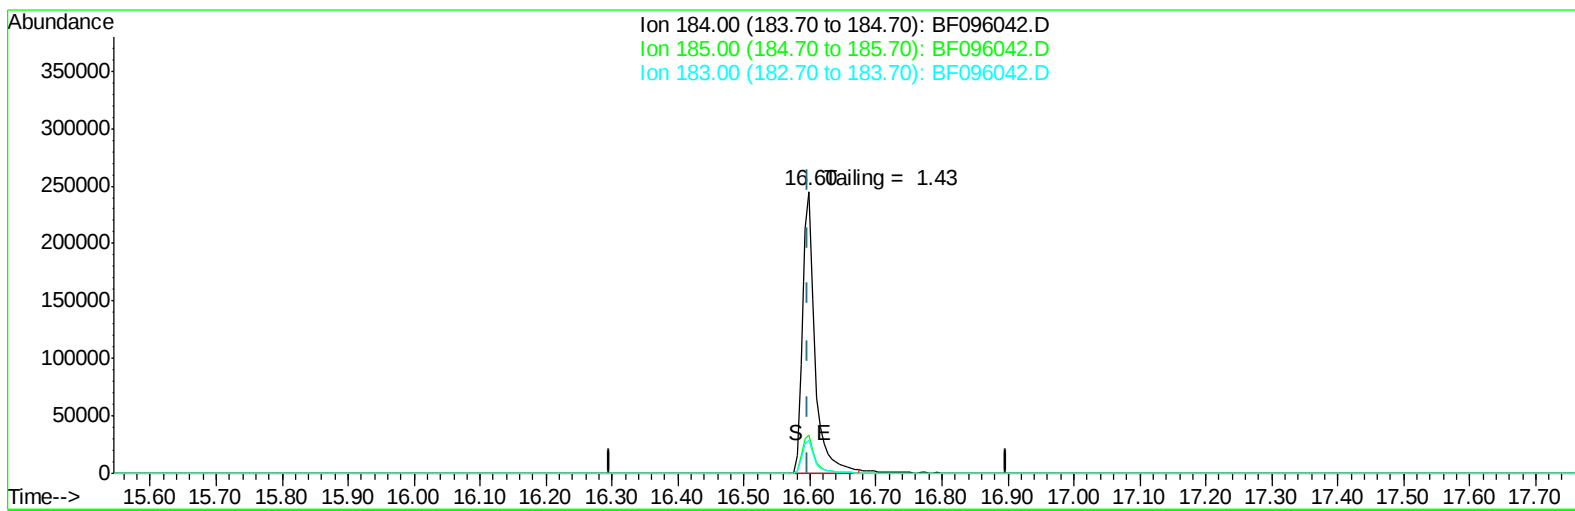

TIC: BF096042.D

(76) Benzidine



16.598min (+0.000) 0.00ng

response 333399

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.53#
183.00	12.20	11.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
Data File : BF096042.D
Acq On : 20 Jun 2017 13:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 07:52:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

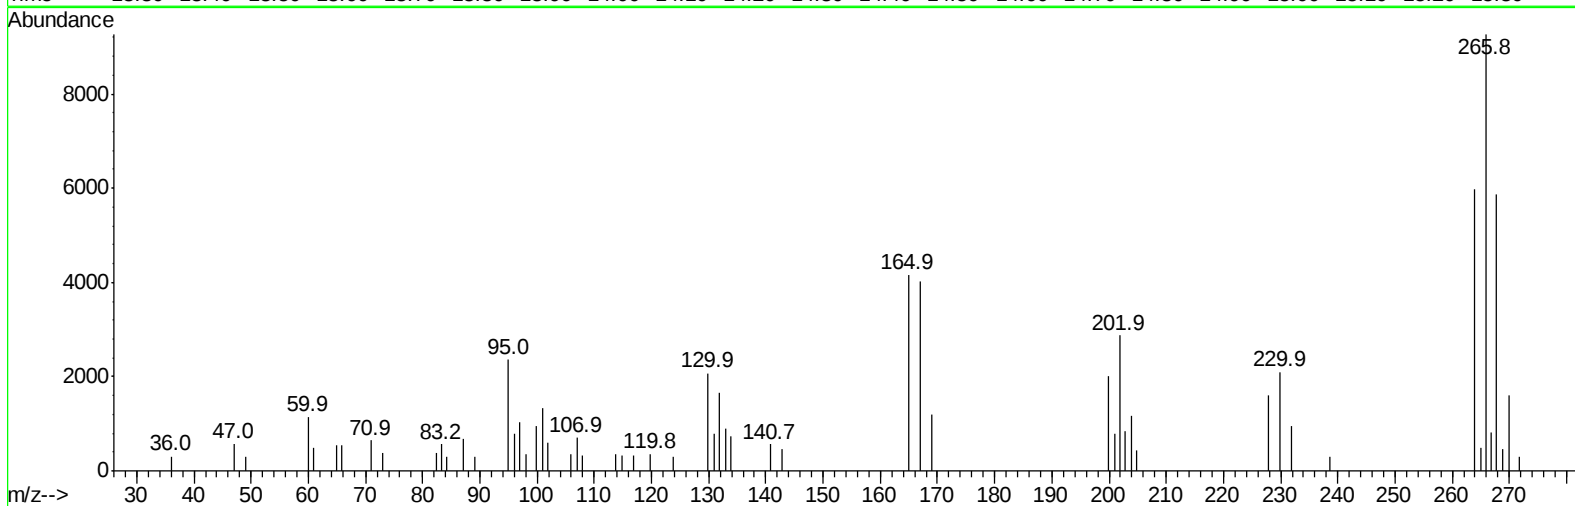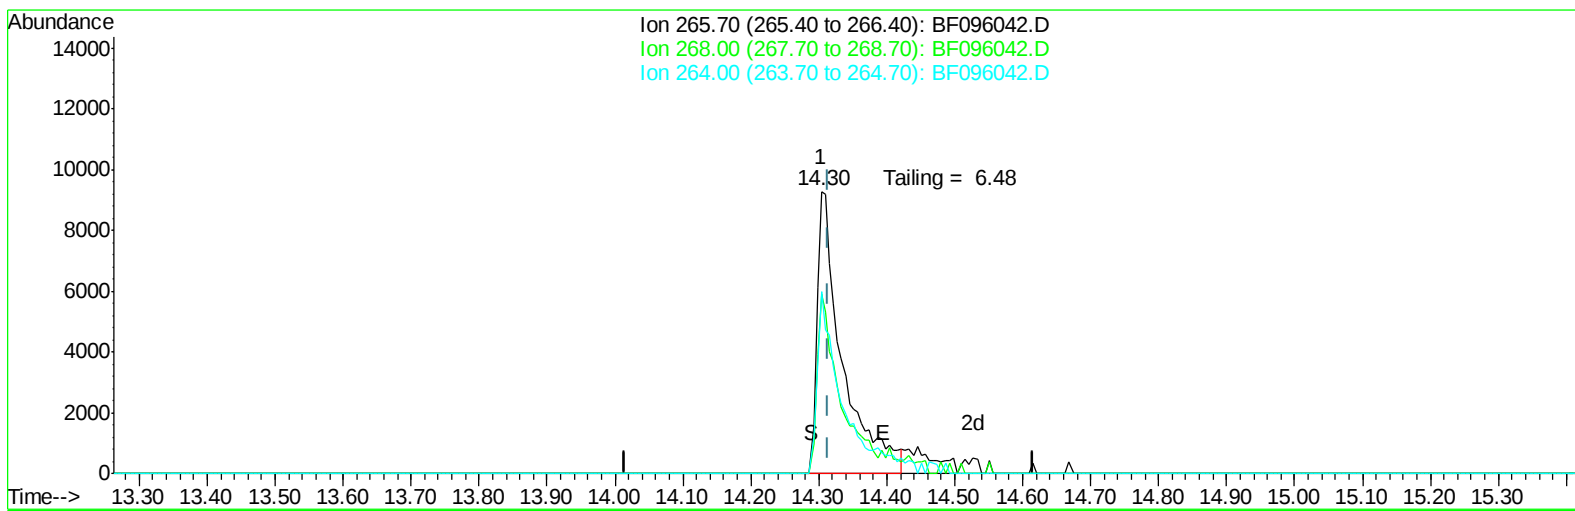

TIC: BF096042.D

(69) Pentachlorophenol (C)

14.304min (-0.012) 0.00ng

response 23791

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.44
264.00	64.60	64.49
0.00	0.00	0.00