
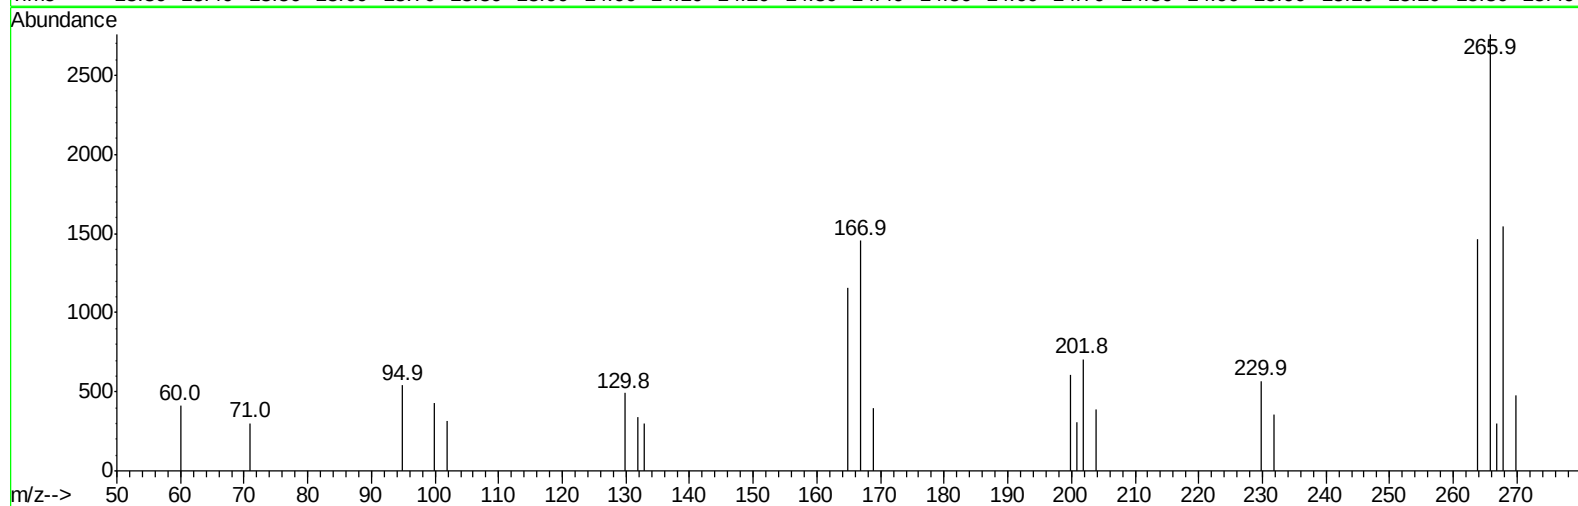


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
Data File : BF096064.D
Acq On : 21 Jun 2017 2:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 07:53:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

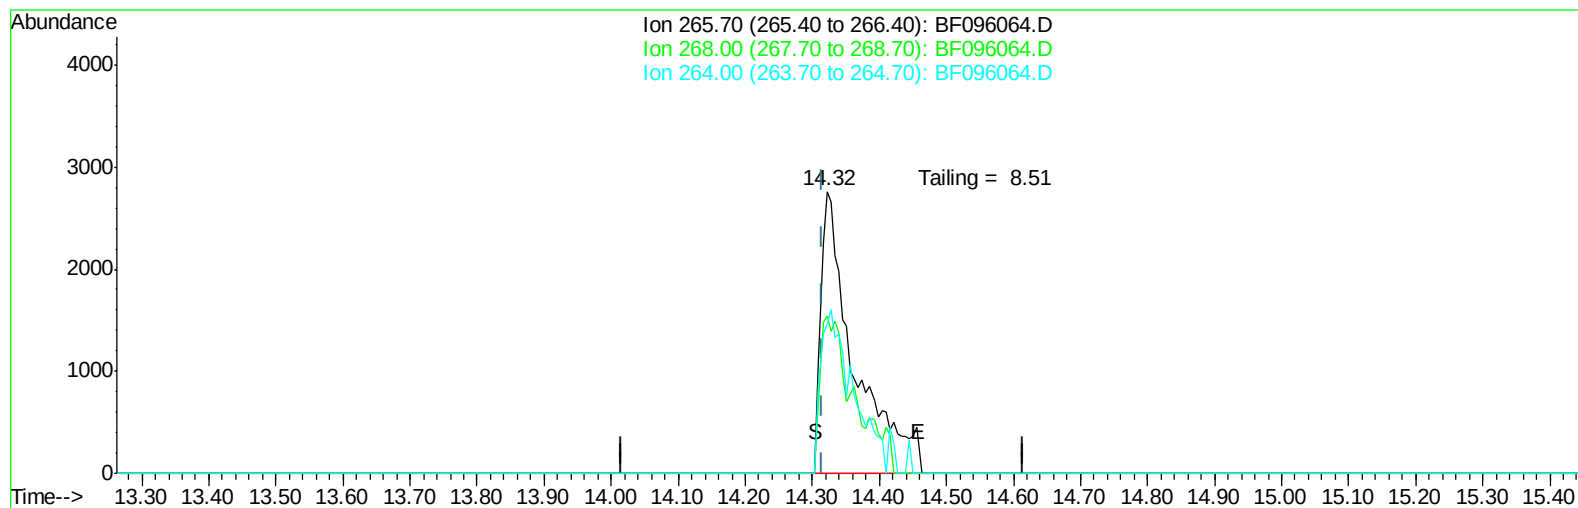

TIC: BF096064.D

(69) Pentachlorophenol (C)



14.321min (+0.006) 0.00ng

response 9186

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.03
264.00	64.60	53.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
 Data File : BF096064.D
 Acq On : 21 Jun 2017 2:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 07:53:18 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 16:05:47 2017
 Response via : Initial Calibration

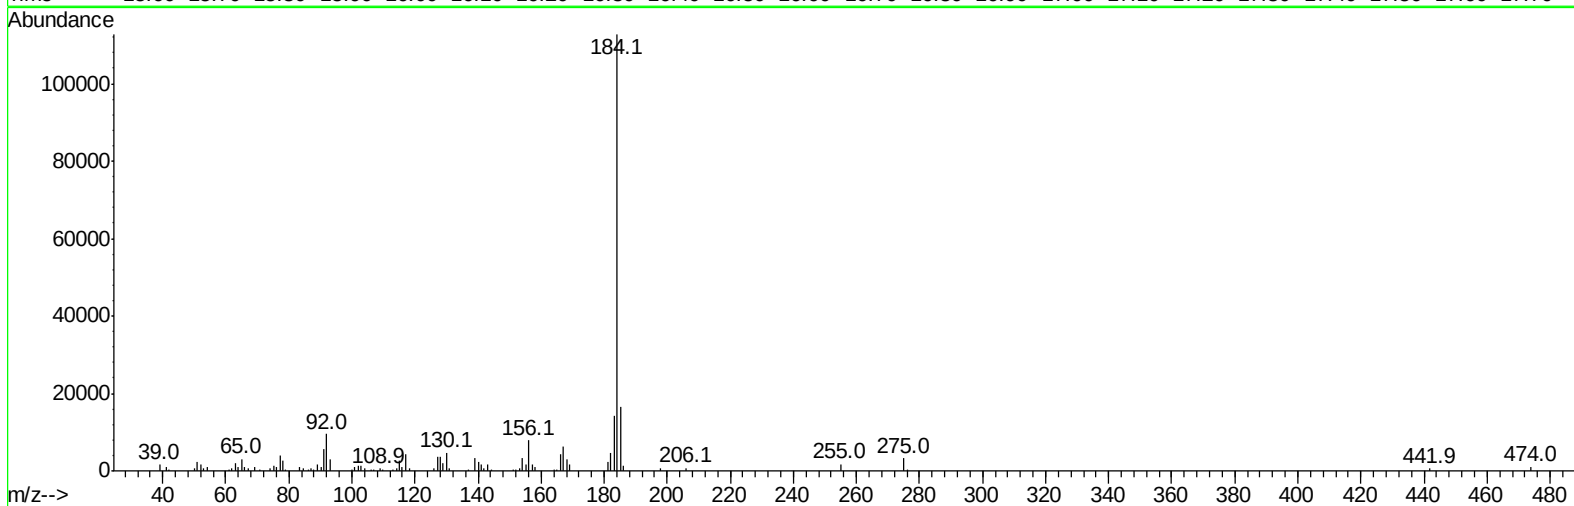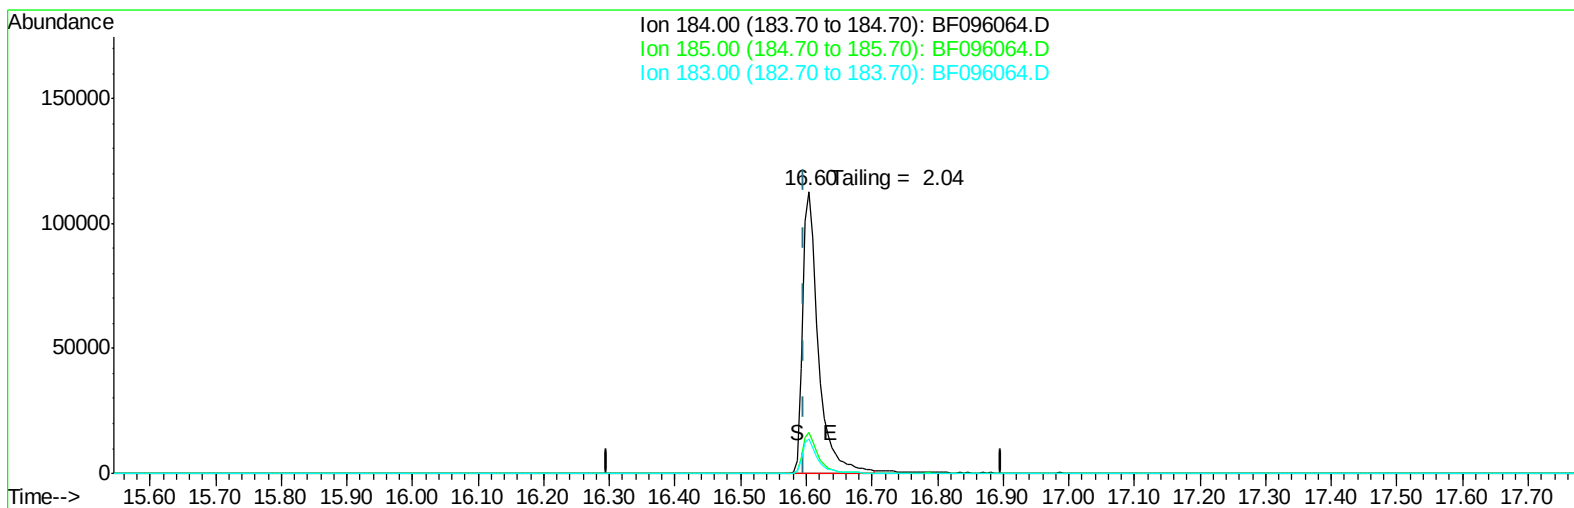

TIC: BF096064.D

(76) Benzidine

16.604min (+0.006) 0.00ng

response 191686

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.75#
183.00	12.20	12.48
0.00	0.00	0.00