

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
 Data File : BF096070.D
 Acq On : 21 Jun 2017 6:45
 Operator : SJ/MA
 Sample : I3722-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 C1-B

Quant Time: Jun 21 07:17:28 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 16:05:47 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.29	152	87855	20.00	ng	0.00
21) Naphthalene-d8	9.32	136	342222	20.00	ng	0.00
38) Acenaphthene-d10	12.15	164	135501	20.00	ng	0.00
63) Phenanthrene-d10	14.54	188	211177	20.00	ng	0.00
75) Chrysene-d12	18.27	240	159757	20.00	ng	0.00
86) Perylene-d12	19.94	264	114106	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	638699	115.84	ng	0.00
7) Phenol-d6	6.87	99	801648	121.45	ng	0.00
23) Nitrobenzene-d5	8.21	82	448213	81.34	ng	-0.01
41) 2,4,6-Tribromophenol	13.45	330	116050	96.80	ng	0.00
44) 2-Fluorobiphenyl	11.10	172	838788	86.14	ng	0.00
78) Terphenyl-d14	16.92	244	569855	88.52	ng	0.00
Target Compounds						
49) Dimethylphthalate	11.80	163	149730	14.55	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
Data File : BF096070.D
Acq On : 21 Jun 2017 6:45
Operator : SJ/MA
Sample : I3722-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C1-B

Quant Time: Jun 21 07:17:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

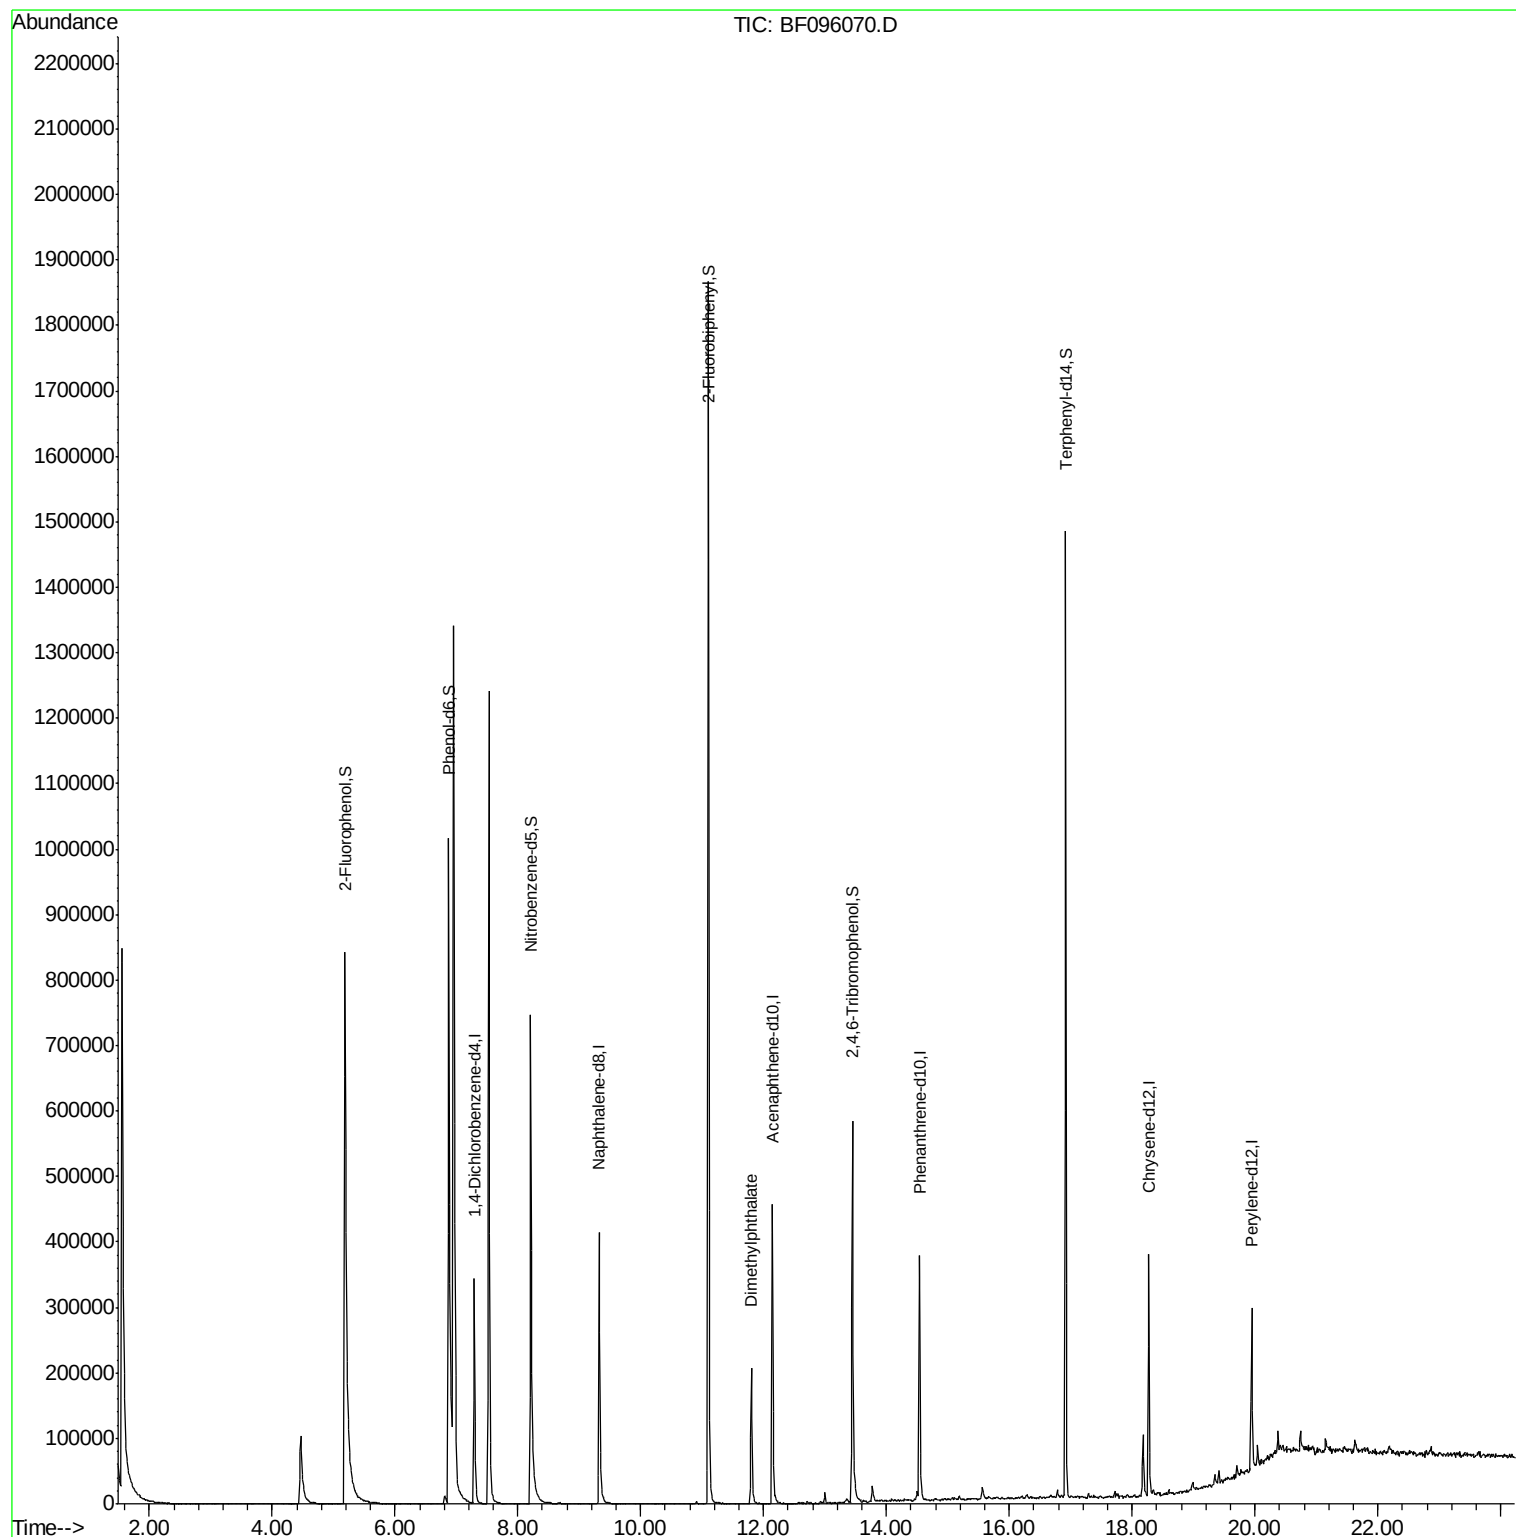

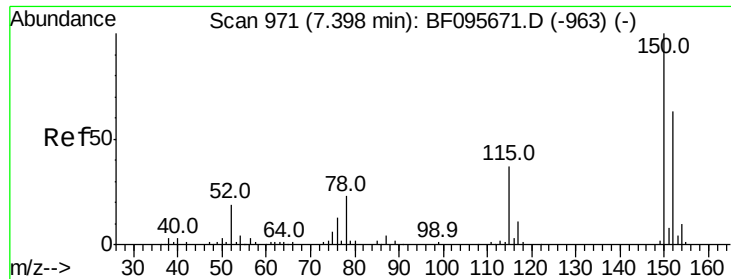


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.29 min Scan# 987
 Delta R.T. 0.00 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Instrument :
 BNA_F
 ClientSampled :
 C1-B

Tot Ion:152 Resp: 87855
 Ion Ratio Lower Upper
 152 100
 150 152.5 126.2 189.2
 115 57.3 52.2 78.2

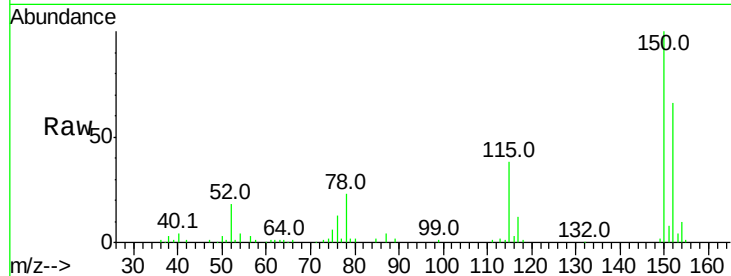


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

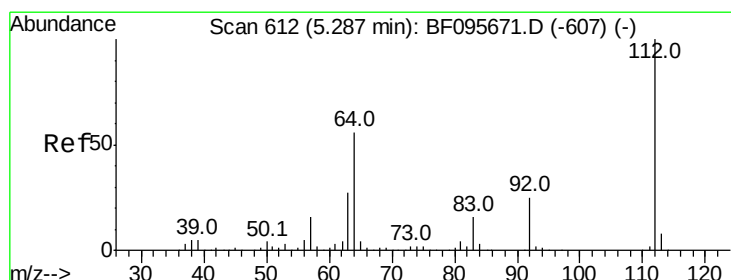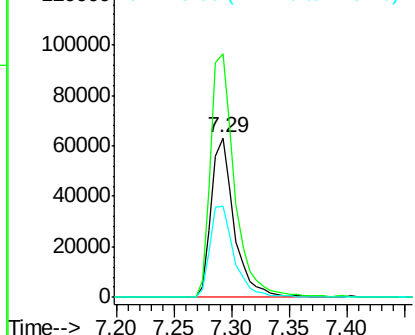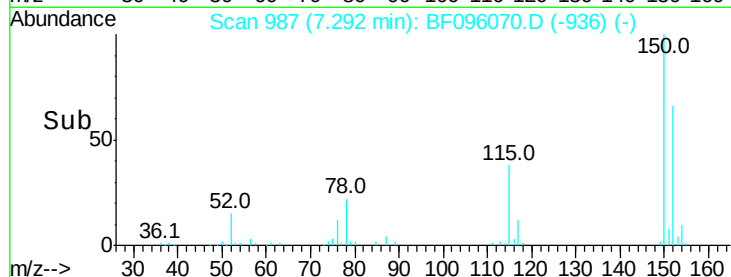



#5


2-Fluorophenol
 Concen: 115.84 ng
 RT: 5.19 min Scan# 629
 Delta R.T. 0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Tgt Ion:112 Resp: 638699
 Ion Ratio Lower Upper
 112 100
 64 55.3 46.0 69.0
 63 26.3 23.4 35.0

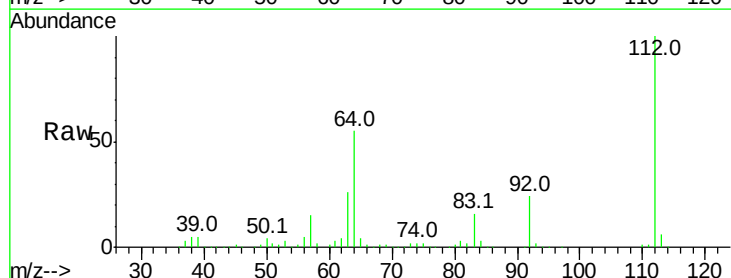

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

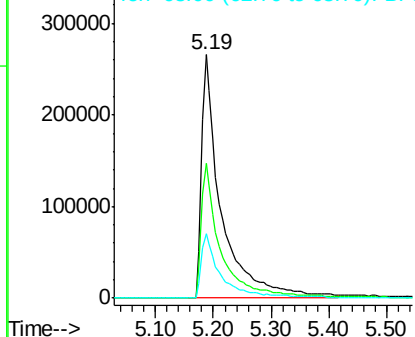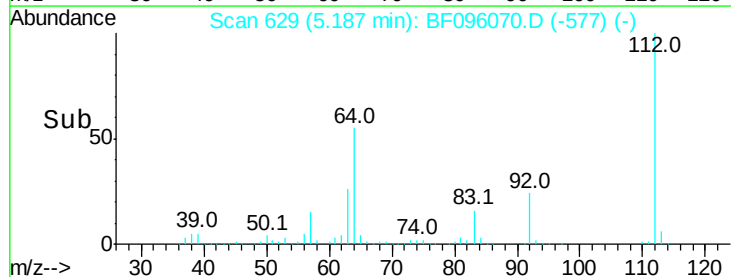

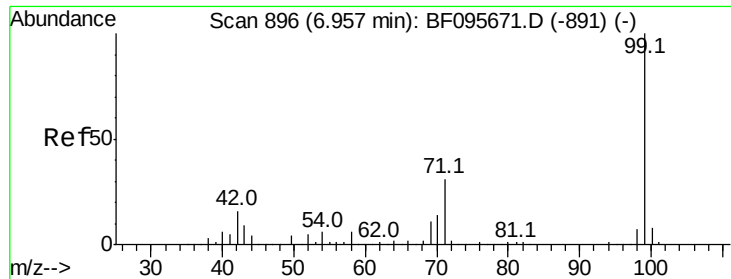

#7

Phenol-d6

Concen: 121.45 ng

RT: 6.87 min Scan# 916

Delta R.T. 0.00 min

Lab File: BF096070.D

Acq: 21 Jun 2017 6:45

Instrument :

BNA_F

ClientSampled :

C1-B


Tot Ion: 99 Resp: 801648

Ion Ratio Lower Upper

99 100

42 15.9 13.5 20.3




71 31.6 24.5 36.7

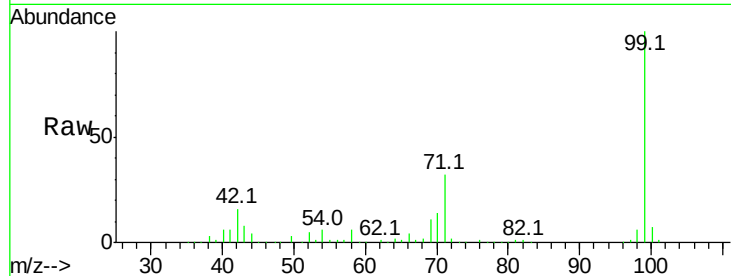

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

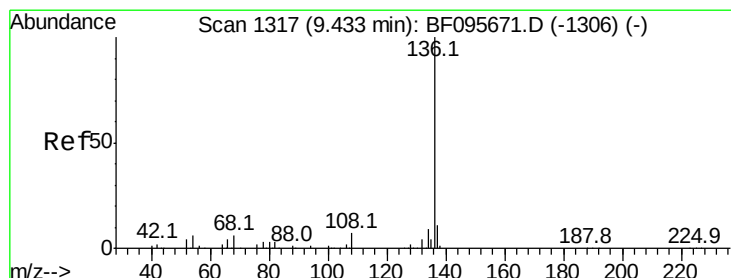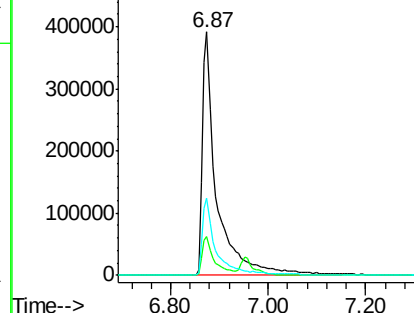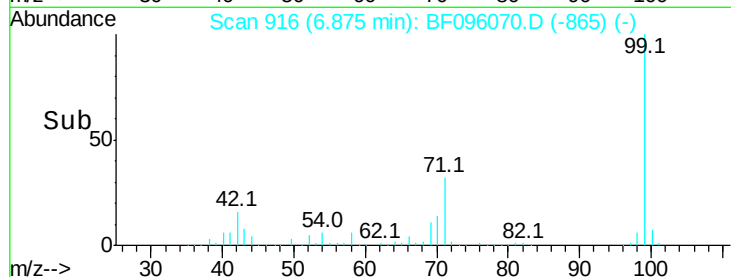

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.32 min Scan# 1332

Delta R.T. -0.01 min

Lab File: BF096070.D

Acq: 21 Jun 2017 6:45

Tgt Ion:136 Resp: 342222


Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 6.9 4.9 7.3

68 6.5 4.1 6.1#


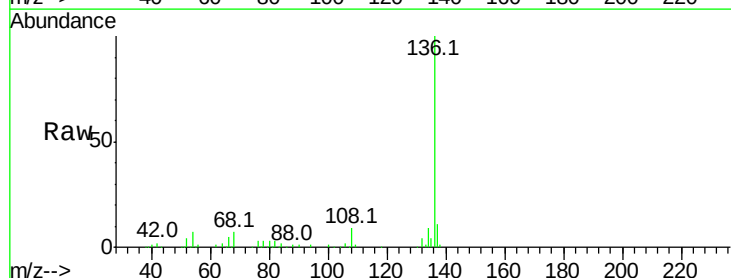



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

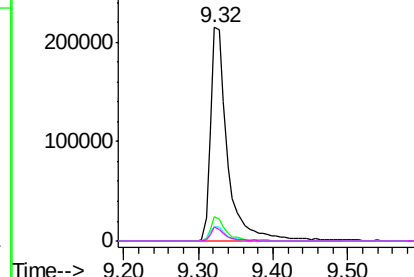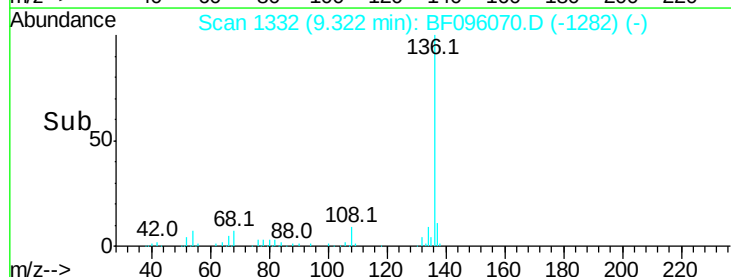


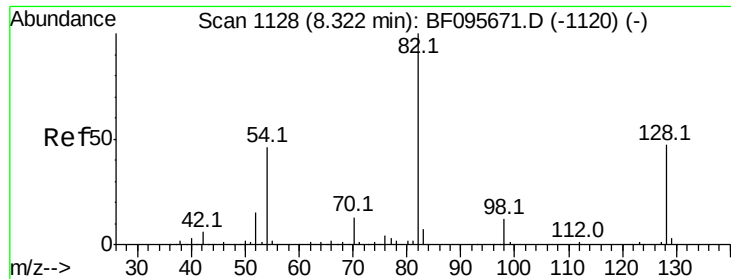




#23
 Nitrobenzene-d5
 Concen: 81.34 ng
 RT: 8.21 min Scan# 1143
 Delta R.T. -0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Instrument :
 BNA_F
 ClientSampleId :
 C1-B

Tot Ion: 82 Resp: 448213
 Ion Ratio Lower Upper
 82 100
 128 44.0 34.0 51.0
 54 46.3 42.2 63.2

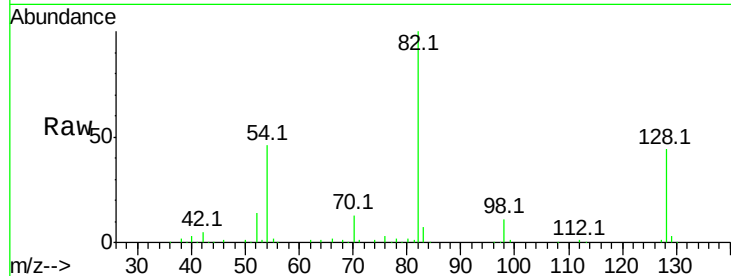


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

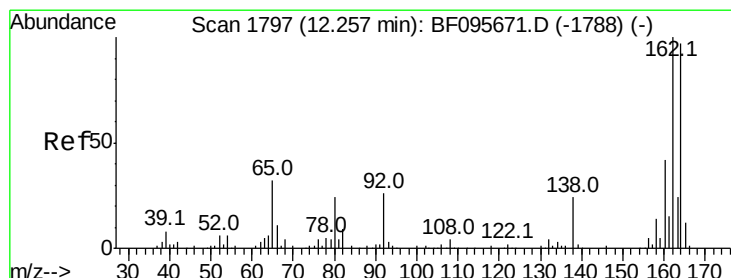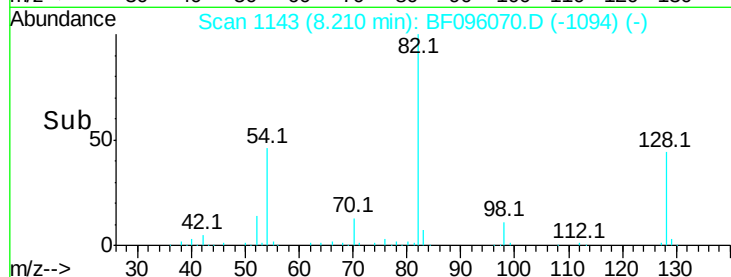
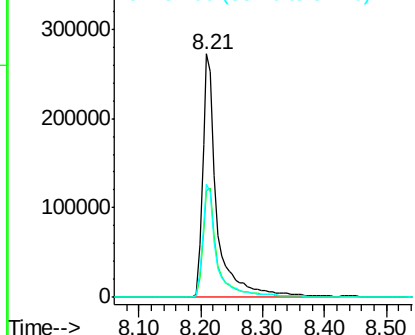



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.15 min Scan# 1812
 Delta R.T. -0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Tgt Ion:164 Resp: 135501
 Ion Ratio Lower Upper
 164 100
 162 101.6 82.6 123.8
 160 44.7 36.2 54.2

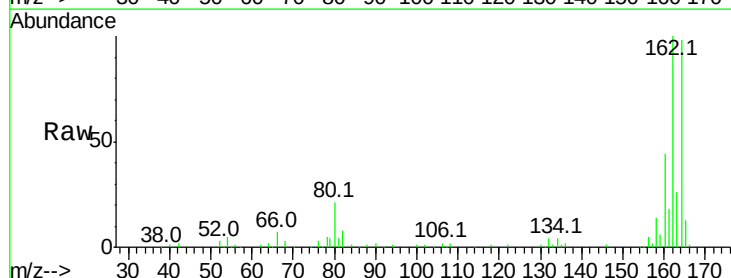

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

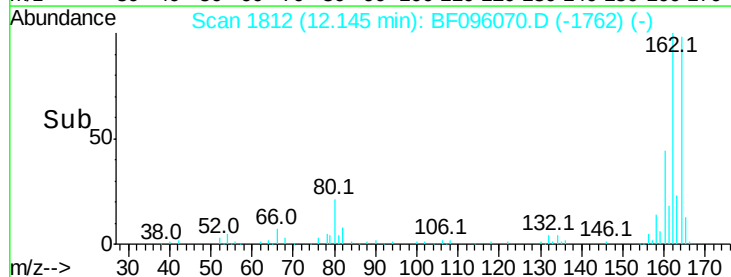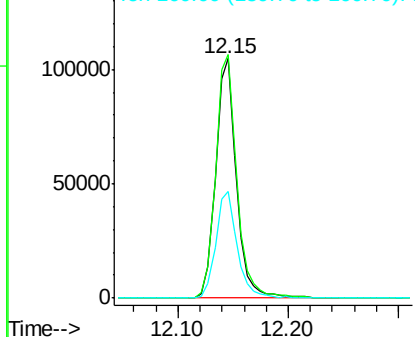


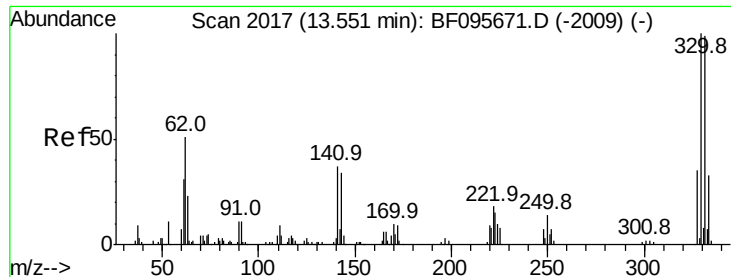




#41
 2,4,6-Tribromophenol
 Concen: 96.80 ng
 RT: 13.45 min Scan# 2033
 Delta R.T. -0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Instrument :
 BNA_F
 ClientSampled :
 C1-B

Tot Ion:330 Resp: 116050
 Ion Ratio Lower Upper
 330 100
 332 94.6 76.6 115.0
 141 37.9 31.4 47.2

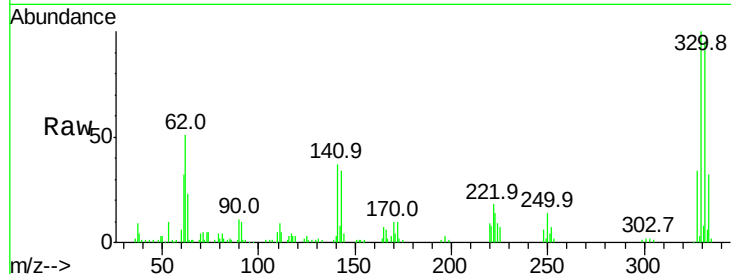


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

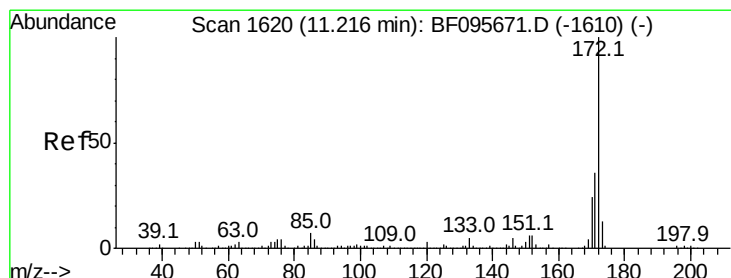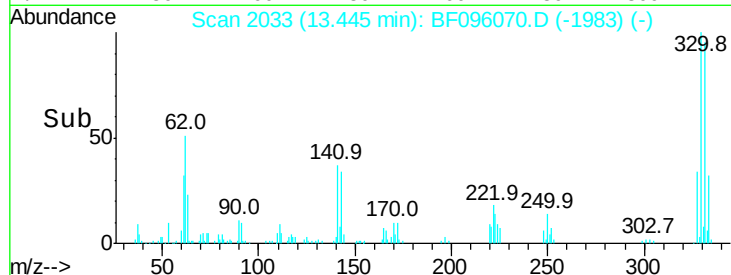
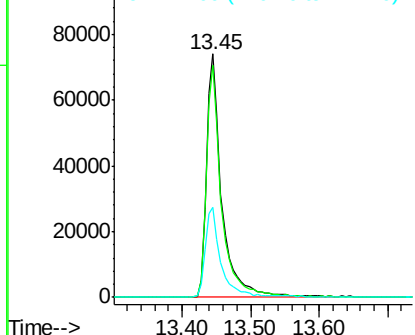



#44
 2-Fluorobiphenyl
 Concen: 86.14 ng
 RT: 11.10 min Scan# 1635
 Delta R.T. -0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Tgt Ion:172 Resp: 838788
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.6 44.4
 170 23.6 19.8 29.8

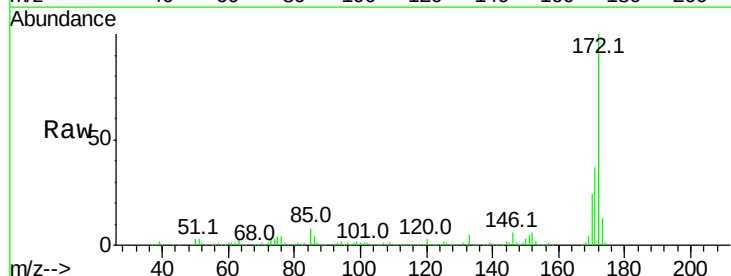

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

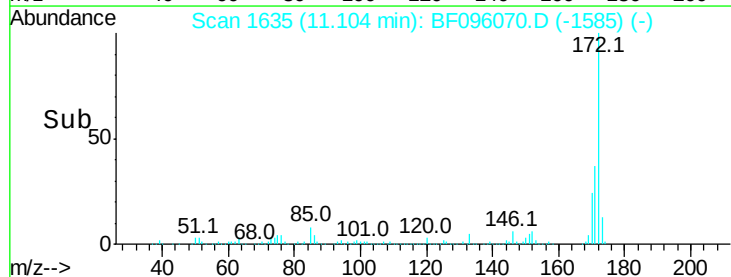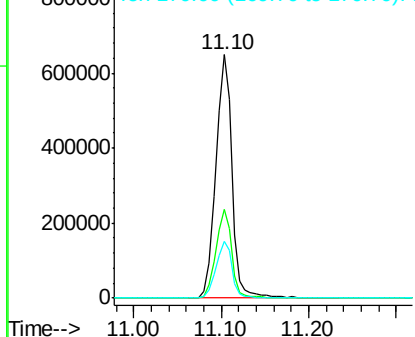

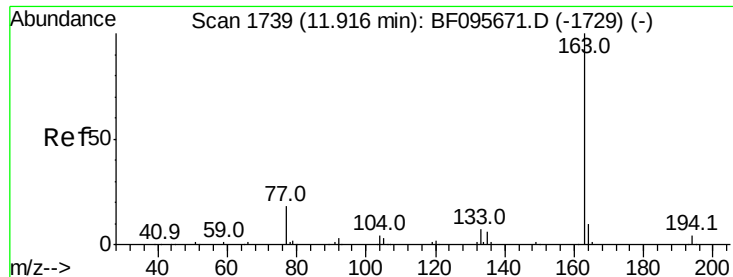

#49

Dimethylphthalate

Concen: 14.55 ng

RT: 11.80 min Scan# 1754

Delta R.T. -0.02 min

Lab File: BF096070.D

Acq: 21 Jun 2017 6:45

Instrument :

BNA_F

ClientSampleId :

C1-B


Tot Ion:163 Resp: 149730

Ion Ratio Lower Upper

163 100

194 3.0 2.6 4.0




164 9.7 8.4 12.6

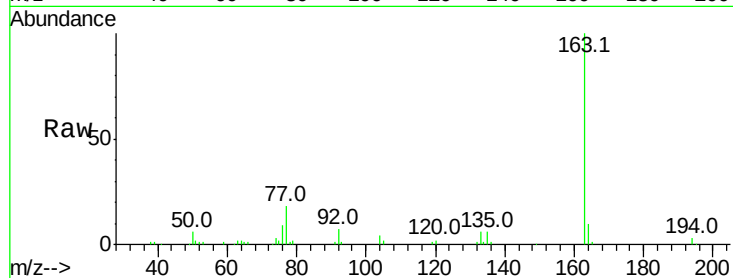

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

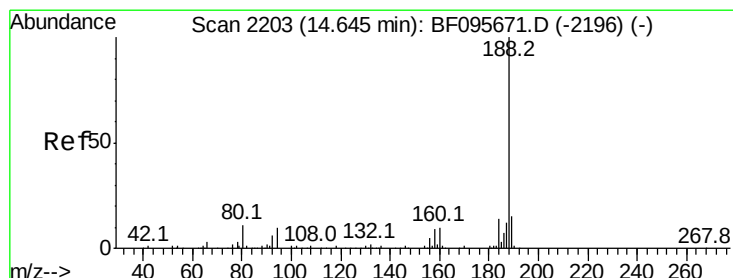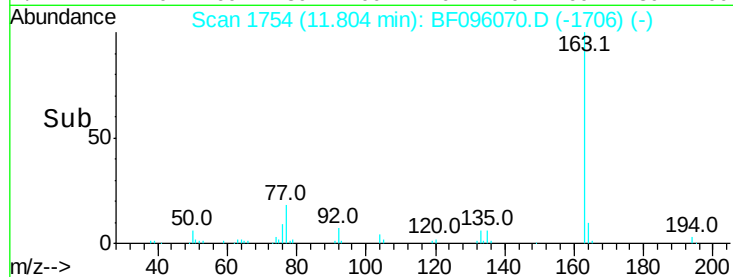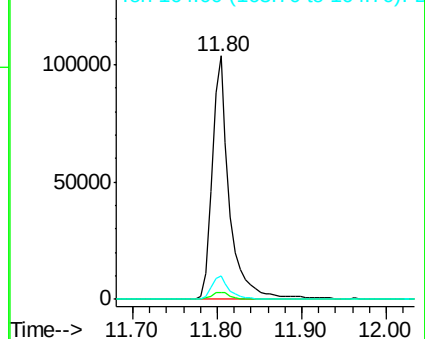

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.54 min Scan# 2219

Delta R.T. 0.00 min

Lab File: BF096070.D

Acq: 21 Jun 2017 6:45


Tgt Ion:188 Resp: 211177

Ion Ratio Lower Upper

188 100

94 10.8 9.4 14.2



80 11.5 10.2 15.2

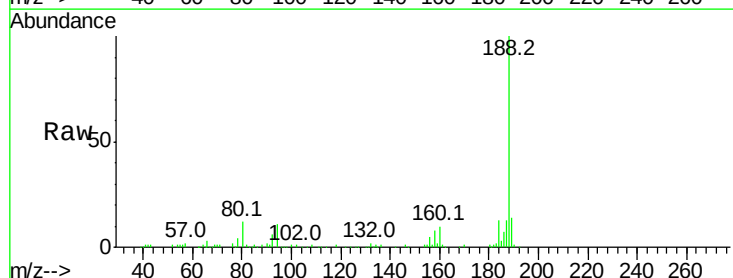


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



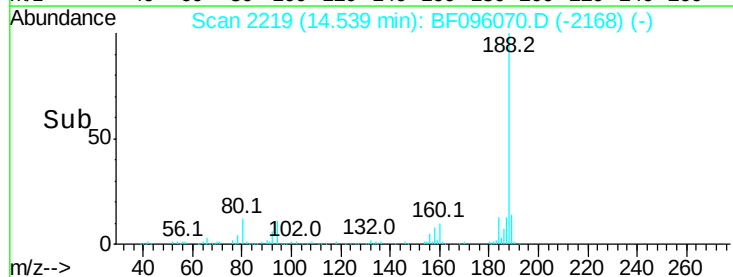
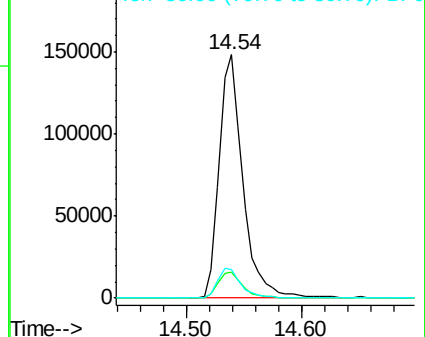


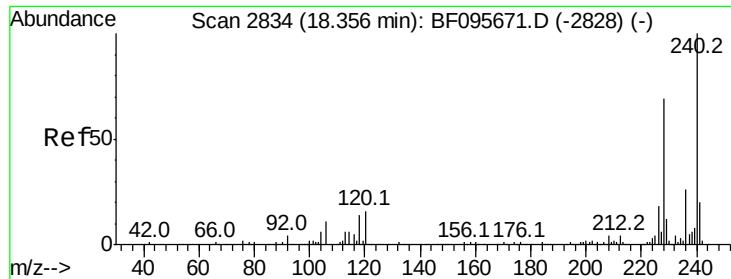

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.27 min Scan# 2853
 Delta R.T. -0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45




Instrument :
 BNA_F
 ClientSampleId :
 C1-B


Tot Ion:240 Resp: 159757
 Ion Ratio Lower Upper
 240 100
 120 15.4 5.8 8.8#
 236 24.7 20.5 30.7

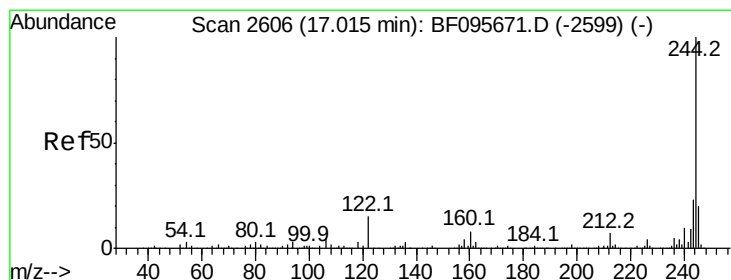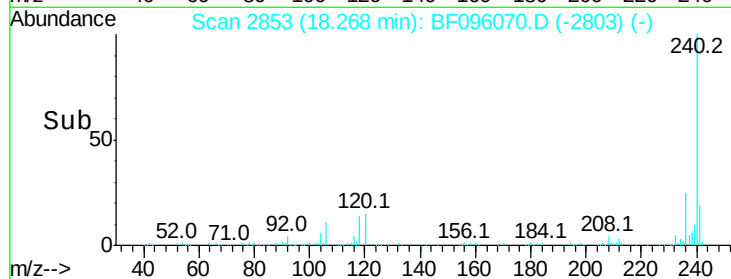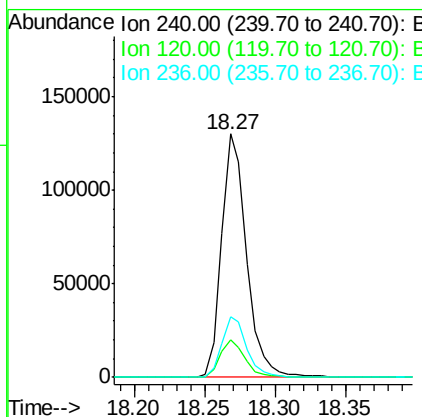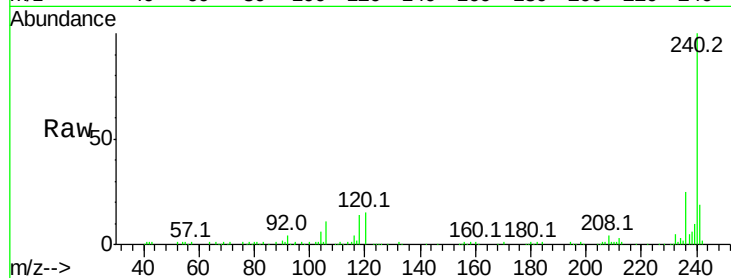

#78
 Terphenyl-d14
 Concen: 88.52 ng
 RT: 16.92 min Scan# 2624
 Delta R.T. -0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Tgt Ion:244 Resp: 569855
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.0 9.0
 122 14.6 10.3 15.5

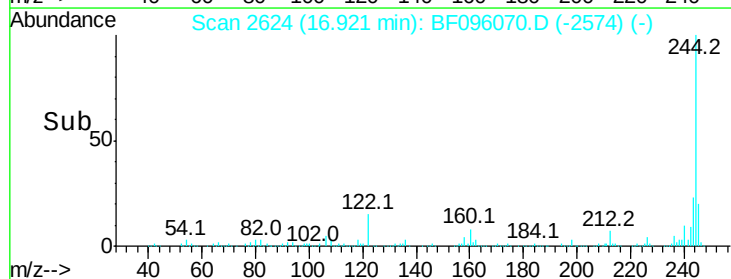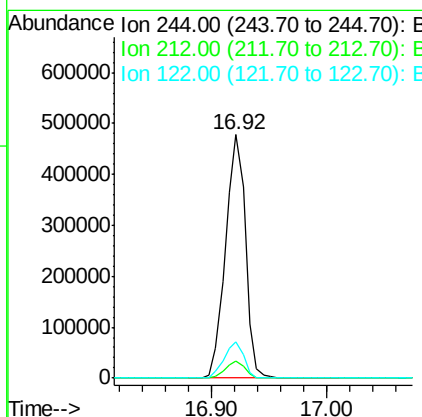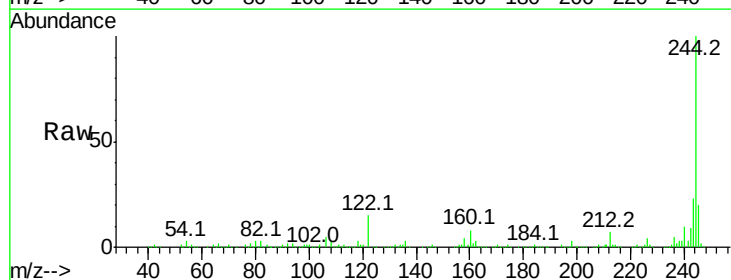


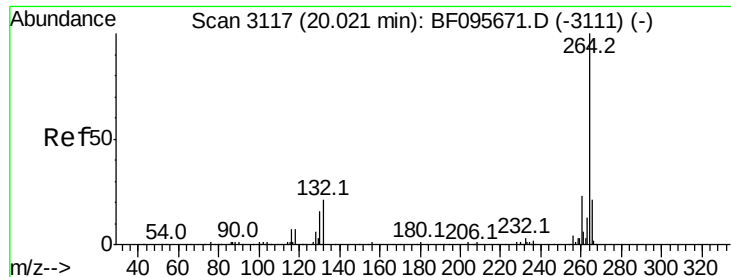

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 19.94 min Scan# 3138
 Delta R.T. 0.01 min
 Lab File: BF096070.D
 Acq: 21 Jun 2017 6:45

Instrument :
 BNA_F
 ClientSampleId :
 C1-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.2	19.5	29.3
265	21.3	17.2	25.8

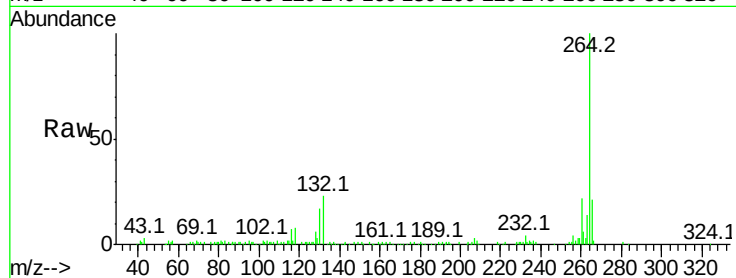

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

