

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062017\
 Data File : BF096049.D
 Acq On : 20 Jun 2017 17:31
 Operator : SJ/MA
 Sample : I3697-01 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-SF-02-001-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.551	9	11	66	rVB	1572620	3311253	100.00%	42.065%
2	4.439	499	502	512	rBV	14065	34435	1.04%	0.437%
3	5.257	637	641	653	rBV3	14230	52513	1.59%	0.667%
4	6.922	920	924	931	rBV2	36383	94837	2.86%	1.205%
5	6.980	931	934	951	rVB	73919	198483	5.99%	2.521%
6	7.286	982	986	998	rBV	290314	402670	12.16%	5.115%
7	7.533	1023	1028	1042	rVB	87594	138492	4.18%	1.759%
8	8.233	1144	1147	1161	rBV	31102	84602	2.55%	1.075%
9	9.321	1328	1332	1346	rBV	392762	553721	16.72%	7.034%
10	11.104	1631	1635	1645	rBV	176505	221269	6.68%	2.811%
11	12.145	1807	1812	1818	rBV2	410556	529090	15.98%	6.721%
12	14.539	2215	2219	2223	rVV	340985	445230	13.45%	5.656%
13	14.574	2223	2225	2234	rVB	79271	109100	3.29%	1.386%
14	14.674	2238	2242	2252	rVB	28113	42410	1.28%	0.539%
15	15.221	2332	2335	2342	rVB	33769	41964	1.27%	0.533%
16	16.368	2523	2530	2536	rVB	126456	172829	5.22%	2.196%
17	16.668	2577	2581	2589	rBV	132253	173105	5.23%	2.199%
18	16.915	2620	2623	2630	rVB	149569	170326	5.14%	2.164%
19	18.268	2848	2853	2857	rBV2	409654	524053	15.83%	6.657%
20	18.303	2857	2859	2872	rVB3	50400	96344	2.91%	1.224%
21	18.597	2906	2909	2919	rVB5	27855	46337	1.40%	0.589%
22	19.544	3067	3070	3076	rBV	52831	95835	2.89%	1.217%
23	19.938	3134	3137	3146	rVB	253389	332864	10.05%	4.229%


Sum of corrected areas: 7871762

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062017\
Data File : BF096049.D
Acq On : 20 Jun 2017 17:31
Operator : SJ/MA
Sample : I3697-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-02-001-A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

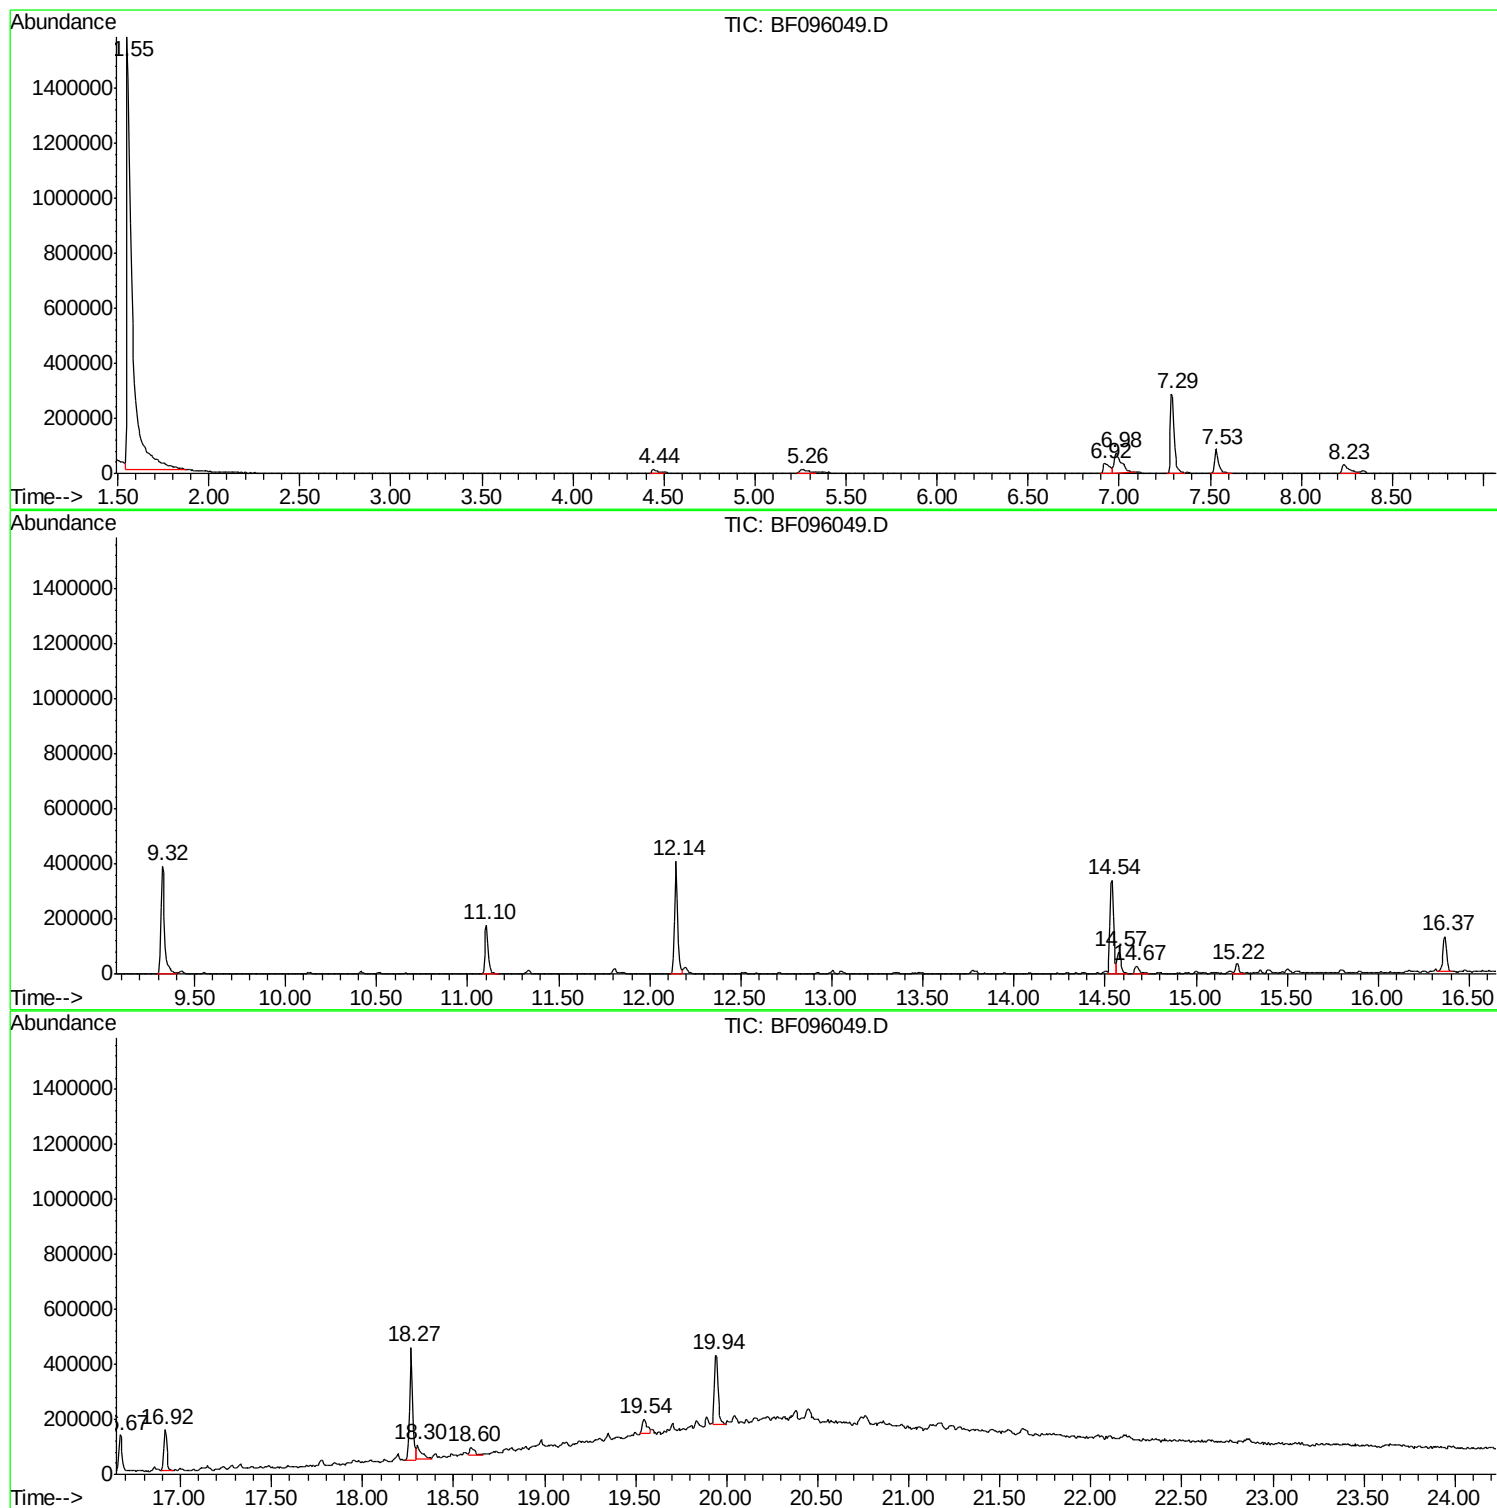

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062017\
Data File : BF096049.D
Acq On : 20 Jun 2017 17:31
Operator : SJ/MA
Sample : I3697-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-02-001-A










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.98 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.98	9.86 ng	198483	1,4-Dichlorobenzene-d4	7.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	43
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	43
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	43
4		Xenon	132	Xe	007440-63-3	38
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	25

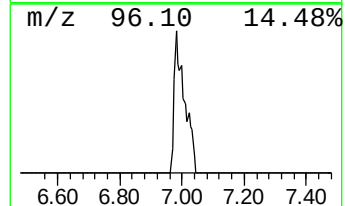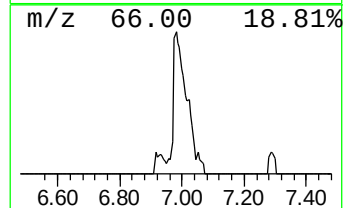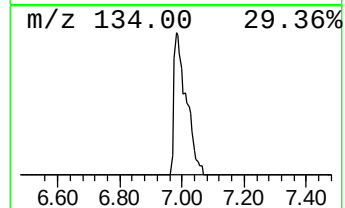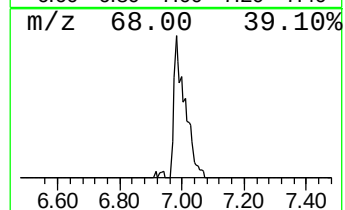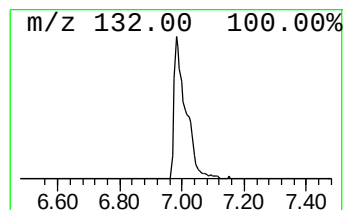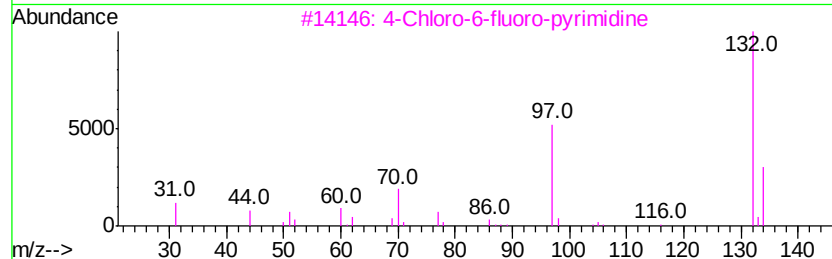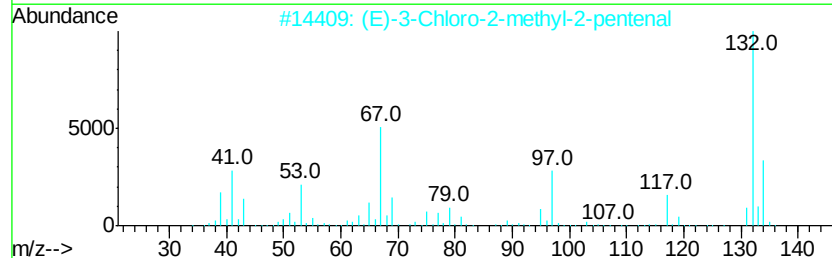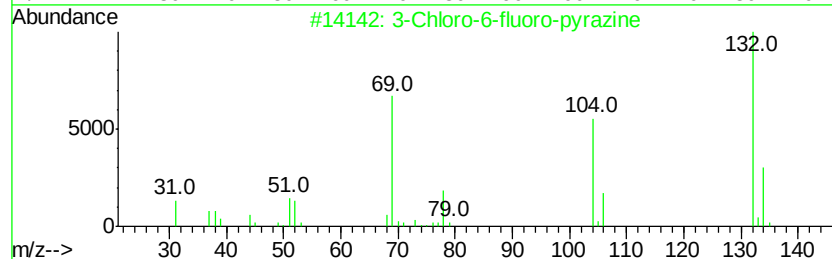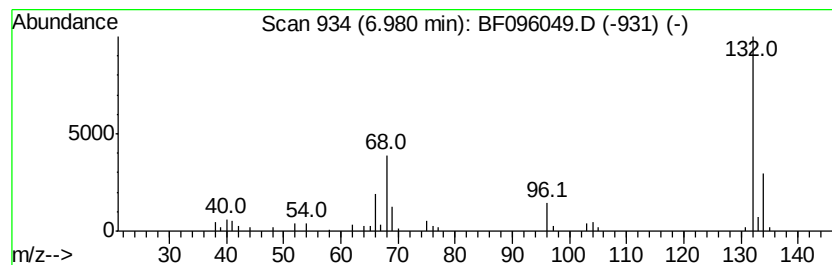

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062017\
Data File : BF096049.D
Acq On : 20 Jun 2017 17:31
Operator : SJ/MA
Sample : I3697-01 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-02-001-A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.98	6.98	9.9	ng	198483	1	7.29	402670	20.0